

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030891.D
 Acq On : 26 Apr 2023 19:59
 Operator : SY/MD
 Sample : 02475-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030891.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	90	rBV	89797	97783	12.65%	1.577%
2	1.539	148	155	169	rVB	88498	106981	13.84%	1.726%
3	2.027	305	307	308	rBV2	1695	598	0.08%	0.010%
4	2.066	310	319	336	rVB	179936	266030	34.41%	4.291%
5	2.387	413	419	422	rVB7	903	932	0.12%	0.015%
6	2.455	436	440	445	rBV7	1309	1286	0.17%	0.021%
7	2.632	493	495	497	rBV3	1574	803	0.10%	0.013%
8	2.770	535	538	541	rBV4	913	827	0.11%	0.013%
9	2.799	545	547	548	rBV	1362	591	0.08%	0.010%
10	2.834	555	558	563	rBV8	1392	1179	0.15%	0.019%
11	2.860	563	566	569	rBV5	1107	923	0.12%	0.015%
12	2.966	596	599	601	rVV3	1431	861	0.11%	0.014%
13	2.979	601	603	607	rVB5	1277	842	0.11%	0.014%
14	3.002	607	610	611	rBV2	1031	620	0.08%	0.010%
15	3.207	671	674	677	rVB5	1260	731	0.09%	0.012%
16	3.223	677	679	680	rBV	1770	825	0.11%	0.013%
17	3.320	705	709	713	rBV5	2264	1891	0.24%	0.031%
18	3.609	795	799	801	rBV3	974	678	0.09%	0.011%
19	3.703	825	828	831	rBV5	1420	791	0.10%	0.013%
20	3.767	841	848	849	rBV5	1126	1303	0.17%	0.021%
21	3.805	851	860	886	rVV	44904	136232	17.62%	2.198%
22	4.108	952	954	956	rBV2	1364	708	0.09%	0.011%
23	4.259	984	1001	1022	rBV2	126334	324138	41.93%	5.229%
24	4.519	1080	1082	1086	rVB5	1192	686	0.09%	0.011%
25	4.706	1133	1140	1143	rBV7	1553	1654	0.21%	0.027%
26	4.860	1186	1188	1191	rBV4	1331	756	0.10%	0.012%
27	4.879	1191	1194	1195	rBV3	903	604	0.08%	0.010%
28	4.966	1202	1221	1247	rBV2	286520	773103	100.00%	12.471%
29	5.320	1329	1331	1336	rVB5	1466	1036	0.13%	0.017%
30	5.542	1388	1400	1423	rBV	263216	551513	71.34%	8.896%
31	5.995	1528	1541	1564	rBV	172597	364341	47.13%	5.877%
32	6.223	1608	1612	1615	rVB6	1844	1427	0.18%	0.023%
33	6.288	1628	1632	1633	rBV3	1349	958	0.12%	0.015%
34	6.436	1674	1678	1681	rBV7	1157	894	0.12%	0.014%
35	6.767	1779	1781	1783	rBV3	1195	688	0.09%	0.011%
36	6.921	1814	1829	1844	rBV	88166	170160	22.01%	2.745%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030891.D
 Acq On : 26 Apr 2023 19:59
 Operator : SY/MD
 Sample : 02475-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.252	1921	1932	1955	rBV	324833	583909	75.53%	9.419%
38	7.561	2015	2028	2045	rBV	65696	122516	15.85%	1.976%
39	7.722	2074	2078	2082	rVB7	1129	994	0.13%	0.016%
40	7.850	2116	2118	2121	rBV3	1146	715	0.09%	0.012%
41	7.876	2122	2126	2128	rVV4	1339	922	0.12%	0.015%
42	7.960	2149	2152	2155	rBV3	1034	698	0.09%	0.011%
43	8.034	2166	2175	2207	rBV	145684	317899	41.12%	5.128%
44	8.442	2300	2302	2305	rVB4	1516	642	0.08%	0.010%
45	8.689	2377	2379	2383	rVB5	1394	680	0.09%	0.011%
46	8.709	2383	2385	2394	rBV8	960	1024	0.13%	0.017%
47	8.792	2400	2411	2433	rBV	404707	687506	88.93%	11.090%
48	9.085	2500	2502	2503	rBV2	1502	663	0.09%	0.011%
49	9.143	2517	2520	2523	rBV5	1282	742	0.10%	0.012%
50	9.178	2528	2531	2537	rVB6	1531	1674	0.22%	0.027%
51	9.207	2537	2540	2542	rBV	1013	725	0.09%	0.012%
52	9.246	2547	2552	2554	rBV5	1316	1141	0.15%	0.018%
53	9.352	2581	2585	2589	rVB7	1425	1209	0.16%	0.020%
54	9.371	2589	2591	2595	rBV4	1041	861	0.11%	0.014%
55	9.406	2599	2602	2606	rVB5	971	721	0.09%	0.012%
56	9.474	2619	2623	2625	rBV4	1423	1321	0.17%	0.021%
57	9.542	2639	2644	2645	rBV3	1590	1126	0.15%	0.018%
58	10.001	2785	2787	2790	rBV3	1382	664	0.09%	0.011%
59	10.159	2825	2836	2853	rBV	240344	386453	49.99%	6.234%
60	10.313	2877	2884	2887	rBV9	1854	2757	0.36%	0.044%
61	10.410	2911	2914	2920	rBV5	1162	1016	0.13%	0.016%
62	10.654	2987	2990	2992	rBV3	1144	619	0.08%	0.010%
63	10.722	3009	3011	3014	rVB3	1717	819	0.11%	0.013%
64	10.738	3014	3016	3021	rBV5	1342	1194	0.15%	0.019%
65	10.789	3028	3032	3033	rBV5	1577	721	0.09%	0.012%
66	10.824	3041	3043	3046	rVB4	1345	717	0.09%	0.012%
67	10.992	3090	3095	3096	rBV4	1197	878	0.11%	0.014%
68	11.049	3110	3113	3116	rBV4	1377	817	0.11%	0.013%
69	11.146	3141	3143	3145	rVB3	1397	619	0.08%	0.010%
70	11.194	3145	3158	3183	rBV	408902	659812	85.35%	10.643%
71	11.361	3207	3210	3212	rBV3	1485	879	0.11%	0.014%
72	11.426	3227	3230	3232	rBV3	1325	854	0.11%	0.014%
73	11.567	3263	3274	3291	rBV	355174	570268	73.76%	9.199%
74	11.853	3360	3363	3364	rBV3	1128	625	0.08%	0.010%
75	12.056	3423	3426	3429	rBV4	1474	931	0.12%	0.015%
76	12.191	3464	3468	3469	rBV3	1492	1001	0.13%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042623\
 Data File : VW030891.D
 Acq On : 26 Apr 2023 19:59
 Operator : SY/MD
 Sample : 02475-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.313	3501	3506	3508	rBV7	1174	1087	0.14%	0.018%
78	12.458	3548	3551	3553	rBV3	933	671	0.09%	0.011%
79	12.548	3575	3579	3580	rBV3	1428	833	0.11%	0.013%
80	12.654	3611	3612	3616	rVV3	951	614	0.08%	0.010%
81	12.734	3635	3637	3639	rBV3	1410	838	0.11%	0.014%
82	12.815	3659	3662	3666	rBV6	1247	1095	0.14%	0.018%
83	12.959	3704	3707	3712	rVB5	1547	1395	0.18%	0.023%
84	12.985	3712	3715	3717	rBV4	1143	869	0.11%	0.014%
85	13.146	3760	3765	3768	rBV7	1850	2060	0.27%	0.033%
86	13.207	3780	3784	3786	rBV5	1717	1105	0.14%	0.018%
87	13.300	3811	3813	3815	rVV3	1269	667	0.09%	0.011%
88	13.355	3826	3830	3833	rBV6	1326	1139	0.15%	0.018%
89	13.461	3861	3863	3866	rBV3	1304	951	0.12%	0.015%
90	13.512	3874	3879	3880	rBV4	1561	833	0.11%	0.013%
91	13.548	3888	3890	3892	rBV3	1194	593	0.08%	0.010%
92	13.619	3909	3912	3916	rBV6	1668	1364	0.18%	0.022%
93	13.773	3956	3960	3964	rBV7	1661	1356	0.18%	0.022%
94	14.223	4097	4100	4106	rVB5	1337	1236	0.16%	0.020%
95	14.252	4106	4109	4111	rBV3	1113	621	0.08%	0.010%
96	14.442	4165	4168	4169	rBV3	1191	685	0.09%	0.011%
97	14.757	4264	4266	4269	rVV4	1428	768	0.10%	0.012%
98	14.827	4284	4288	4291	rBV5	2096	2041	0.26%	0.033%
99	14.975	4331	4334	4338	rBV5	1326	944	0.12%	0.015%
100	15.387	4460	4462	4464	rBV3	1463	925	0.12%	0.015%

Sum of corrected areas: 6199395




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030891.D
Acq On : 26 Apr 2023 19:59
Operator : SY/MD
Sample : 02475-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

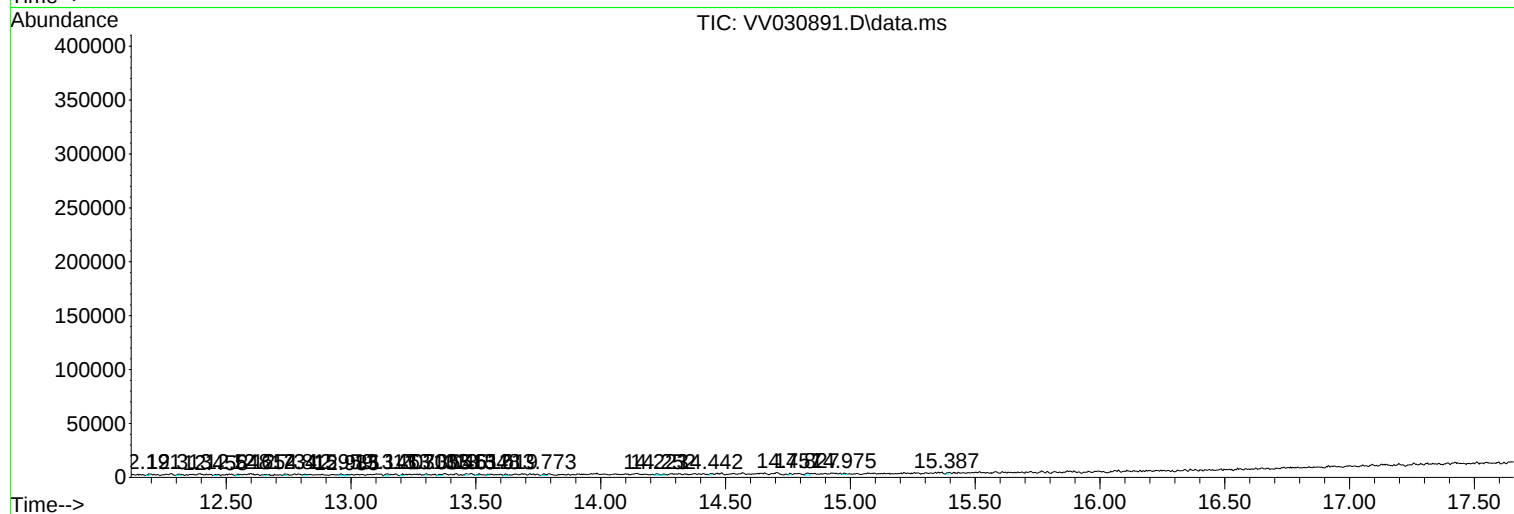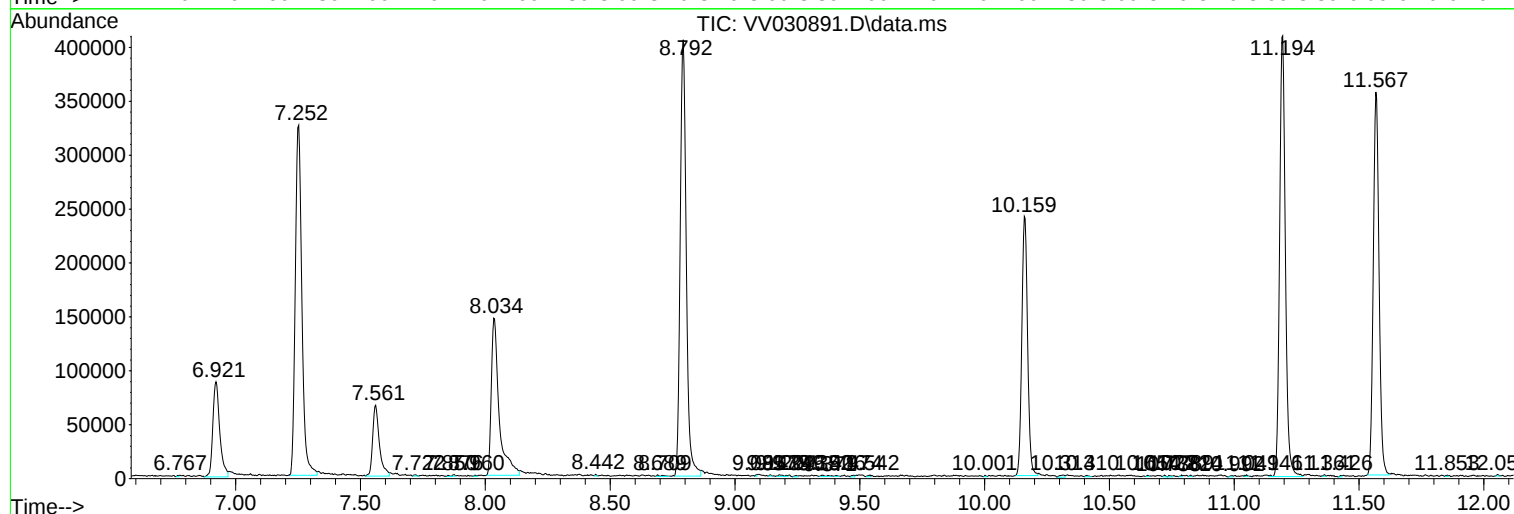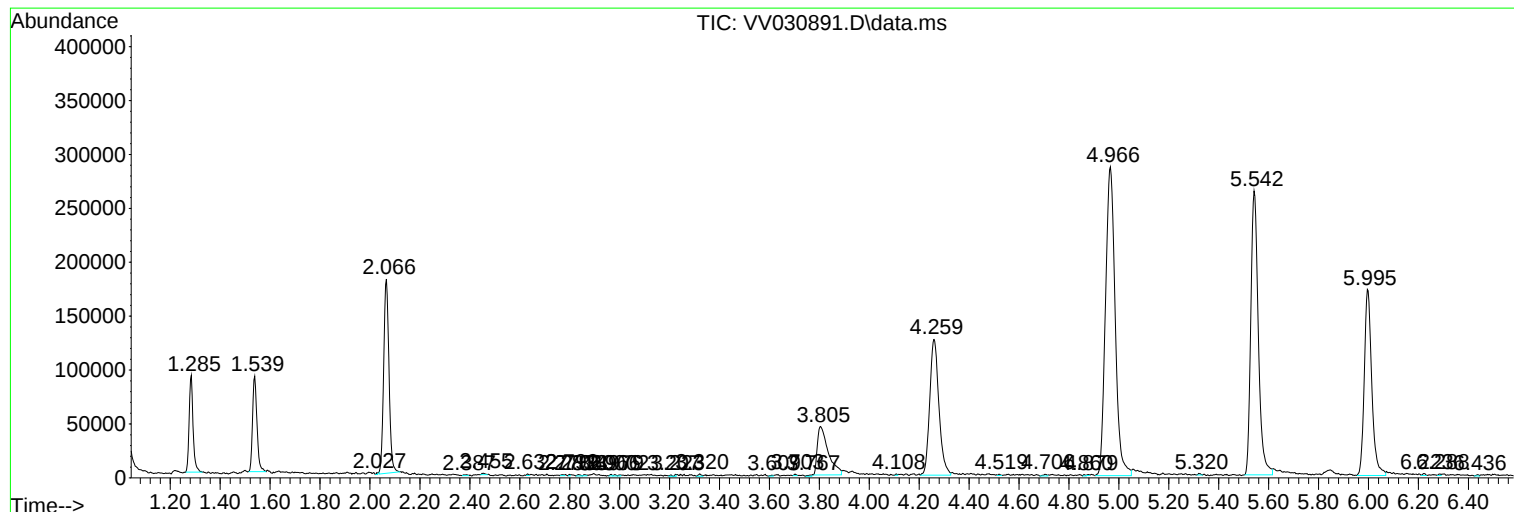

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030891.D
Acq On : 26 Apr 2023 19:59
Operator : SY/MD
Sample : 02475-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030891.D
Acq On : 26 Apr 2023 19:59
Operator : SY/MD
Sample : 02475-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------