

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
 Data File : VV030892.D
 Acq On : 26 Apr 2023 20:23
 Operator : SY/MD
 Sample : 02474-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030892.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	91	rBV	81634	92636	12.41%	1.551%
2	1.539	148	155	169	rVB	81156	98500	13.20%	1.649%
3	2.066	310	319	337	rVB	173853	257745	34.53%	4.314%
4	2.616	486	490	491	rBV3	1217	817	0.11%	0.014%
5	2.664	503	505	510	rVB5	1374	1027	0.14%	0.017%
6	2.786	541	543	546	rVB3	1491	799	0.11%	0.013%
7	2.809	546	550	551	rBV3	1192	828	0.11%	0.014%
8	2.841	558	560	561	rBV2	553	258	0.03%	0.004%
9	3.082	632	635	641	rBV6	1069	900	0.12%	0.015%
10	3.233	677	682	683	rBV4	1004	847	0.11%	0.014%
11	3.278	694	696	699	rBV3	1549	979	0.13%	0.016%
12	3.291	699	700	702	rBV2	670	272	0.04%	0.005%
13	3.355	719	720	721	rBV	798	306	0.04%	0.005%
14	3.442	744	747	749	rBV3	967	749	0.10%	0.013%
15	3.494	759	763	765	rBV4	1116	888	0.12%	0.015%
16	3.619	800	802	807	rVB5	1731	1122	0.15%	0.019%
17	3.687	820	823	825	rBV4	1502	1136	0.15%	0.019%
18	3.809	851	861	890	rBV2	42860	131017	17.55%	2.193%
19	4.259	988	1001	1023	rVB2	121674	303187	40.62%	5.075%
20	4.590	1102	1104	1106	rBV3	984	495	0.07%	0.008%
21	4.722	1142	1145	1147	rBV4	878	449	0.06%	0.008%
22	4.966	1205	1221	1246	rBV3	277538	746483	100.00%	12.495%
23	5.256	1309	1311	1313	rBV3	1030	623	0.08%	0.010%
24	5.542	1387	1400	1425	rBV	259630	544594	72.95%	9.116%
25	5.998	1528	1542	1570	rBV	166252	357535	47.90%	5.985%
26	6.416	1670	1672	1675	rBV3	998	577	0.08%	0.010%
27	6.580	1720	1723	1726	rBV4	1441	1168	0.16%	0.020%
28	6.722	1765	1767	1768	rBV	1091	280	0.04%	0.005%
29	6.860	1808	1810	1814	rBV4	782	664	0.09%	0.011%
30	6.921	1820	1829	1844	rBV2	82811	153158	20.52%	2.564%
31	7.117	1886	1890	1893	rBV5	2030	1344	0.18%	0.022%
32	7.178	1907	1909	1911	rBV3	1324	758	0.10%	0.013%
33	7.252	1920	1932	1958	rBV	324830	579161	77.59%	9.694%
34	7.561	2019	2028	2043	rBV2	61926	110364	14.78%	1.847%
35	7.783	2096	2097	2099	rBV2	1010	555	0.07%	0.009%
36	8.034	2166	2175	2212	rBV	144037	324108	43.42%	5.425%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042623\
 Data File : VW030892.D
 Acq On : 26 Apr 2023 20:23
 Operator : SY/MD
 Sample : 02474-21
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	8.673	2372	2374	2375	rBV2	922	311	0.04%	0.005%
38	8.709	2384	2385	2387	rBV2	719	368	0.05%	0.006%
39	8.792	2400	2411	2431	rBV	398963	659230	88.31%	11.035%
40	9.066	2494	2496	2498	rBV3	1357	723	0.10%	0.012%
41	9.124	2512	2514	2516	rBV3	1125	548	0.07%	0.009%
42	9.362	2586	2588	2590	rBV2	1095	429	0.06%	0.007%
43	9.371	2590	2591	2593	rVV3	1294	333	0.04%	0.006%
44	9.390	2593	2597	2601	rVV6	1617	1302	0.17%	0.022%
45	9.522	2636	2638	2641	rBV4	1288	892	0.12%	0.015%
46	9.686	2686	2689	2690	rBV2	1343	742	0.10%	0.012%
47	9.757	2708	2711	2714	rBV4	1758	1566	0.21%	0.026%
48	9.841	2736	2737	2742	rBV5	1037	520	0.07%	0.009%
49	9.902	2755	2756	2757	rBV	870	245	0.03%	0.004%
50	10.159	2825	2836	2853	rBV	236996	379064	50.78%	6.345%
51	10.435	2920	2922	2923	rBV	732	267	0.04%	0.004%
52	10.661	2989	2992	2995	rVB4	840	490	0.07%	0.008%
53	10.680	2995	2998	2999	rBV2	1044	551	0.07%	0.009%
54	10.734	3013	3015	3016	rBV	579	224	0.03%	0.004%
55	10.770	3022	3026	3027	rBV3	1339	951	0.13%	0.016%
56	10.870	3052	3057	3062	rBV7	1459	1801	0.24%	0.030%
57	11.194	3147	3158	3177	rBV	391666	634398	84.98%	10.619%
58	11.509	3252	3256	3259	rBV5	949	786	0.11%	0.013%
59	11.567	3264	3274	3295	rVB	347193	560668	75.11%	9.385%
60	11.802	3345	3347	3348	rBV2	858	320	0.04%	0.005%
61	11.847	3359	3361	3364	rBV3	856	459	0.06%	0.008%
62	11.886	3371	3373	3374	rBV2	762	287	0.04%	0.005%
63	11.895	3374	3376	3378	rVV3	928	454	0.06%	0.008%
64	12.021	3411	3415	3416	rBV4	1164	769	0.10%	0.013%
65	12.149	3453	3455	3456	rBV	1239	558	0.07%	0.009%
66	12.255	3486	3488	3490	rBV2	1497	613	0.08%	0.010%
67	12.648	3607	3610	3613	rVB3	1441	720	0.10%	0.012%
68	12.667	3613	3616	3618	rBV4	1877	1265	0.17%	0.021%
69	12.808	3657	3660	3661	rBV3	903	335	0.04%	0.006%
70	13.146	3763	3765	3768	rBV3	1047	600	0.08%	0.010%
71	13.336	3820	3824	3825	rBV2	967	630	0.08%	0.011%
72	13.461	3861	3863	3866	rBV3	1457	1101	0.15%	0.018%
73	13.512	3877	3879	3880	rBV2	1062	292	0.04%	0.005%
74	13.667	3926	3927	3933	rBV6	654	472	0.06%	0.008%
75	13.757	3950	3955	3956	rBV5	1241	872	0.12%	0.015%
76	14.506	4186	4188	4191	rBV4	1385	911	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030892.D
Acq On : 26 Apr 2023 20:23
Operator : SY/MD
Sample : 02474-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Title : VOC Analysis

77	15.001	4340	4342	4345	rBV4	1318	790	0.11%	0.013%
----	--------	------	------	------	------	------	-----	-------	--------




Sum of corrected areas: 5974186

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030892.D
Acq On : 26 Apr 2023 20:23
Operator : SY/MD
Sample : 02474-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

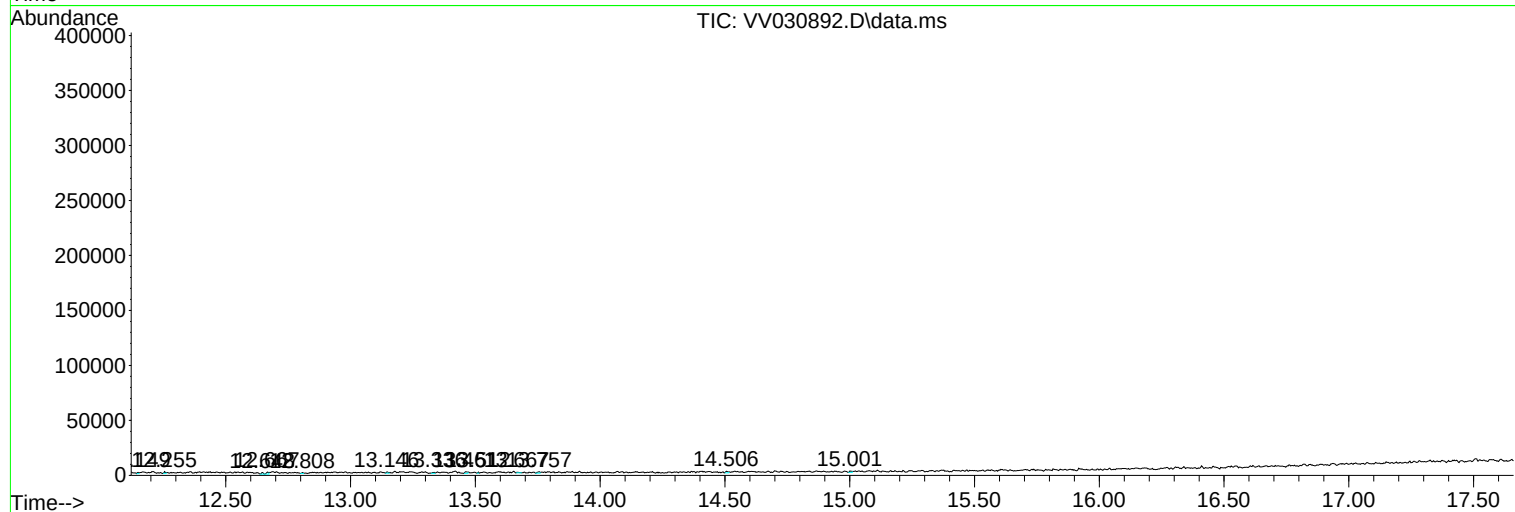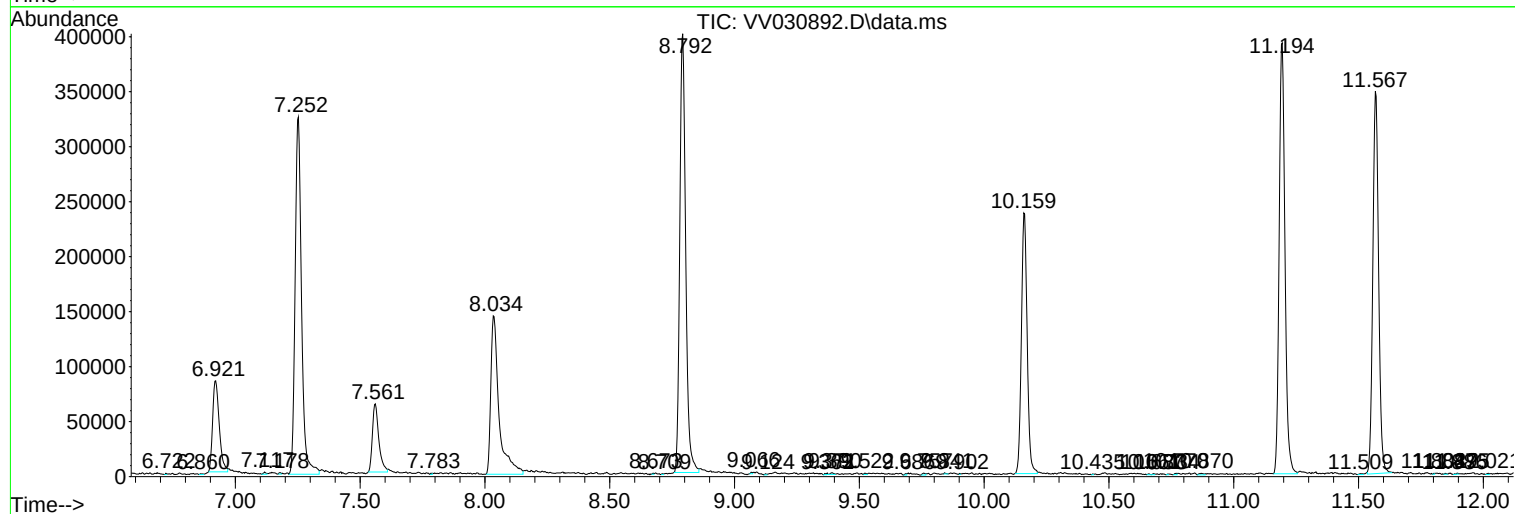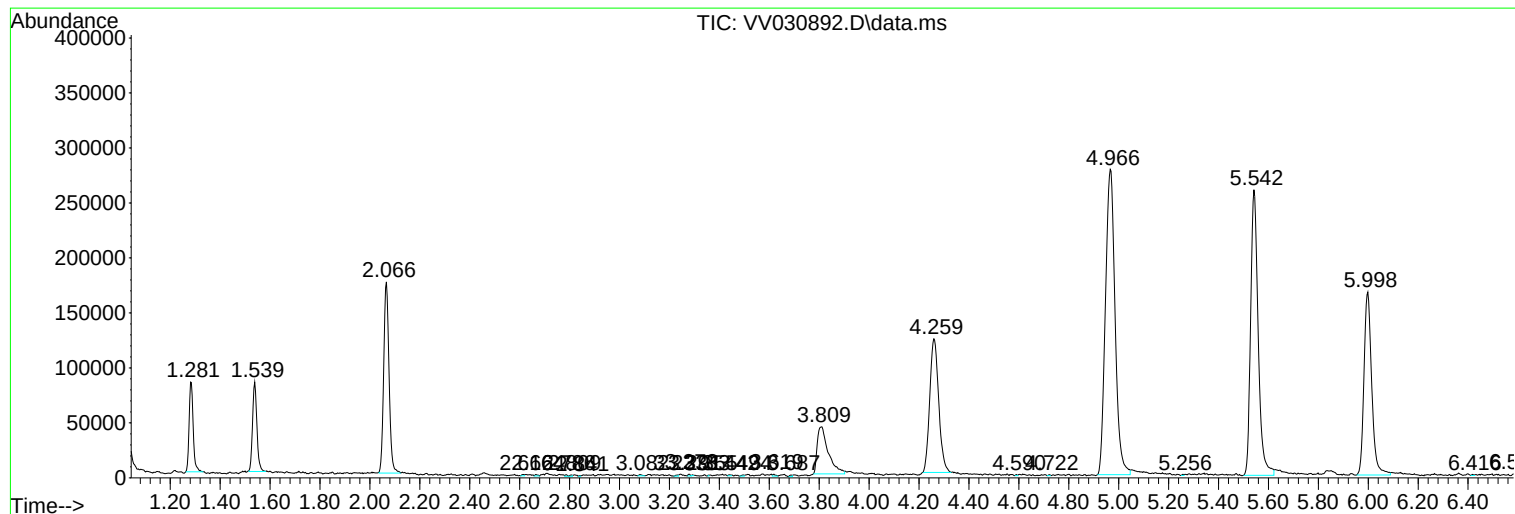

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030892.D
Acq On : 26 Apr 2023 20:23
Operator : SY/MD
Sample : 02474-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030892.D
Acq On : 26 Apr 2023 20:23
Operator : SY/MD
Sample : 02474-21
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------