


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042623\
Data File : VV030873.D
Acq On : 26 Apr 2023 10:50
Operator : SY/MD
Sample : BFB373
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB373

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Title : VOC Analysis
Last Update : Thu Apr 27 04:45:18 2023

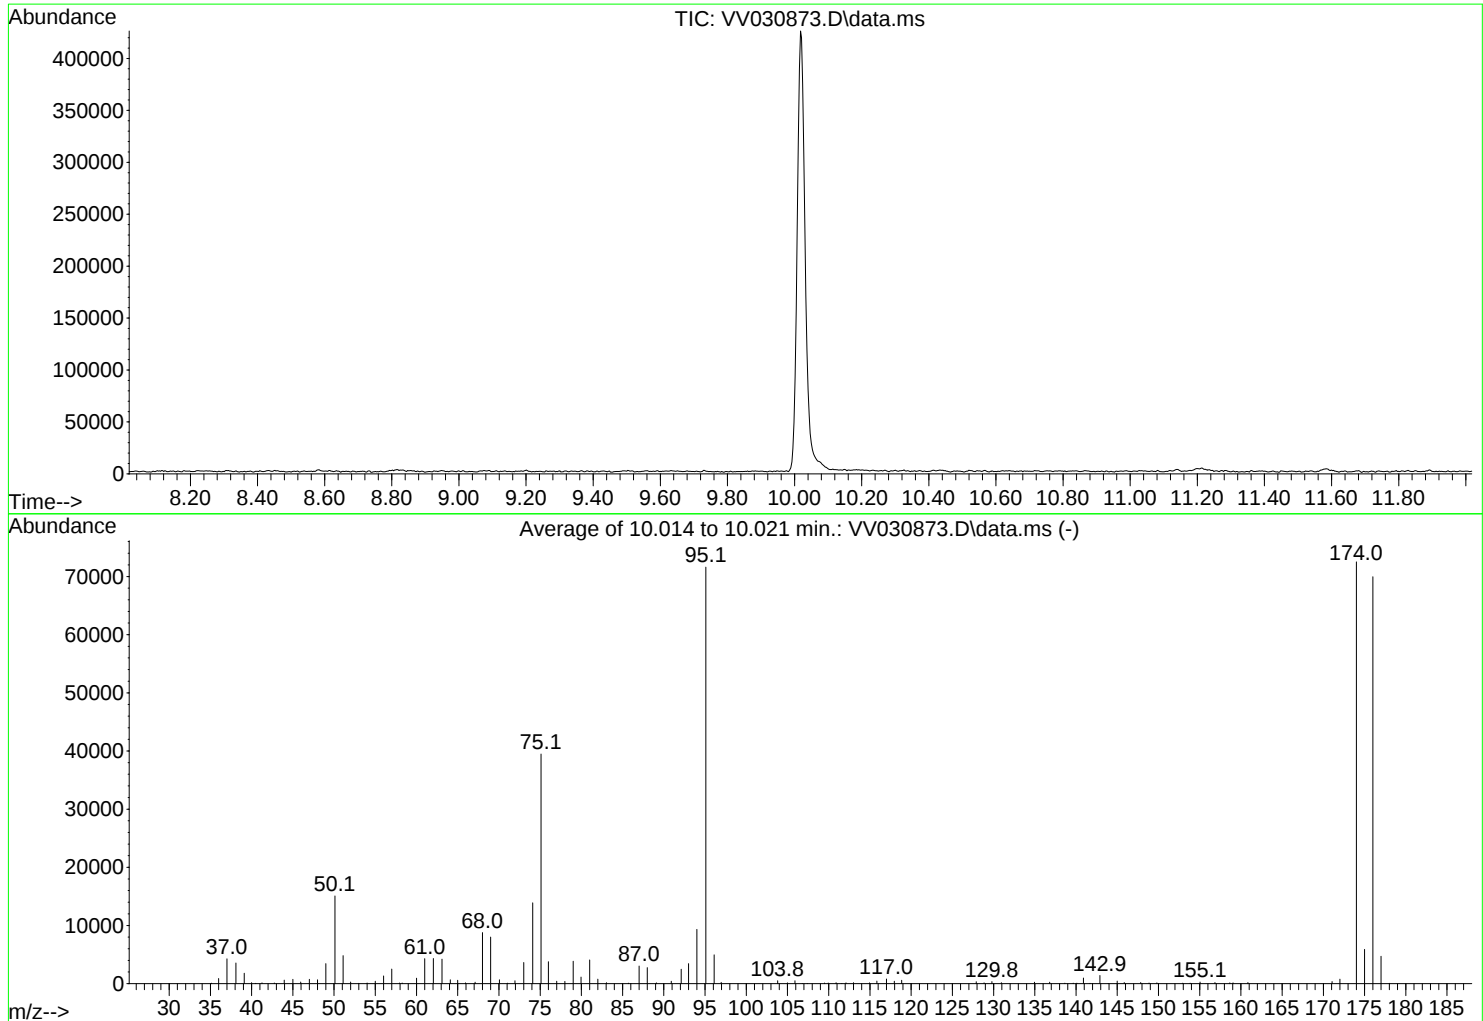

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2780

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	15066	PASS
75	95	30	80	55.1	39475	PASS
95	95	100	100	100.0	71616	PASS
96	95	5	9	6.9	4940	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	101.3	72525	PASS
175	174	5	9	8.1	5876	PASS
176	174	95	105	96.5	69963	PASS
177	176	5	10	6.7	4717	PASS

m/z	Abundance
35.60	107.0
36.30	148.0
37.10	111.0
37.70	121.0
38.20	128.0
38.70	161.0
40.00	181.0
41.90	114.0
42.30	118.0
43.90	201.0
51.50	119.0
53.00	117.0
54.00	111.0
61.40	120.0
65.10	118.0
67.90	101.0
71.40	113.0
76.90	107.0
228.30	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB373

m/z	Abundance
35.10	109.0
36.00	846.0
37.00	4110.0
38.10	3590.0
39.10	1739.0
40.00	319.0
40.50	202.0
41.20	119.0
42.30	104.0
42.80	123.0
44.00	853.0
45.00	660.0
46.00	241.0
47.10	789.0
48.00	625.0
49.00	3644.0
50.10	14225.0
51.10	4571.0
52.00	280.0
53.00	181.0
54.10	179.0
55.00	369.0
56.00	1311.0
57.00	2205.0
58.00	178.0
60.00	908.0
61.00	4073.0
62.00	4241.0
63.10	4199.0
64.00	651.0
65.00	726.0
65.90	111.0
67.10	264.0
68.10	8458.0
69.00	7717.0
70.00	687.0
71.00	115.0
72.00	525.0
73.00	3501.0
74.10	13098.0
75.10	37296.0
76.00	3588.0
77.10	551.0
78.00	482.0
79.00	3550.0
79.90	1120.0
81.00	3777.0
81.90	731.0
83.00	166.0
85.70	139.0
87.00	2941.0
88.00	2570.0
89.10	148.0
90.90	440.0
92.10	2383.0
93.00	3294.0
94.00	9103.0
95.10	68688.0
96.10	4778.0
97.00	224.0
103.80	452.0
104.90	151.0
105.90	468.0
109.50	117.0
109.90	126.0
110.90	201.0
111.60	109.0
112.10	153.0
113.00	156.0
115.00	140.0
115.90	428.0
117.00	752.0
117.90	395.0
118.80	536.0
120.00	108.0
127.90	315.0
128.80	127.0
129.80	357.0
130.90	150.0
135.00	215.0
136.80	224.0
138.70	117.0
140.10	119.0
140.90	815.0
141.70	164.0
142.90	1392.0
143.90	123.0
145.00	376.0
145.80	192.0
147.90	149.0
148.80	103.0
149.80	170.0

Instrument :
MSVOA_V
ClientSampleId :
BFB373

153.00	123.0
155.10	242.0
156.80	193.0
158.60	111.0
159.00	121.0
160.80	148.0
171.10	255.0
172.00	689.0
174.00	67352.0
175.00	5687.0
176.00	64912.0
177.00	4459.0

Instrument :
MSVOA_V
ClientSampleId :
BFB373

m/z	Abundance
36.00	897.0
37.00	4533.0
38.10	3729.0
39.10	1858.0
40.00	374.0
41.20	135.0
42.30	114.0
42.80	108.0
44.00	806.0
45.00	748.0
45.90	289.0
47.00	765.0
48.00	706.0
49.00	3499.0
50.10	15524.0
51.10	5003.0
52.00	292.0
53.00	195.0
54.00	202.0
55.00	431.0
56.00	1369.0
57.00	2640.0
57.90	173.0
58.20	175.0
60.00	962.0
61.00	4461.0
62.00	4502.0
63.10	4382.0
64.10	717.0
65.00	716.0
65.90	132.0
67.10	237.0
68.00	9212.0
69.00	8356.0
70.10	674.0
71.10	116.0
71.90	530.0
73.00	3730.0
74.10	14286.0
75.10	40912.0
76.00	3954.0
77.00	561.0
78.00	419.0
79.00	3977.0
80.00	1129.0
81.00	4227.0
82.00	773.0
83.10	174.0
85.70	135.0
87.00	3171.0
88.00	2880.0
89.10	146.0
90.90	426.0
92.10	2607.0
93.00	3535.0
94.00	9671.0
95.10	74104.0
96.10	5113.0
97.00	242.0
103.80	524.0
105.00	139.0
105.90	514.0
107.40	103.0
109.50	130.0
110.00	126.0
110.90	169.0
112.10	159.0
113.00	187.0
114.90	136.0
115.90	461.0
117.00	827.0
117.90	408.0
118.80	579.0
127.90	320.0
128.80	121.0
129.80	382.0
130.90	162.0
134.90	239.0
136.80	262.0
138.60	104.0
139.60	118.0
140.10	115.0
140.90	950.0
142.00	109.0
142.90	1436.0
145.00	449.0
145.80	203.0
147.90	205.0
148.80	103.0
149.80	154.0
152.90	114.0
153.90	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB373

155.00	298.0
156.80	191.0
158.60	153.0
159.00	164.0
160.80	215.0
171.10	293.0
172.00	814.0
174.00	75304.0
175.00	6064.0
176.00	72192.0
177.00	4871.0

Instrument :
MSVOA_V
ClientSampleId :
BFB373

m/z	Abundance
35.20	107.0
36.00	904.0
37.00	4527.0
38.10	3741.0
39.10	1800.0
40.00	360.0
41.30	140.0
42.30	113.0
42.70	105.0
44.00	737.0
45.00	801.0
45.90	293.0
46.90	709.0
48.00	676.0
49.00	3201.0
50.10	15448.0
51.10	4876.0
52.00	246.0
53.10	173.0
54.00	252.0
55.00	481.0
56.00	1289.0
57.00	2694.0
58.30	186.0
60.00	931.0
61.00	4380.0
62.10	4256.0
63.10	4061.0
64.20	651.0
65.00	655.0
66.00	163.0
67.10	208.0
68.00	8961.0
69.00	7997.0
70.10	641.0
72.00	463.0
73.00	3683.0
74.10	14317.0
75.10	40216.0
76.00	3750.0
77.00	489.0
78.00	293.0
79.00	4008.0
80.00	1125.0
81.00	4195.0
82.10	785.0
83.10	152.0
86.00	112.0
87.00	2987.0
88.00	2848.0
89.10	114.0
90.90	407.0
92.10	2440.0
93.00	3488.0
94.00	9218.0
95.10	72056.0
96.10	4930.0
96.90	227.0
103.80	547.0
105.10	134.0
105.90	514.0
106.80	113.0
109.50	100.0
109.90	121.0
110.90	112.0
112.10	132.0
113.00	176.0
114.90	131.0
115.80	443.0
117.00	801.0
118.00	409.0
118.90	661.0
127.90	351.0
128.90	146.0
129.80	355.0
131.00	176.0
134.90	276.0
136.80	228.0
139.70	148.0
140.90	1105.0
142.90	1400.0
145.00	471.0
145.90	199.0
147.80	248.0
148.90	101.0
149.80	126.0
153.80	146.0
155.00	315.0
156.90	157.0
158.70	185.0
159.10	175.0
160.90	195.0

Instrument :
MSVOA_V
ClientSampleId :
BFB373

170.90	269.0
171.10	272.0
172.00	856.0
174.00	74920.0
175.00	5878.0
176.00	72784.0
177.00	4820.0
178.00	132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB373