

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042624\
 Data File : VW035423.D
 Acq On : 26 Apr 2024 13:35
 Operator : SY/MD
 Sample : P2269-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ3

Quant Time: Apr 27 00:34:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 27 00:18:54 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	433725	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	420529	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	184145	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	161027	46.197	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	92.400%	
7) Chloroethane-d5	1.529	69	136172	68.185	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	136.360%#	
11) 1,1-Dichloroethene-d2	2.056	65	70139	49.234	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	98.460%	
21) 2-Butanone-d5	3.789	46	222070	124.308	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	124.310%	
24) Chloroform-d	4.243	84	331799	56.570	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	113.140%	
26) 1,2-Dichloroethane-d4	4.937	65	206666	60.494	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	120.980%	
32) Benzene-d6	4.956	84	642371	58.127	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	116.260%	
36) 1,2-Dichloropropane-d6	5.985	67	210489	61.733	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	123.460%#	
41) Toluene-d8	7.239	98	542391	54.453	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	108.900%	
43) trans-1,3-Dichloroprop...	7.551	79	83826	52.554	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	105.100%	
47) 2-Hexanone-d5	8.024	63	118309	120.361	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	120.360%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84	296489	61.009	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	122.020%#	
66) 1,2-Dichlorobenzene-d4	11.558	152	216715	67.267	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	134.540%#	
Target Compounds						
13) Acetone	2.124	43	8412	3.963	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035423.D
Acq On : 26 Apr 2024 13:35
Operator : SY/MD
Sample : P2269-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ3

Quant Time: Apr 27 00:34:09 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 27 00:18:54 2024
Response via : Initial Calibration

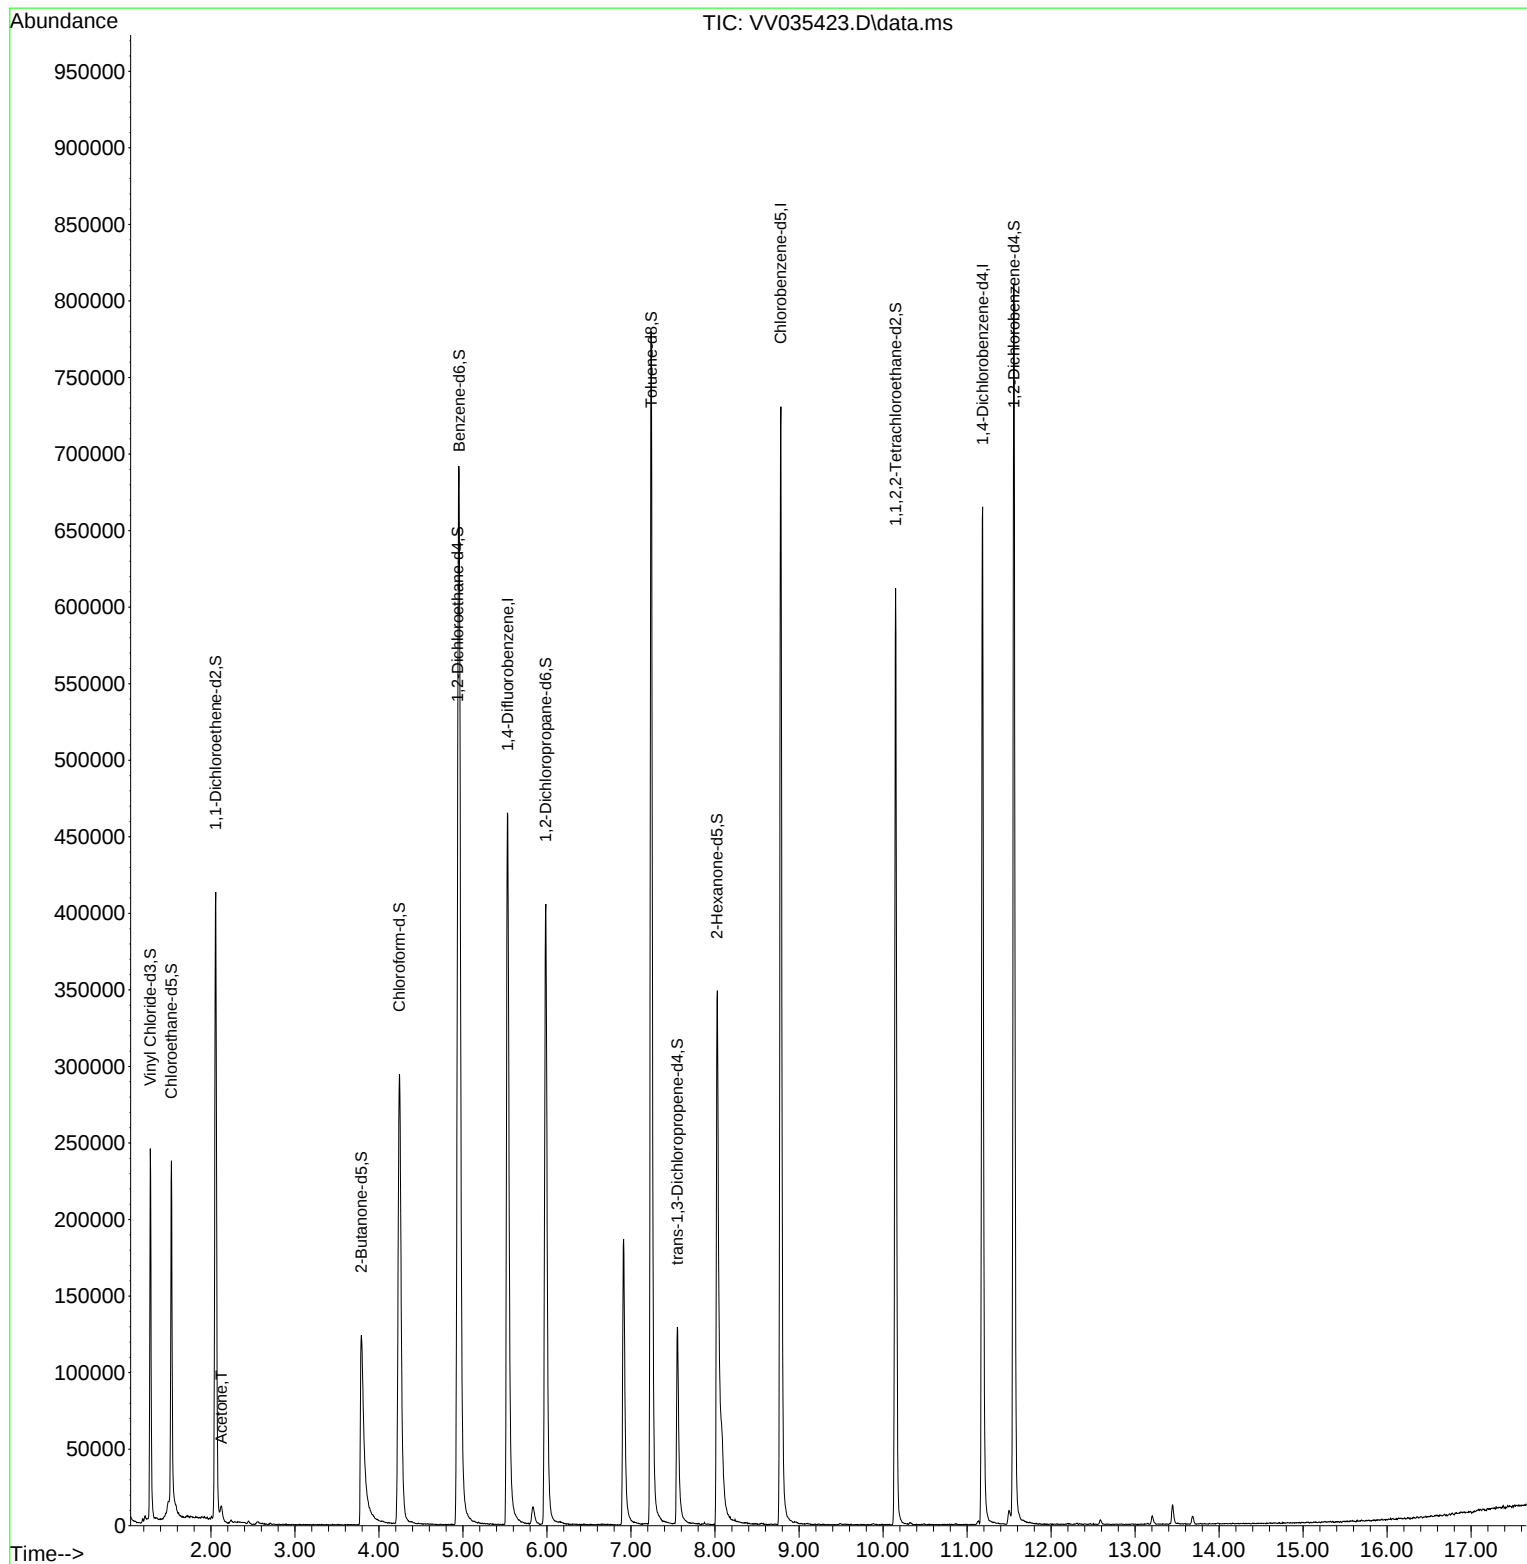

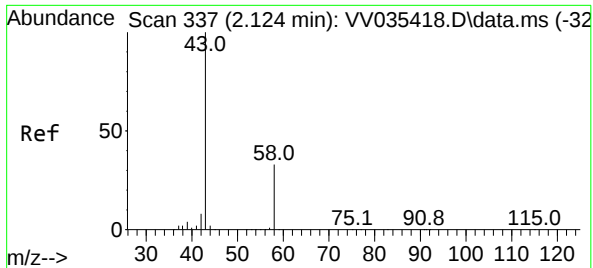

#13
 Acetone
 Concen: 3.963 ug/L
 RT: 2.124 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: VV035423.D
 Acq: 26 Apr 2024 13:35

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ3

Tgt Ion: 43 Resp: 8412
 Ion Ratio Lower Upper
 43 100
 58 34.5 0.0 65.8

