

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035422.D
 Acq On : 26 Apr 2024 13:09
 Operator : SY/MD
 Sample : VV0426WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK277

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M

Title : VOC Analysis

Signal : TIC: VV035422.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rBV	291912	304748	16.71%	2.185%
2	1.532	145	153	169	rVB	243868	278575	15.28%	1.997%
3	2.056	305	316	334	rBV	450214	664815	36.46%	4.766%
4	2.449	429	438	447	rVB3	4060	6900	0.38%	0.049%
5	2.490	447	451	454	rVB	395	356	0.02%	0.003%
6	2.551	469	470	477	rVB4	414	303	0.02%	0.002%
7	2.606	485	487	491	rBV2	324	269	0.01%	0.002%
8	2.696	510	515	519	rBV4	595	680	0.04%	0.005%
9	2.796	540	546	547	rBV2	504	456	0.03%	0.003%
10	2.844	556	561	564	rBV2	257	268	0.01%	0.002%
11	2.912	578	582	585	rVV2	293	237	0.01%	0.002%
12	2.986	599	605	608	rBV2	288	289	0.02%	0.002%
13	3.040	618	622	627	rBV3	315	337	0.02%	0.002%
14	3.066	627	630	633	rVV2	358	255	0.01%	0.002%
15	3.117	641	646	651	rVB3	371	336	0.02%	0.002%
16	3.156	651	658	664	rBV3	208	256	0.01%	0.002%
17	3.204	670	673	677	rBV3	274	240	0.01%	0.002%
18	3.407	730	736	740	rVB2	388	401	0.02%	0.003%
19	3.442	740	747	751	rBV3	324	449	0.02%	0.003%
20	3.516	765	770	774	rBV	323	324	0.02%	0.002%
21	3.793	847	856	906	rBV	106873	343925	18.86%	2.466%
22	4.246	977	997	1031	rBV	279511	725474	39.78%	5.201%
23	4.516	1078	1081	1085	rVB3	518	360	0.02%	0.003%
24	4.619	1110	1113	1117	rBV4	497	327	0.02%	0.002%
25	4.696	1133	1137	1142	rBV3	326	279	0.02%	0.002%
26	4.870	1188	1191	1196	rVB	334	253	0.01%	0.002%
27	4.953	1196	1217	1263	rBV2	686828	1823505	100.00%	13.073%
28	5.458	1372	1374	1380	rVB4	363	266	0.01%	0.002%
29	5.529	1385	1396	1442	rBV	569509	1206323	66.15%	8.648%
30	5.838	1480	1492	1510	rBV3	9367	23183	1.27%	0.166%
31	5.985	1524	1538	1573	rBV	385964	812810	44.57%	5.827%
32	6.201	1602	1605	1612	rVB5	787	722	0.04%	0.005%
33	6.236	1612	1616	1619	rBV5	373	304	0.02%	0.002%
34	6.362	1652	1655	1661	rVB2	261	228	0.01%	0.002%
35	6.403	1664	1668	1672	rBV	347	376	0.02%	0.003%
36	6.445	1677	1681	1687	rVB2	287	374	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035422.D
 Acq On : 26 Apr 2024 13:09
 Operator : SY/MD
 Sample : VV0426WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK277

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.493	1695	1696	1701	rVB	402	229	0.01%	0.002%
38	6.612	1728	1733	1736	rBV2	301	279	0.02%	0.002%
39	6.664	1746	1749	1753	rVB2	393	262	0.01%	0.002%
40	6.911	1815	1826	1851	rBV	192485	371305	20.36%	2.662%
41	7.239	1917	1928	1960	rBV	792851	1415196	77.61%	10.146%
42	7.551	2016	2025	2052	rBV	130379	247312	13.56%	1.773%
43	8.027	2163	2173	2218	rBV3	286066	738343	40.49%	5.293%
44	8.468	2306	2310	2311	rBV	571	338	0.02%	0.002%
45	8.587	2343	2347	2353	rVB3	471	423	0.02%	0.003%
46	8.616	2353	2356	2358	rBV3	380	233	0.01%	0.002%
47	8.780	2396	2407	2441	rBV	883479	1476712	80.98%	10.587%
48	9.017	2478	2481	2484	rBV4	429	320	0.02%	0.002%
49	9.062	2493	2495	2499	rVB3	548	280	0.02%	0.002%
50	9.091	2499	2504	2507	rBV3	489	511	0.03%	0.004%
51	9.120	2510	2513	2516	rVV2	586	451	0.02%	0.003%
52	9.165	2520	2527	2528	rBV3	454	340	0.02%	0.002%
53	9.191	2531	2535	2538	rVB2	365	264	0.01%	0.002%
54	9.239	2548	2550	2556	rVB3	323	280	0.02%	0.002%
55	9.265	2556	2558	2563	rVB2	507	416	0.02%	0.003%
56	9.320	2563	2575	2578	rBV3	395	450	0.02%	0.003%
57	9.464	2614	2620	2624	rBV2	333	381	0.02%	0.003%
58	9.493	2625	2629	2636	rVV4	631	793	0.04%	0.006%
59	9.628	2668	2671	2673	rBV	346	235	0.01%	0.002%
60	9.751	2703	2709	2713	rBV2	443	319	0.02%	0.002%
61	10.021	2787	2793	2794	rBV	307	299	0.02%	0.002%
62	10.149	2819	2833	2861	rBV	537739	866186	47.50%	6.210%
63	10.352	2892	2896	2903	rVB3	540	730	0.04%	0.005%
64	10.484	2931	2937	2938	rVV3	606	560	0.03%	0.004%
65	10.493	2938	2940	2945	rVV3	671	569	0.03%	0.004%
66	10.677	2995	2997	3003	rVV3	220	263	0.01%	0.002%
67	10.789	3028	3032	3043	rBV3	496	616	0.03%	0.004%
68	10.866	3049	3056	3063	rVV3	925	1305	0.07%	0.009%
69	11.098	3122	3128	3129	rBV	294	269	0.01%	0.002%
70	11.130	3130	3138	3144	rVV5	2686	3369	0.18%	0.024%
71	11.181	3144	3154	3188	rVV	828885	1307495	71.70%	9.374%
72	11.451	3235	3238	3241	rBV2	508	301	0.02%	0.002%
73	11.558	3258	3271	3310	rBV	770031	1237626	67.87%	8.873%
74	11.725	3320	3323	3329	rVB3	922	791	0.04%	0.006%
75	11.818	3349	3352	3357	rVB2	351	325	0.02%	0.002%
76	11.847	3359	3361	3365	rVB3	417	275	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035422.D
 Acq On : 26 Apr 2024 13:09
 Operator : SY/MD
 Sample : VV0426WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK277

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	11.889	3371	3374	3377	rBV3	310	234	0.01%	0.002%
78	11.956	3391	3395	3398	rBV2	297	284	0.02%	0.002%
79	11.995	3405	3407	3411	rVB2	418	284	0.02%	0.002%
80	12.133	3448	3450	3453	rVV2	394	259	0.01%	0.002%
81	12.162	3456	3459	3463	rVB2	284	243	0.01%	0.002%
82	12.233	3478	3481	3484	rBV2	262	254	0.01%	0.002%
83	12.323	3502	3509	3510	rBV2	535	395	0.02%	0.003%
84	12.381	3524	3527	3529	rBV2	548	230	0.01%	0.002%
85	12.455	3547	3550	3555	rVV3	315	324	0.02%	0.002%
86	12.590	3583	3592	3606	rVB8	3043	5484	0.30%	0.039%
87	12.686	3620	3622	3628	rVB3	369	259	0.01%	0.002%
88	12.718	3628	3632	3635	rBV	371	298	0.02%	0.002%
89	12.763	3643	3646	3649	rBV2	383	270	0.01%	0.002%
90	12.844	3668	3671	3674	rBV3	296	230	0.01%	0.002%
91	13.001	3717	3720	3725	rBV2	388	349	0.02%	0.003%
92	13.082	3742	3745	3749	rBV3	422	328	0.02%	0.002%
93	13.207	3775	3784	3794	rBV4	7193	11462	0.63%	0.082%
94	13.358	3828	3831	3833	rBV	350	227	0.01%	0.002%
95	13.445	3847	3858	3880	rBV	20633	37355	2.05%	0.268%
96	13.683	3924	3932	3943	rVV3	7972	12258	0.67%	0.088%
97	13.808	3967	3971	3974	rBV3	501	402	0.02%	0.003%
98	14.313	4126	4128	4131	rBV2	528	289	0.02%	0.002%
99	14.622	4221	4224	4226	rBV2	537	391	0.02%	0.003%
100	14.934	4317	4321	4325	rBV5	730	749	0.04%	0.005%




Sum of corrected areas: 13948712

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035422.D
Acq On : 26 Apr 2024 13:09
Operator : SY/MD
Sample : VV0426WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK277

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

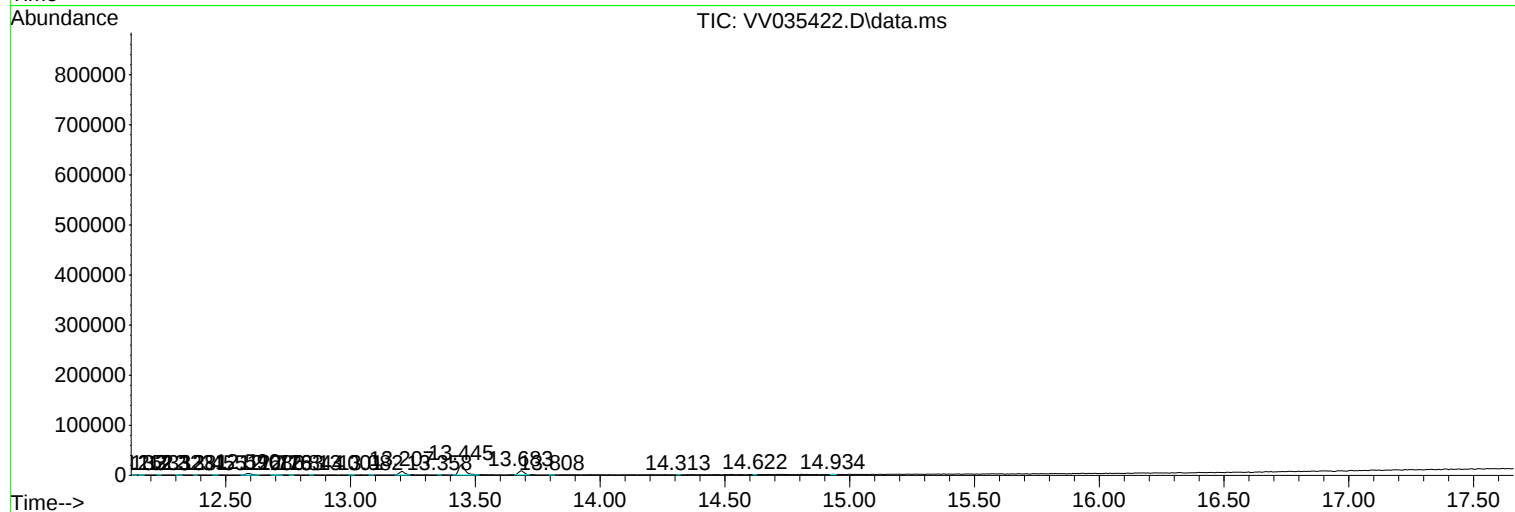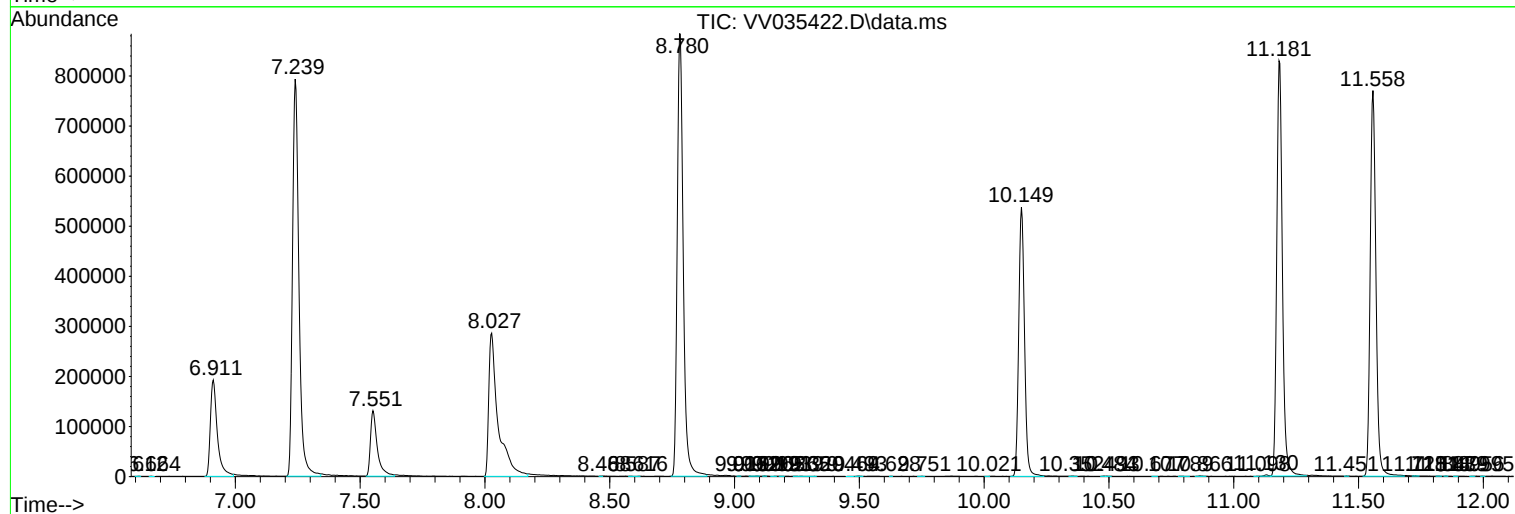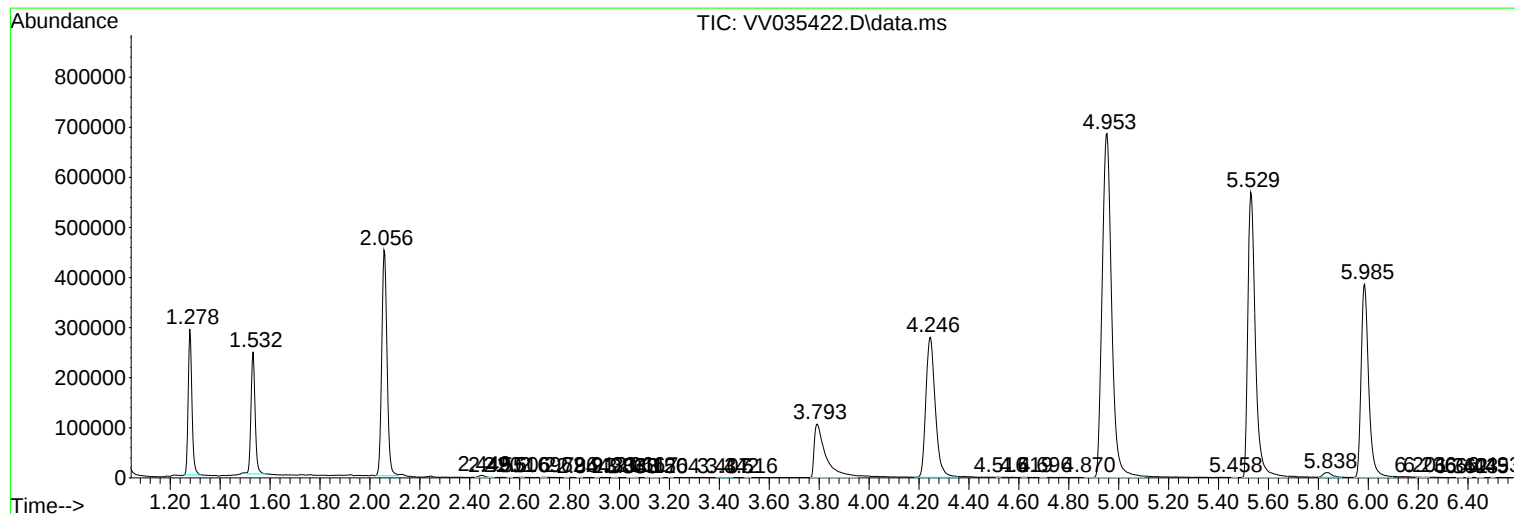

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035422.D
Acq On : 26 Apr 2024 13:09
Operator : SY/MD
Sample : VV0426WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK277

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035422.D
Acq On : 26 Apr 2024 13:09
Operator : SY/MD
Sample : VV0426WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK277

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------