

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035424.D
 Acq On : 26 Apr 2024 13:59
 Operator : SY/MD
 Sample : P2280-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08P0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035424.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.191	42	47	51	rBV3	6137	5820	0.32%	0.043%
2	1.278	67	74	92	rVB	290770	307525	16.73%	2.253%
3	1.523	143	150	169	rVB	219543	271586	14.78%	1.989%
4	2.056	306	316	328	rBV	455786	662464	36.04%	4.852%
5	2.445	432	437	446	rBV6	1626	2216	0.12%	0.016%
6	2.558	462	472	476	rBV5	3075	4705	0.26%	0.034%
7	2.699	509	516	517	rBV4	787	727	0.04%	0.005%
8	2.802	545	548	549	rBV	156	88	0.00%	0.001%
9	2.883	570	573	575	rBV3	647	492	0.03%	0.004%
10	2.953	592	595	596	rBV	267	102	0.01%	0.001%
11	3.024	615	617	619	rBV2	281	157	0.01%	0.001%
12	3.082	632	635	637	rBV	238	170	0.01%	0.001%
13	3.114	643	645	647	rVB2	254	106	0.01%	0.001%
14	3.127	647	649	651	rBV3	126	47	0.00%	0.000%
15	3.178	663	665	669	rBV2	271	194	0.01%	0.001%
16	3.201	669	672	674	rBV2	283	220	0.01%	0.002%
17	3.256	687	689	691	rBV	232	133	0.01%	0.001%
18	3.291	697	700	702	rBV2	157	100	0.01%	0.001%
19	3.384	728	729	731	rVB	128	26	0.00%	0.000%
20	3.394	731	732	733	rBV	115	27	0.00%	0.000%
21	3.445	746	748	751	rVB2	258	135	0.01%	0.001%
22	3.461	751	753	757	rBV2	148	93	0.01%	0.001%
23	3.481	757	759	761	rBV2	64	30	0.00%	0.000%
24	3.494	761	763	765	rBV	175	66	0.00%	0.000%
25	3.561	781	784	788	rBV2	108	104	0.01%	0.001%
26	3.584	788	791	792	rBV2	349	239	0.01%	0.002%
27	3.632	803	806	807	rBV	286	144	0.01%	0.001%
28	3.658	811	814	817	rVV	220	140	0.01%	0.001%
29	3.783	844	853	894	rBV	106075	310825	16.91%	2.277%
30	4.246	980	997	1032	rBV	287280	806933	43.90%	5.910%
31	4.600	1104	1107	1109	rBV2	498	313	0.02%	0.002%
32	4.735	1146	1149	1152	rBV2	278	226	0.01%	0.002%
33	4.834	1175	1180	1183	rBV3	424	468	0.03%	0.003%
34	4.950	1201	1216	1264	rBV2	689500	1838140	100.00%	13.464%
35	5.529	1385	1396	1435	rBV	545532	1158814	63.04%	8.488%
36	5.834	1482	1491	1507	rBV2	9428	21184	1.15%	0.155%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035424.D
 Acq On : 26 Apr 2024 13:59
 Operator : SY/MD
 Sample : P2280-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08P0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	5.985	1525	1538	1575	rBV	391753	817290	44.46%	5.986%
38	6.243	1616	1618	1620	rBV2	474	260	0.01%	0.002%
39	6.297	1633	1635	1637	rBV2	199	117	0.01%	0.001%
40	6.336	1645	1647	1649	rBV2	363	163	0.01%	0.001%
41	6.365	1654	1656	1658	rBV	173	74	0.00%	0.001%
42	6.387	1659	1663	1665	rBV	308	228	0.01%	0.002%
43	6.442	1672	1680	1697	rVB2	7968	15328	0.83%	0.112%
44	6.564	1714	1718	1719	rBV	305	168	0.01%	0.001%
45	6.603	1729	1730	1734	rVB	144	61	0.00%	0.000%
46	6.622	1734	1736	1738	rBV2	253	116	0.01%	0.001%
47	6.648	1738	1744	1751	rVV2	227	360	0.02%	0.003%
48	6.677	1751	1753	1755	rBV	71	37	0.00%	0.000%
49	6.690	1755	1757	1760	rBV2	103	54	0.00%	0.000%
50	6.709	1760	1763	1767	rBV2	129	105	0.01%	0.001%
51	6.757	1776	1778	1780	rVB	109	58	0.00%	0.000%
52	6.789	1784	1788	1790	rVV2	239	173	0.01%	0.001%
53	6.911	1815	1826	1864	rBV	193214	381776	20.77%	2.796%
54	7.239	1917	1928	1950	rBV	797822	1409239	76.67%	10.322%
55	7.551	2016	2025	2053	rBV	132354	251073	13.66%	1.839%
56	7.876	2119	2126	2133	rBV5	960	1412	0.08%	0.010%
57	7.947	2147	2148	2151	rVB	323	116	0.01%	0.001%
58	7.960	2151	2152	2154	rBV	180	72	0.00%	0.001%
59	7.985	2158	2160	2161	rBV	224	60	0.00%	0.000%
60	8.024	2163	2172	2213	rBV2	279012	660825	35.95%	4.840%
61	8.561	2337	2339	2345	rVB3	501	387	0.02%	0.003%
62	8.664	2368	2371	2375	rBV2	284	192	0.01%	0.001%
63	8.783	2396	2408	2445	rBV	844304	1408673	76.64%	10.318%
64	9.259	2554	2556	2560	rVB3	296	113	0.01%	0.001%
65	9.336	2574	2580	2582	rVB2	388	281	0.02%	0.002%
66	9.355	2582	2586	2588	rBV3	407	282	0.02%	0.002%
67	9.445	2611	2614	2618	rBV2	155	139	0.01%	0.001%
68	9.487	2620	2627	2628	rBV4	1349	1216	0.07%	0.009%
69	9.628	2668	2671	2673	rBV2	229	139	0.01%	0.001%
70	9.673	2682	2685	2693	rBB3	339	387	0.02%	0.003%
71	9.706	2693	2695	2701	rVB2	255	161	0.01%	0.001%
72	9.744	2704	2707	2710	rBV2	214	149	0.01%	0.001%
73	9.821	2728	2731	2733	rBV2	179	82	0.00%	0.001%
74	9.927	2761	2764	2766	rVB	212	91	0.00%	0.001%
75	9.950	2766	2771	2775	rBV2	294	238	0.01%	0.002%
76	10.098	2815	2817	2818	rBV2	230	90	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035424.D
 Acq On : 26 Apr 2024 13:59
 Operator : SY/MD
 Sample : P2280-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08P0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	10.149	2821	2833	2863	rVV	538561	856375	46.59%	6.273%
78	10.381	2903	2905	2906	rBV2	297	126	0.01%	0.001%
79	10.403	2910	2912	2915	rVB	343	166	0.01%	0.001%
80	10.419	2915	2917	2918	rBV	164	68	0.00%	0.000%
81	10.480	2934	2936	2937	rBV	271	149	0.01%	0.001%
82	10.709	3005	3007	3016	rVB2	577	772	0.04%	0.006%
83	10.792	3029	3033	3039	rVB3	530	473	0.03%	0.003%
84	10.860	3049	3054	3062	rBV5	867	1170	0.06%	0.009%
85	10.927	3069	3075	3076	rBV	443	336	0.02%	0.002%
86	11.024	3102	3105	3107	rVB3	445	247	0.01%	0.002%
87	11.181	3143	3154	3183	rBV	755576	1211385	65.90%	8.873%
88	11.442	3232	3235	3240	rBV2	322	337	0.02%	0.002%
89	11.558	3258	3271	3296	rBV	757214	1208390	65.74%	8.851%
90	11.937	3384	3389	3394	rBV4	668	768	0.04%	0.006%
91	12.011	3410	3412	3417	rBV2	413	232	0.01%	0.002%
92	12.442	3543	3546	3549	rBV2	301	169	0.01%	0.001%
93	12.458	3549	3551	3553	rBV	322	169	0.01%	0.001%
94	12.561	3581	3583	3585	rBV2	293	149	0.01%	0.001%
95	12.596	3586	3594	3601	rVB6	1524	2418	0.13%	0.018%
96	12.648	3608	3610	3612	rBV	382	154	0.01%	0.001%
97	12.866	3674	3678	3679	rBV2	437	257	0.01%	0.002%
98	13.448	3849	3859	3876	rBV2	8153	15536	0.85%	0.114%
99	13.635	3915	3917	3919	rBV2	405	236	0.01%	0.002%
100	13.686	3925	3933	3943	rVB4	3784	5914	0.32%	0.043%




Sum of corrected areas: 13652540

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035424.D
Acq On : 26 Apr 2024 13:59
Operator : SY/MD
Sample : P2280-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08P0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

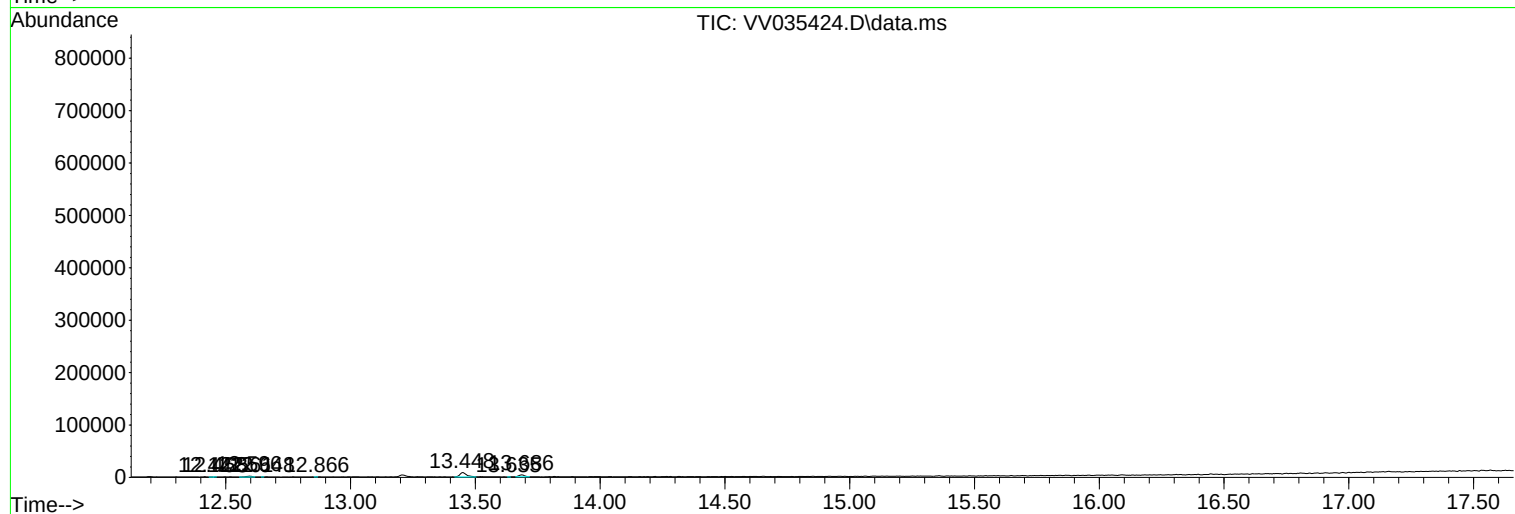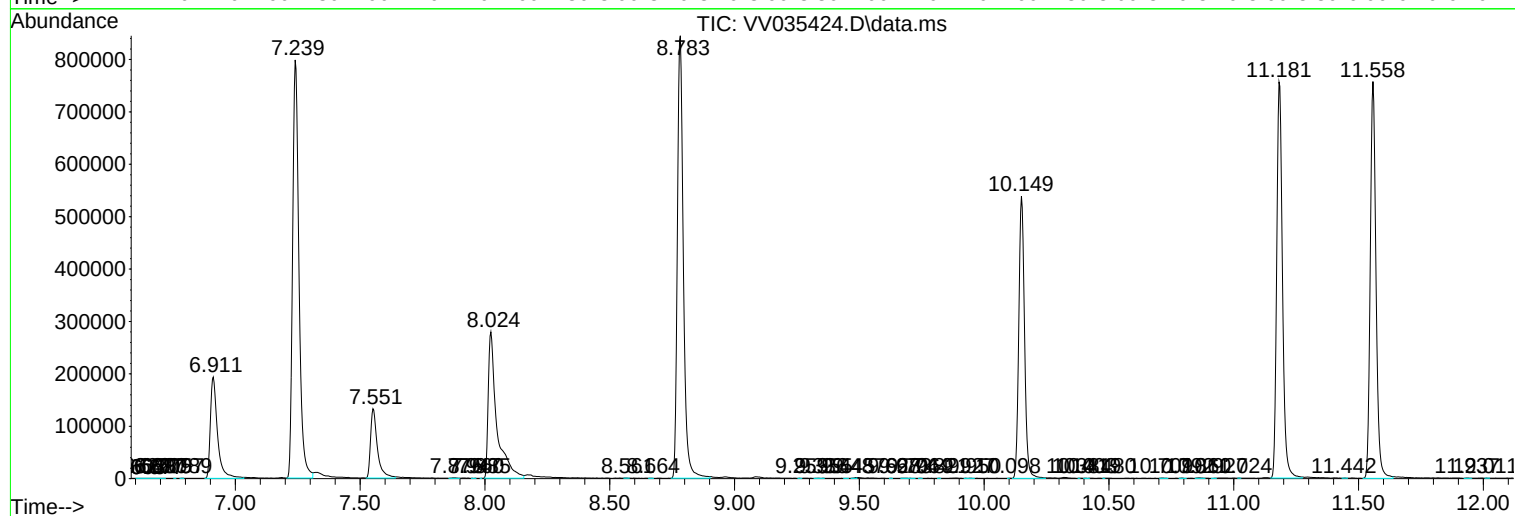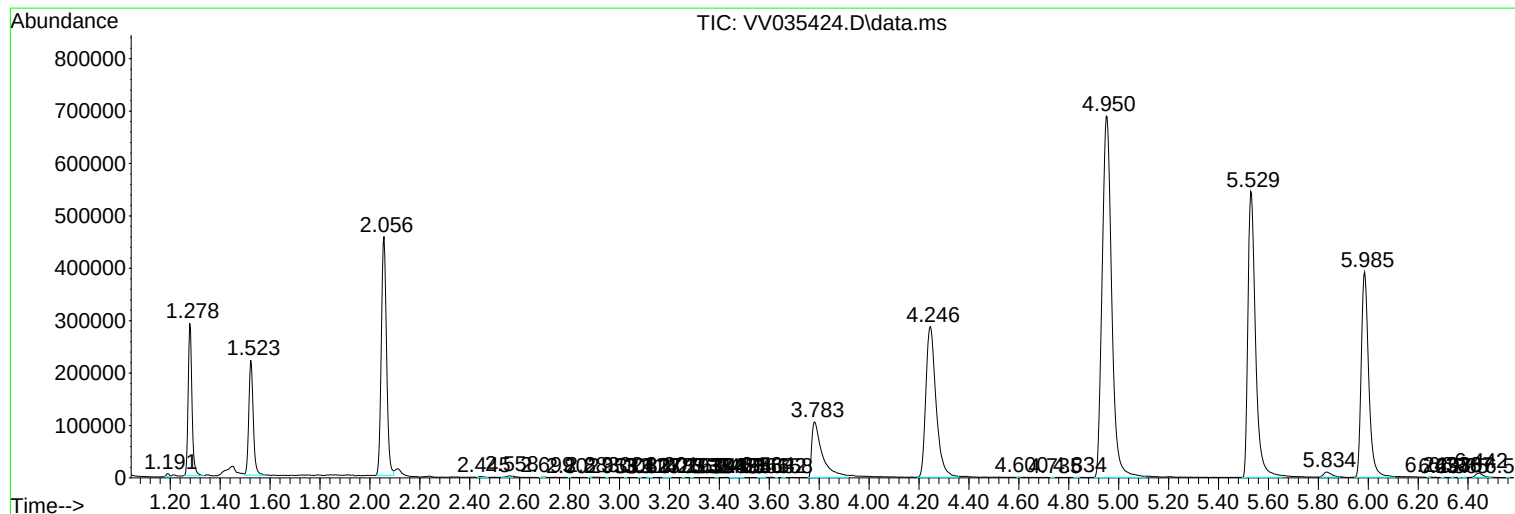

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035424.D
Acq On : 26 Apr 2024 13:59
Operator : SY/MD
Sample : P2280-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08P0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035424.D
Acq On : 26 Apr 2024 13:59
Operator : SY/MD
Sample : P2280-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08P0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------