

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035425.D
 Acq On : 26 Apr 2024 14:28
 Operator : SY/MD
 Sample : P2269-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035425.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	42	46	49	rBV	2988	2415	0.05%	0.010%
2	1.214	49	54	60	rBV	8850	9613	0.20%	0.040%
3	1.278	67	74	89	rVB	279927	303788	6.47%	1.260%
4	1.526	144	151	174	rVB	201207	256153	5.45%	1.063%
5	2.053	305	315	329	rBV	456169	661165	14.07%	2.743%
6	2.121	330	336	362	rVB	28210	54462	1.16%	0.226%
7	2.233	362	371	380	rBV3	2244	3619	0.08%	0.015%
8	2.301	390	392	394	rBV2	440	235	0.01%	0.001%
9	2.330	399	401	404	rBV4	465	282	0.01%	0.001%
10	2.442	431	436	445	rVB5	1860	2912	0.06%	0.012%
11	2.555	458	471	483	rBV	23599	51414	1.09%	0.213%
12	2.838	556	559	566	rVB3	389	271	0.01%	0.001%
13	2.870	566	569	575	rBV2	304	437	0.01%	0.002%
14	2.915	580	583	589	rVB2	430	329	0.01%	0.001%
15	2.982	602	604	612	rVB2	451	389	0.01%	0.002%
16	3.066	623	630	632	rBV2	257	296	0.01%	0.001%
17	3.092	635	638	641	rBV2	355	243	0.01%	0.001%
18	3.400	730	734	741	rVB3	272	258	0.01%	0.001%
19	3.455	747	751	754	rVB2	301	241	0.01%	0.001%
20	3.478	754	758	762	rBV2	471	405	0.01%	0.002%
21	3.793	844	856	909	rBV2	122036	427342	9.10%	1.773%
22	4.243	980	996	1033	rBV2	284086	737758	15.70%	3.061%
23	4.777	1159	1162	1165	rBV2	359	266	0.01%	0.001%
24	4.802	1165	1170	1172	rVV2	244	273	0.01%	0.001%
25	4.818	1172	1175	1177	rVV2	377	249	0.01%	0.001%
26	4.831	1178	1179	1184	rVV3	358	300	0.01%	0.001%
27	4.857	1184	1187	1191	rVB	325	231	0.00%	0.001%
28	4.950	1200	1216	1262	rBV2	699232	1883373	40.09%	7.815%
29	5.400	1353	1356	1359	rBV2	456	301	0.01%	0.001%
30	5.529	1384	1396	1450	rBV	1223736	2491411	53.03%	10.337%
31	5.831	1480	1490	1508	rBV6	9900	22441	0.48%	0.093%
32	5.934	1520	1522	1524	rVB	505	240	0.01%	0.001%
33	5.982	1525	1537	1566	rBV	392617	827204	17.61%	3.432%
34	6.339	1645	1648	1652	rVB3	518	397	0.01%	0.002%
35	6.362	1652	1655	1659	rVB3	356	250	0.01%	0.001%
36	6.461	1684	1686	1692	rVB3	749	560	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035425.D
 Acq On : 26 Apr 2024 14:28
 Operator : SY/MD
 Sample : P2269-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.571	1716	1720	1724	rBV3	314	294	0.01%	0.001%
38	6.658	1742	1747	1750	rBV2	371	334	0.01%	0.001%
39	6.912	1815	1826	1857	rBV	201697	392673	8.36%	1.629%
40	7.239	1917	1928	1956	rBV	807802	1429031	30.42%	5.929%
41	7.551	2015	2025	2052	rBV	138873	259842	5.53%	1.078%
42	7.735	2079	2082	2085	rVB2	407	283	0.01%	0.001%
43	7.911	2134	2137	2145	rVB4	1403	1725	0.04%	0.007%
44	7.947	2145	2148	2154	rVB2	297	323	0.01%	0.001%
45	8.027	2163	2173	2232	rBV2	321095	783277	16.67%	3.250%
46	8.317	2260	2263	2273	rVB6	936	1237	0.03%	0.005%
47	8.439	2297	2301	2305	rBV4	532	480	0.01%	0.002%
48	8.625	2356	2359	2362	rBV	377	269	0.01%	0.001%
49	8.735	2389	2393	2396	rBV2	491	356	0.01%	0.001%
50	8.780	2396	2407	2445	rBV2	1902924	3461108	73.67%	14.361%
51	9.066	2494	2496	2499	rBV2	433	240	0.01%	0.001%
52	9.088	2500	2503	2504	rBV2	1129	560	0.01%	0.002%
53	9.159	2520	2525	2526	rBV	433	423	0.01%	0.002%
54	9.223	2543	2545	2550	rVB3	423	275	0.01%	0.001%
55	9.301	2566	2569	2572	rBV3	402	337	0.01%	0.001%
56	9.407	2600	2602	2605	rBV2	456	273	0.01%	0.001%
57	9.493	2621	2629	2633	rBV4	1268	1592	0.03%	0.007%
58	9.574	2650	2654	2656	rBV	301	268	0.01%	0.001%
59	9.677	2682	2686	2692	rBV3	366	406	0.01%	0.002%
60	9.870	2740	2746	2747	rBV3	969	763	0.02%	0.003%
61	9.937	2762	2767	2770	rBV2	300	266	0.01%	0.001%
62	10.030	2790	2796	2798	rBV2	299	288	0.01%	0.001%
63	10.063	2802	2806	2810	rVB2	400	306	0.01%	0.001%
64	10.085	2810	2813	2820	rBV2	353	306	0.01%	0.001%
65	10.149	2820	2833	2865	rBV	565943	890894	18.96%	3.697%
66	10.352	2893	2896	2900	rVB3	402	233	0.00%	0.001%
67	10.487	2928	2938	2949	rBV5	1035	1929	0.04%	0.008%
68	10.571	2961	2964	2967	rVB	534	263	0.01%	0.001%
69	10.789	3029	3032	3035	rVV2	345	306	0.01%	0.001%
70	10.815	3038	3040	3044	rVB2	419	268	0.01%	0.001%
71	10.863	3049	3055	3064	rVB2	1123	1537	0.03%	0.006%
72	11.030	3101	3107	3112	rBV2	402	427	0.01%	0.002%
73	11.120	3124	3135	3144	rBV	89039	144168	3.07%	0.598%
74	11.181	3144	3154	3186	rVB	1837749	3032779	64.55%	12.584%
75	11.516	3250	3258	3259	rBV5	2693	2707	0.06%	0.011%
76	11.574	3260	3276	3302	rVV2	2392094	4698198	100.00%	19.494%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035425.D
 Acq On : 26 Apr 2024 14:28
 Operator : SY/MD
 Sample : P2269-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	11.870	3362	3368	3369	rBV2	521	433	0.01%	0.002%
78	11.960	3394	3396	3401	rVB2	403	320	0.01%	0.001%
79	12.053	3420	3425	3426	rBV2	468	360	0.01%	0.001%
80	12.204	3469	3472	3477	rVB4	539	496	0.01%	0.002%
81	12.413	3533	3537	3541	rBV2	415	465	0.01%	0.002%
82	12.542	3571	3577	3580	rBV3	611	649	0.01%	0.003%
83	12.580	3580	3589	3608	rBV	32981	65172	1.39%	0.270%
84	12.689	3616	3623	3628	rVV5	2532	3285	0.07%	0.014%
85	13.136	3759	3762	3765	rBV3	375	275	0.01%	0.001%
86	13.197	3769	3781	3810	rVV	469077	743536	15.83%	3.085%
87	13.403	3843	3845	3849	rVB3	480	307	0.01%	0.001%
88	13.448	3849	3859	3874	rBV	8667	14912	0.32%	0.062%
89	13.680	3919	3931	3950	rBV	222729	358436	7.63%	1.487%
90	13.812	3969	3972	3974	rBV2	620	363	0.01%	0.002%
91	13.844	3979	3982	3984	rBV3	420	266	0.01%	0.001%
92	14.104	4052	4063	4071	rBV8	5865	12084	0.26%	0.050%
93	14.162	4078	4081	4082	rBV3	517	281	0.01%	0.001%
94	14.484	4178	4181	4182	rBV2	580	310	0.01%	0.001%
95	14.603	4215	4218	4221	rBV2	397	271	0.01%	0.001%
96	14.722	4252	4255	4257	rBV2	640	385	0.01%	0.002%
97	14.760	4257	4267	4279	rVB3	7299	11213	0.24%	0.047%
98	15.210	4405	4407	4410	rVB2	709	290	0.01%	0.001%
99	15.336	4437	4446	4460	rBV3	20695	33336	0.71%	0.138%
100	15.461	4483	4485	4488	rVB4	1083	543	0.01%	0.002%




Sum of corrected areas: 24100755

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035425.D
Acq On : 26 Apr 2024 14:28
Operator : SY/MD
Sample : P2269-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

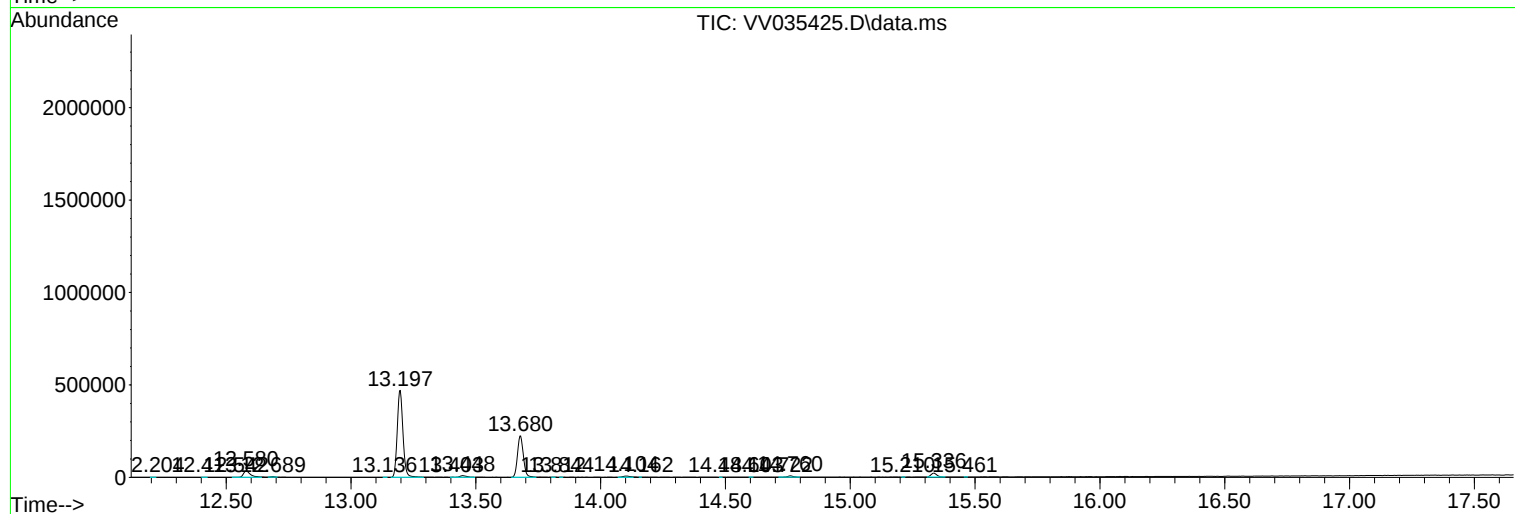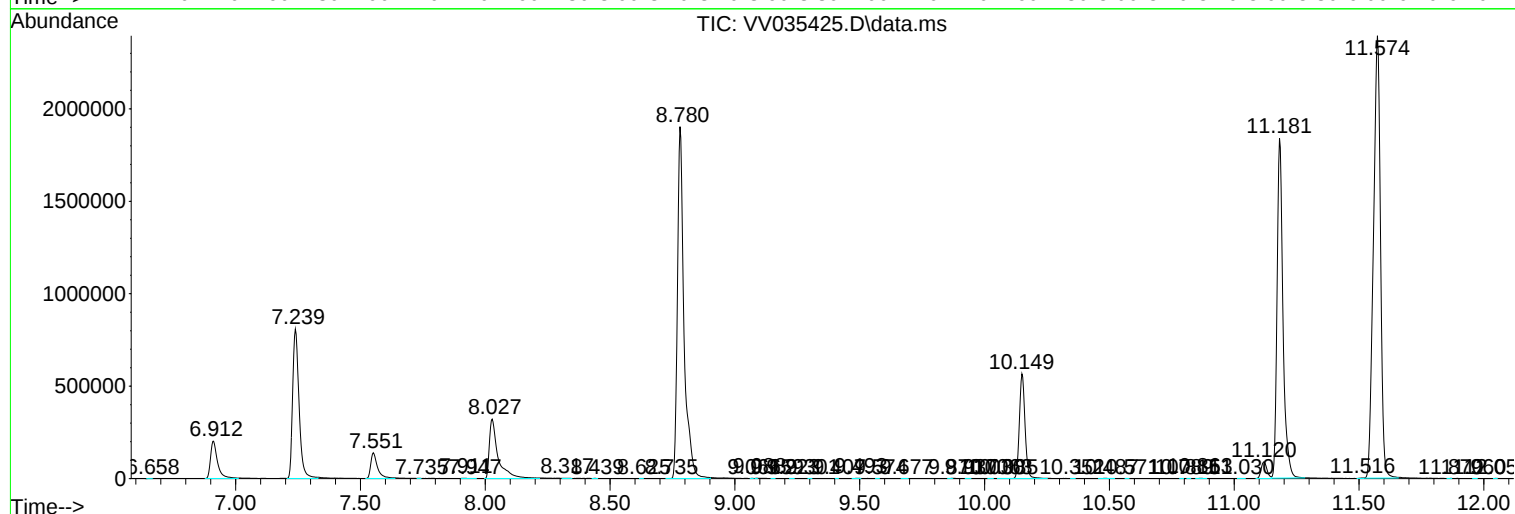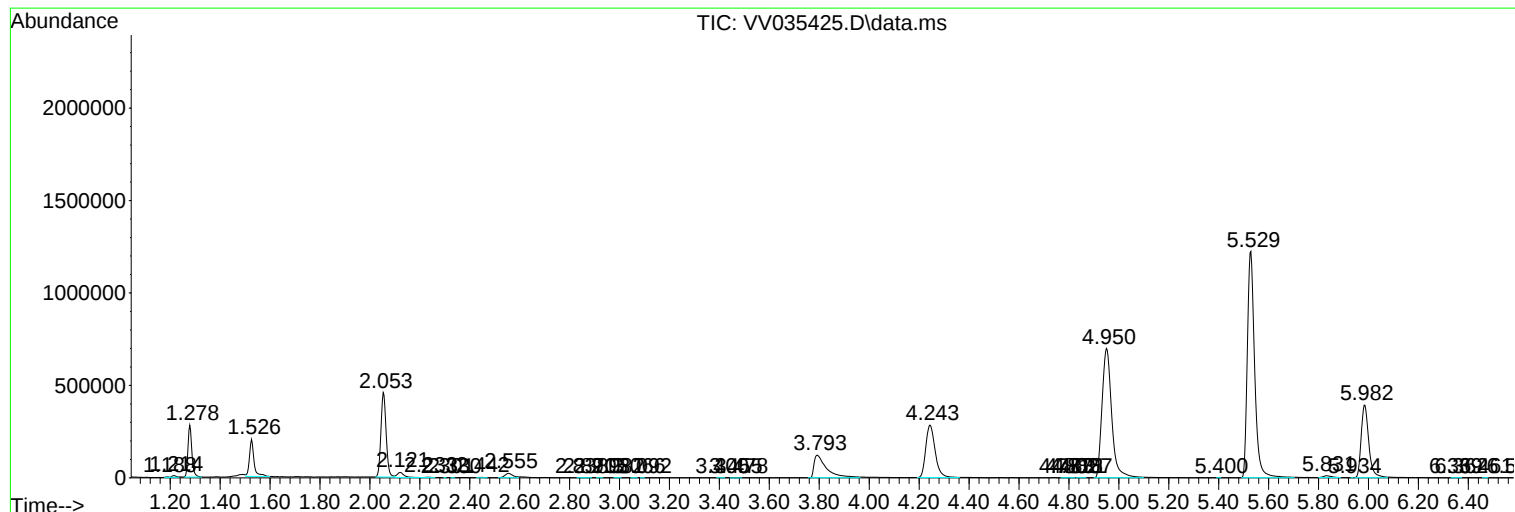

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035425.D
Acq On : 26 Apr 2024 14:28
Operator : SY/MD
Sample : P2269-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035425.D
Acq On : 26 Apr 2024 14:28
Operator : SY/MD
Sample : P2269-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RP7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------