

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035426.D
 Acq On : 26 Apr 2024 14:53
 Operator : SY/MD
 Sample : P2269-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035426.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rVB	271436	290317	16.03%	2.090%
2	1.526	145	151	165	rVB	206969	249693	13.79%	1.797%
3	2.056	306	316	331	rBV	436758	634912	35.07%	4.571%
4	2.555	458	471	504	rBV2	23187	59910	3.31%	0.431%
5	2.706	512	518	520	rBV2	389	496	0.03%	0.004%
6	2.815	548	552	555	rBV3	407	289	0.02%	0.002%
7	2.851	560	563	566	rBV	264	219	0.01%	0.002%
8	2.896	574	577	579	rBV	299	197	0.01%	0.001%
9	2.934	587	589	593	rBV3	235	225	0.01%	0.002%
10	3.011	609	613	614	rBV2	212	133	0.01%	0.001%
11	3.069	627	631	635	rVB2	193	208	0.01%	0.001%
12	3.156	654	658	659	rBV2	208	102	0.01%	0.001%
13	3.191	666	669	673	rBV	330	304	0.02%	0.002%
14	3.323	708	710	713	rVB2	252	125	0.01%	0.001%
15	3.343	713	716	720	rBV2	165	111	0.01%	0.001%
16	3.372	722	725	732	rVB3	340	345	0.02%	0.002%
17	3.410	732	737	740	rBV3	316	290	0.02%	0.002%
18	3.426	740	742	745	rBV	238	114	0.01%	0.001%
19	3.442	745	747	751	rVV2	149	124	0.01%	0.001%
20	3.484	759	760	764	rBV2	214	113	0.01%	0.001%
21	3.558	780	783	784	rBV2	201	111	0.01%	0.001%
22	3.568	784	786	788	rVV2	224	106	0.01%	0.001%
23	3.680	818	821	824	rBV2	208	168	0.01%	0.001%
24	3.725	834	835	839	rVB	242	117	0.01%	0.001%
25	3.744	839	841	843	rBV	201	104	0.01%	0.001%
26	3.790	843	855	904	rBV2	126690	432120	23.87%	3.111%
27	4.246	982	997	1031	rBV	283492	736128	40.66%	5.299%
28	4.738	1145	1150	1152	rBV3	368	303	0.02%	0.002%
29	4.806	1168	1171	1172	rBV	314	169	0.01%	0.001%
30	4.953	1201	1217	1250	rBV2	690397	1810544	100.00%	13.034%
31	5.269	1314	1315	1316	rBV	379	120	0.01%	0.001%
32	5.532	1386	1397	1430	rBV	566717	1182607	65.32%	8.513%
33	5.934	1520	1522	1525	rVB2	522	251	0.01%	0.002%
34	5.986	1525	1538	1574	rBV	390865	815737	45.05%	5.872%
35	6.320	1640	1642	1643	rBV2	388	104	0.01%	0.001%
36	6.371	1655	1658	1659	rBV	267	136	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035426.D
 Acq On : 26 Apr 2024 14:53
 Operator : SY/MD
 Sample : P2269-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.400	1663	1667	1669	rBV2	577	373	0.02%	0.003%
38	6.436	1675	1678	1682	rBV3	365	317	0.02%	0.002%
39	6.458	1682	1685	1688	rBV	322	238	0.01%	0.002%
40	6.500	1697	1698	1700	rVB	249	89	0.00%	0.001%
41	6.513	1700	1702	1703	rBV	201	100	0.01%	0.001%
42	6.551	1710	1714	1718	rBV2	371	334	0.02%	0.002%
43	6.593	1723	1727	1728	rBV	200	121	0.01%	0.001%
44	6.600	1728	1729	1732	rBV	240	126	0.01%	0.001%
45	6.651	1743	1745	1747	rVB	377	141	0.01%	0.001%
46	6.686	1754	1756	1757	rBV	285	97	0.01%	0.001%
47	6.738	1769	1772	1774	rBV2	194	134	0.01%	0.001%
48	6.783	1784	1786	1790	rBV	335	159	0.01%	0.001%
49	6.802	1790	1792	1794	rVV	244	139	0.01%	0.001%
50	6.912	1815	1826	1858	rBV	196781	379729	20.97%	2.734%
51	7.195	1911	1914	1917	rBV2	457	309	0.02%	0.002%
52	7.240	1917	1928	1957	rBV	771409	1390682	76.81%	10.011%
53	7.551	2016	2025	2050	rBV	134805	251575	13.89%	1.811%
54	7.844	2113	2116	2117	rBV3	328	163	0.01%	0.001%
55	7.879	2125	2127	2129	rVB2	328	146	0.01%	0.001%
56	7.940	2142	2146	2147	rBV	379	237	0.01%	0.002%
57	7.969	2151	2155	2161	rBV4	468	436	0.02%	0.003%
58	8.027	2163	2173	2219	rBV2	308892	743543	41.07%	5.353%
59	8.452	2300	2305	2307	rBV2	646	529	0.03%	0.004%
60	8.532	2328	2330	2331	rBV	323	112	0.01%	0.001%
61	8.783	2396	2408	2445	rBV	865051	1441879	79.64%	10.380%
62	9.342	2577	2582	2584	rBV	238	219	0.01%	0.002%
63	9.352	2584	2585	2587	rBV	276	131	0.01%	0.001%
64	9.439	2608	2612	2613	rBV2	312	209	0.01%	0.002%
65	9.564	2649	2651	2653	rBV2	197	86	0.00%	0.001%
66	9.587	2653	2658	2660	rBV	180	173	0.01%	0.001%
67	9.632	2669	2672	2675	rVB2	223	108	0.01%	0.001%
68	9.651	2675	2678	2679	rBV	271	105	0.01%	0.001%
69	9.683	2685	2688	2691	rVB2	372	268	0.01%	0.002%
70	9.709	2691	2696	2697	rBV2	371	210	0.01%	0.002%
71	9.828	2729	2733	2734	rBV2	215	151	0.01%	0.001%
72	9.873	2744	2747	2749	rBV2	321	183	0.01%	0.001%
73	10.034	2794	2797	2799	rVB	201	108	0.01%	0.001%
74	10.059	2803	2805	2808	rVB	289	142	0.01%	0.001%
75	10.149	2821	2833	2862	rBV	550652	868497	47.97%	6.252%
76	10.365	2898	2900	2908	rVB4	455	480	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035426.D
 Acq On : 26 Apr 2024 14:53
 Operator : SY/MD
 Sample : P2269-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RP9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	10.464	2929	2931	2932	rBV	208	90	0.00%	0.001%
78	10.577	2962	2966	2969	rBV2	157	113	0.01%	0.001%
79	10.770	3024	3026	3030	rVB2	326	193	0.01%	0.001%
80	10.792	3030	3033	3041	rBV4	337	358	0.02%	0.003%
81	10.863	3052	3055	3056	rBV	240	160	0.01%	0.001%
82	10.895	3062	3065	3068	rVB2	340	205	0.01%	0.001%
83	11.130	3130	3138	3144	rBV3	3036	4865	0.27%	0.035%
84	11.181	3144	3154	3189	rVV	784394	1240765	68.53%	8.932%
85	11.558	3259	3271	3301	rBV	741913	1242654	68.63%	8.946%
86	11.889	3372	3374	3376	rBV2	257	96	0.01%	0.001%
87	11.960	3394	3396	3400	rVB2	512	246	0.01%	0.002%
88	11.979	3400	3402	3405	rBV2	297	169	0.01%	0.001%
89	12.053	3422	3425	3426	rBV2	350	220	0.01%	0.002%
90	12.368	3520	3523	3524	rBV	320	186	0.01%	0.001%
91	12.529	3571	3573	3575	rBV	460	264	0.01%	0.002%
92	12.567	3583	3585	3587	rBV	275	187	0.01%	0.001%
93	12.596	3587	3594	3609	rVV7	1913	4636	0.26%	0.033%
94	12.918	3692	3694	3695	rBV7	339	159	0.01%	0.001%
95	12.985	3713	3715	3717	rBV2	353	215	0.01%	0.002%
96	13.088	3745	3747	3750	rBV2	353	195	0.01%	0.001%
97	13.162	3768	3770	3773	rBV2	369	190	0.01%	0.001%
98	13.201	3773	3782	3798	rBV2	32693	52484	2.90%	0.378%
99	13.448	3851	3859	3874	rBV2	4777	9262	0.51%	0.067%
100	13.683	3922	3932	3949	rBV2	20494	33474	1.85%	0.241%




Sum of corrected areas: 13891216

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035426.D
Acq On : 26 Apr 2024 14:53
Operator : SY/MD
Sample : P2269-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

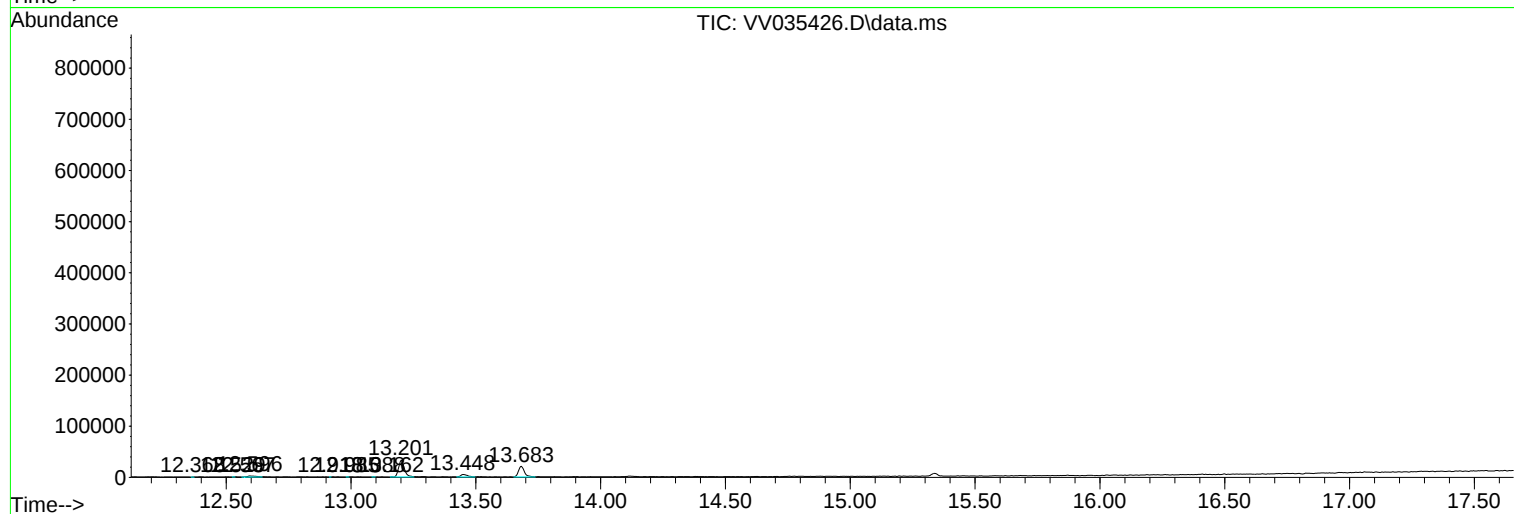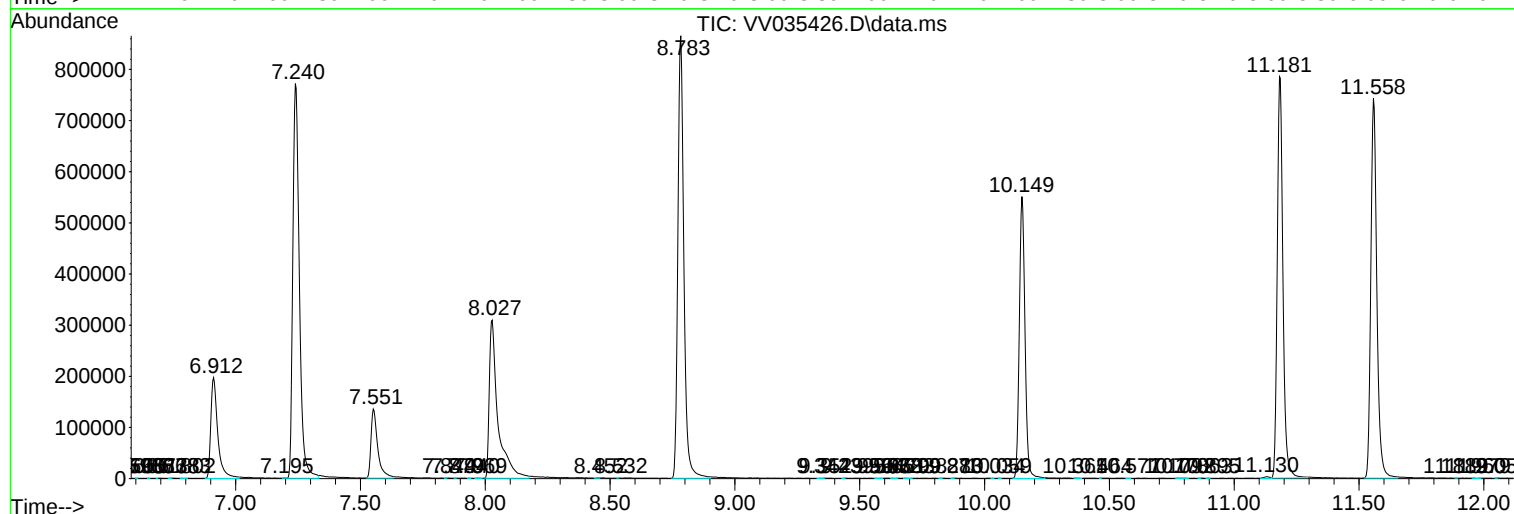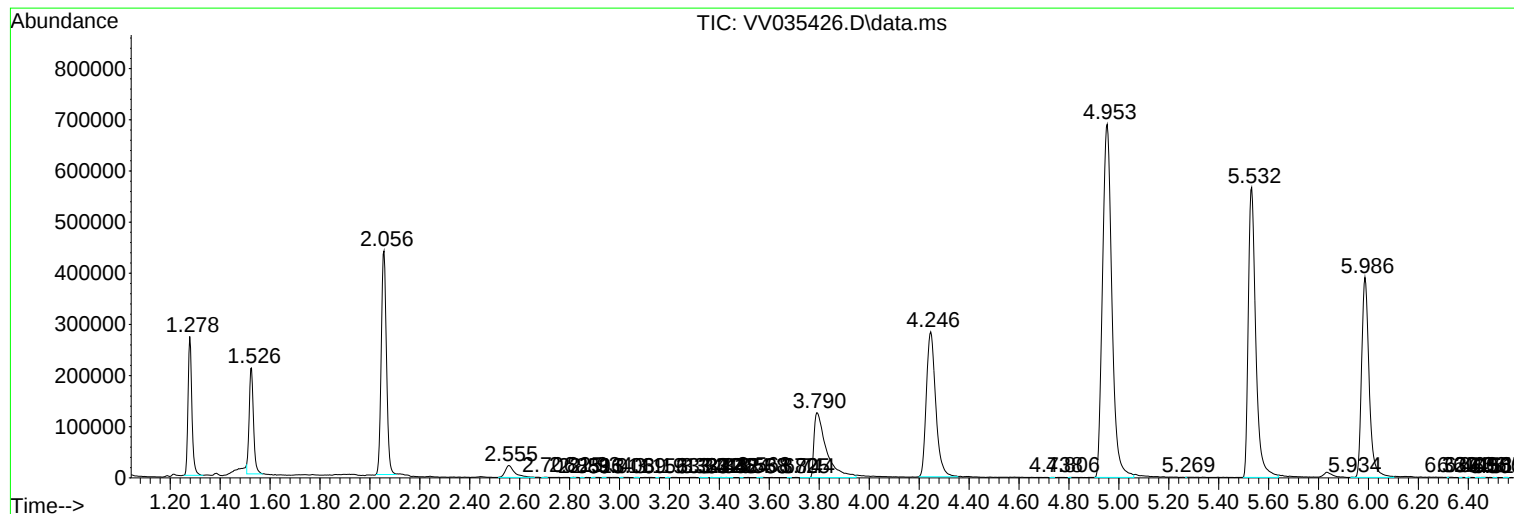

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035426.D
Acq On : 26 Apr 2024 14:53
Operator : SY/MD
Sample : P2269-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035426.D
Acq On : 26 Apr 2024 14:53
Operator : SY/MD
Sample : P2269-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RP9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------