

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035427.D
 Acq On : 26 Apr 2024 15:16
 Operator : SY/MD
 Sample : P2269-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rBV	271205	294788	16.39%	2.152%
2	1.526	145	151	175	rVB	214284	274173	15.24%	2.001%
3	2.056	306	316	332	rBV	440326	637582	35.45%	4.653%
4	2.558	458	472	506	rBV	25417	68956	3.83%	0.503%
5	2.732	523	526	528	rBV2	407	312	0.02%	0.002%
6	2.783	538	542	546	rBV3	291	269	0.01%	0.002%
7	2.860	562	566	567	rBV	220	147	0.01%	0.001%
8	2.934	587	589	594	rVB3	251	171	0.01%	0.001%
9	2.960	594	597	598	rBV	224	121	0.01%	0.001%
10	3.031	616	619	622	rBV2	191	172	0.01%	0.001%
11	3.098	637	640	643	rBV2	168	154	0.01%	0.001%
12	3.133	648	651	652	rBV	159	88	0.00%	0.001%
13	3.195	662	670	676	rBV3	309	548	0.03%	0.004%
14	3.230	678	681	684	rVV2	166	94	0.01%	0.001%
15	3.281	695	697	698	rBV2	121	52	0.00%	0.000%
16	3.342	711	716	719	rBV2	178	191	0.01%	0.001%
17	3.368	722	724	727	rVB2	330	206	0.01%	0.002%
18	3.500	762	765	768	rBV2	198	168	0.01%	0.001%
19	3.519	768	771	776	rVB2	370	310	0.02%	0.002%
20	3.555	776	782	785	rBV2	267	224	0.01%	0.002%
21	3.635	797	807	809	rBV2	288	441	0.02%	0.003%
22	3.680	815	821	823	rBV2	220	156	0.01%	0.001%
23	3.696	824	826	829	rVV2	243	130	0.01%	0.001%
24	3.722	832	834	836	rBV	135	81	0.00%	0.001%
25	3.796	844	857	909	rBV2	125147	444032	24.69%	3.241%
26	4.246	981	997	1032	rBV	278836	718852	39.97%	5.247%
27	4.793	1166	1167	1170	rBV	276	137	0.01%	0.001%
28	4.953	1201	1217	1263	rBV2	684280	1798620	100.00%	13.128%
29	5.471	1375	1378	1380	rBV2	385	232	0.01%	0.002%
30	5.532	1386	1397	1434	rBV	562570	1181496	65.69%	8.623%
31	5.940	1521	1524	1526	rBV2	434	279	0.02%	0.002%
32	5.985	1526	1538	1570	rVV	379529	796875	44.30%	5.816%
33	6.310	1636	1639	1641	rBV2	376	219	0.01%	0.002%
34	6.365	1654	1656	1658	rVB2	366	97	0.01%	0.001%
35	6.374	1658	1659	1661	rVB	383	128	0.01%	0.001%
36	6.464	1685	1687	1689	rVB2	172	74	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035427.D
 Acq On : 26 Apr 2024 15:16
 Operator : SY/MD
 Sample : P2269-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.487	1689	1694	1695	rBV2	326	216	0.01%	0.002%
38	6.497	1695	1697	1701	rVB2	357	199	0.01%	0.001%
39	6.590	1724	1726	1727	rBV	155	42	0.00%	0.000%
40	6.661	1743	1748	1752	rBV2	342	245	0.01%	0.002%
41	6.693	1756	1758	1759	rVV2	168	56	0.00%	0.000%
42	6.702	1759	1761	1766	rVB	369	240	0.01%	0.002%
43	6.728	1766	1769	1772	rBV	177	95	0.01%	0.001%
44	6.757	1775	1778	1779	rBV	203	87	0.00%	0.001%
45	6.805	1790	1793	1796	rBV2	95	55	0.00%	0.000%
46	6.821	1796	1798	1801	rVB2	155	82	0.00%	0.001%
47	6.847	1801	1806	1807	rBV2	116	107	0.01%	0.001%
48	6.857	1807	1809	1811	rBV2	199	114	0.01%	0.001%
49	6.911	1816	1826	1855	rBV	193168	373461	20.76%	2.726%
50	7.239	1917	1928	1964	rBV	774287	1383571	76.92%	10.098%
51	7.551	2016	2025	2058	rBV	129555	249580	13.88%	1.822%
52	7.844	2111	2116	2119	rBV2	425	394	0.02%	0.003%
53	7.915	2135	2138	2142	rVB3	619	470	0.03%	0.003%
54	7.966	2152	2154	2156	rVB2	156	66	0.00%	0.000%
55	7.982	2156	2159	2164	rBV4	369	440	0.02%	0.003%
56	8.027	2164	2173	2222	rBV2	310588	747338	41.55%	5.455%
57	8.577	2342	2344	2345	rBV2	381	125	0.01%	0.001%
58	8.628	2358	2360	2362	rBV	385	194	0.01%	0.001%
59	8.673	2371	2374	2376	rBV	325	212	0.01%	0.002%
60	8.741	2393	2395	2396	rBV	165	62	0.00%	0.000%
61	8.783	2396	2408	2438	rBV	862014	1435462	79.81%	10.477%
62	9.217	2540	2543	2547	rVB	443	314	0.02%	0.002%
63	9.252	2552	2554	2558	rVB2	405	221	0.01%	0.002%
64	9.278	2558	2562	2565	rBV4	455	413	0.02%	0.003%
65	9.310	2569	2572	2574	rBV	208	141	0.01%	0.001%
66	9.320	2574	2575	2577	rVV	276	114	0.01%	0.001%
67	9.333	2577	2579	2582	rVB	297	139	0.01%	0.001%
68	9.451	2614	2616	2619	rBV	301	198	0.01%	0.001%
69	9.484	2624	2626	2628	rBV	152	58	0.00%	0.000%
70	9.500	2628	2631	2633	rBV	218	133	0.01%	0.001%
71	9.587	2656	2658	2661	rBV	175	102	0.01%	0.001%
72	9.606	2661	2664	2669	rVB2	381	210	0.01%	0.002%
73	9.657	2676	2680	2682	rBV	304	221	0.01%	0.002%
74	9.847	2736	2739	2744	rVB2	438	337	0.02%	0.002%
75	9.882	2744	2750	2755	rBV3	563	600	0.03%	0.004%
76	10.107	2818	2820	2822	rBV2	335	210	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035427.D
 Acq On : 26 Apr 2024 15:16
 Operator : SY/MD
 Sample : P2269-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M

Title : VOC Analysis

77	10.149	2822	2833	2864	rVV	546244	862826	47.97%	6.297%
78	10.673	2994	2996	2997	rVB	258	75	0.00%	0.001%
79	10.741	3014	3017	3019	rBV	376	255	0.01%	0.002%
80	10.795	3029	3034	3039	rBV5	539	528	0.03%	0.004%
81	10.869	3055	3057	3058	rBV	369	164	0.01%	0.001%
82	10.918	3070	3072	3077	rVB2	348	187	0.01%	0.001%
83	10.972	3088	3089	3091	rBV	220	78	0.00%	0.001%
84	11.043	3109	3111	3113	rVB	286	94	0.01%	0.001%
85	11.127	3133	3137	3139	rBV3	1071	907	0.05%	0.007%
86	11.181	3144	3154	3178	rBV	757927	1213117	67.45%	8.854%
87	11.467	3239	3243	3247	rBV3	608	517	0.03%	0.004%
88	11.558	3259	3271	3305	rBV	743638	1179203	65.56%	8.607%
89	11.828	3353	3355	3357	rBV2	396	160	0.01%	0.001%
90	11.905	3377	3379	3382	rBV2	371	244	0.01%	0.002%
91	12.024	3414	3416	3418	rBV	422	272	0.02%	0.002%
92	12.197	3464	3470	3471	rBV2	378	446	0.02%	0.003%
93	12.377	3523	3526	3527	rBV	271	131	0.01%	0.001%
94	12.586	3588	3591	3592	rBV2	710	371	0.02%	0.003%
95	12.696	3621	3625	3629	rBV2	467	466	0.03%	0.003%
96	12.972	3707	3711	3714	rBV2	532	496	0.03%	0.004%
97	13.204	3776	3783	3796	rBV4	6454	10946	0.61%	0.080%
98	13.313	3813	3817	3821	rBV3	442	496	0.03%	0.004%
99	13.451	3854	3860	3873	rBV2	2479	4857	0.27%	0.035%
100	13.680	3926	3931	3945	rVB4	4131	7420	0.41%	0.054%




Sum of corrected areas: 13701155

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035427.D
Acq On : 26 Apr 2024 15:16
Operator : SY/MD
Sample : P2269-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

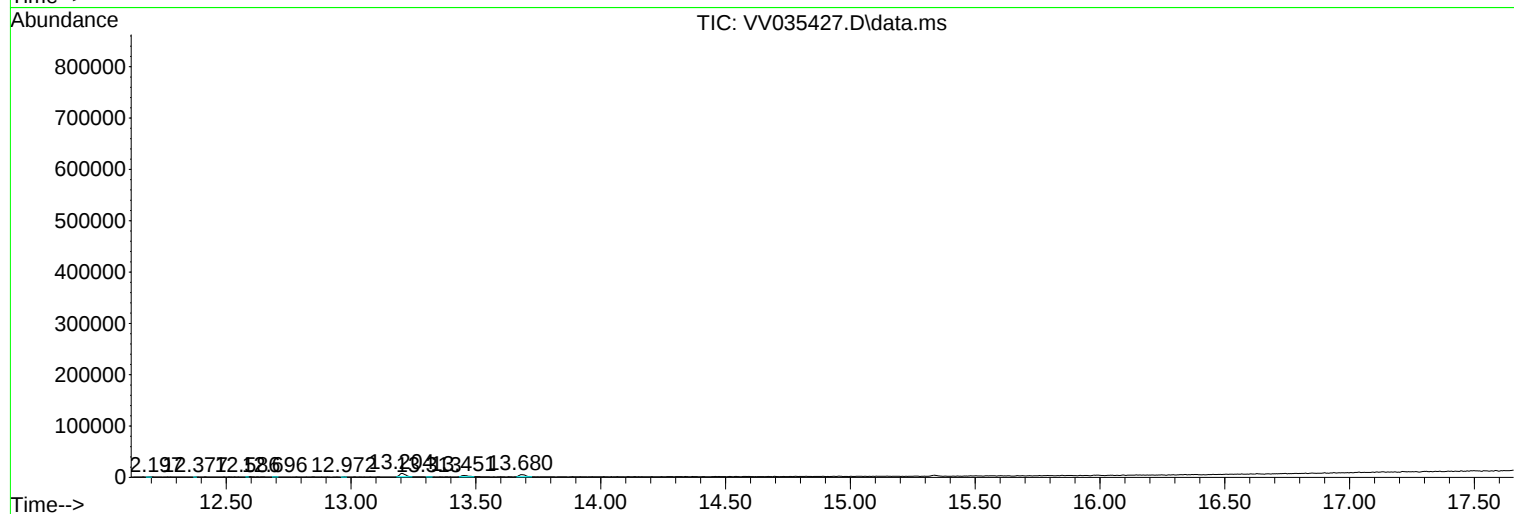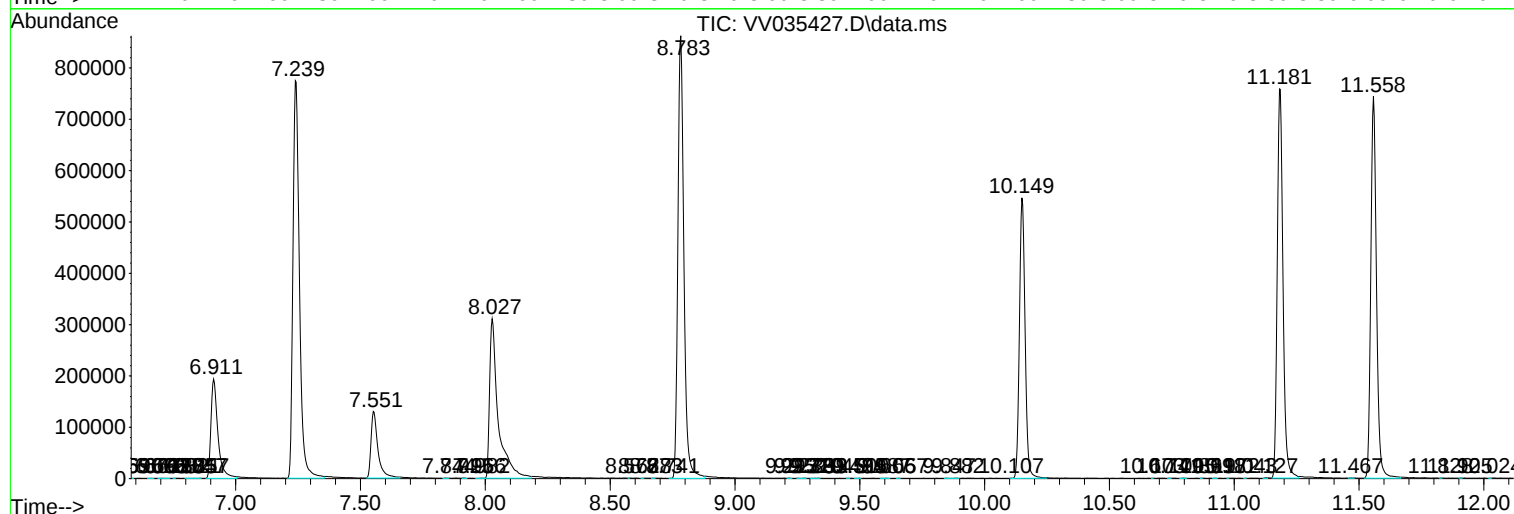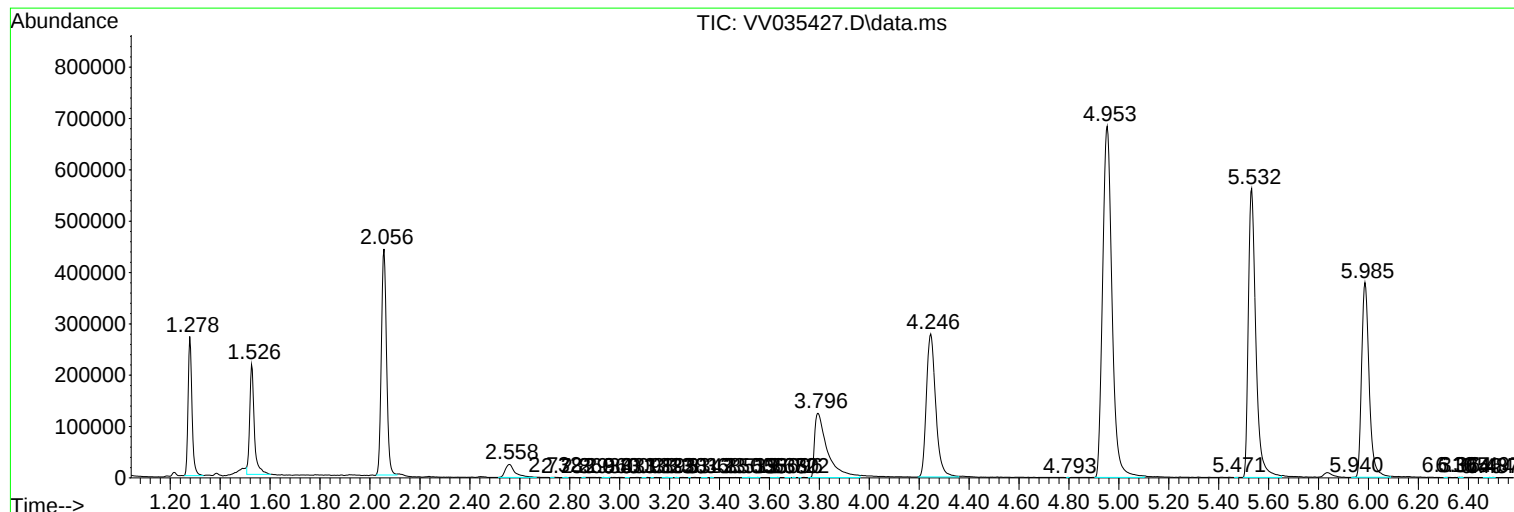

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035427.D
Acq On : 26 Apr 2024 15:16
Operator : SY/MD
Sample : P2269-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035427.D
Acq On : 26 Apr 2024 15:16
Operator : SY/MD
Sample : P2269-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc