

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035428.D
 Acq On : 26 Apr 2024 15:40
 Operator : SY/MD
 Sample : P2269-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035428.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	269490	292025	16.27%	2.124%
2	1.532	146	153	168	rBV	231702	272008	15.15%	1.979%
3	2.056	306	316	333	rBV	441820	640754	35.69%	4.661%
4	2.397	420	422	423	rBV	468	192	0.01%	0.001%
5	2.449	432	438	446	rVB4	1408	1990	0.11%	0.014%
6	2.558	458	472	484	rBV	19750	43947	2.45%	0.320%
7	2.777	538	540	541	rBV	217	103	0.01%	0.001%
8	2.789	541	544	546	rVV2	313	199	0.01%	0.001%
9	2.908	579	581	584	rVB2	261	122	0.01%	0.001%
10	3.024	614	617	619	rBV2	247	160	0.01%	0.001%
11	3.092	633	638	645	rVB3	360	333	0.02%	0.002%
12	3.172	656	663	665	rBV	264	263	0.01%	0.002%
13	3.223	676	679	683	rBV2	232	131	0.01%	0.001%
14	3.252	683	688	692	rVV2	314	299	0.02%	0.002%
15	3.297	699	702	703	rBV	241	108	0.01%	0.001%
16	3.407	732	736	738	rBV2	266	195	0.01%	0.001%
17	3.439	743	746	751	rVV3	234	212	0.01%	0.002%
18	3.481	757	759	763	rVB	430	226	0.01%	0.002%
19	3.503	763	766	767	rBV	183	70	0.00%	0.001%
20	3.580	787	790	794	rBV2	227	179	0.01%	0.001%
21	3.625	802	804	807	rVB2	214	108	0.01%	0.001%
22	3.648	807	811	814	rVB2	154	109	0.01%	0.001%
23	3.667	814	817	819	rBV	150	108	0.01%	0.001%
24	3.725	832	835	837	rVB2	128	72	0.00%	0.001%
25	3.799	839	858	905	rBV2	122085	451256	25.14%	3.283%
26	4.246	983	997	1036	rVB	278806	716816	39.93%	5.214%
27	4.686	1131	1134	1136	rBV2	277	178	0.01%	0.001%
28	4.764	1156	1158	1161	rBV3	309	196	0.01%	0.001%
29	4.818	1171	1175	1176	rBV3	433	310	0.02%	0.002%
30	4.953	1201	1217	1262	rBV2	685358	1795190	100.00%	13.059%
31	5.358	1341	1343	1346	rBV4	503	330	0.02%	0.002%
32	5.429	1363	1365	1366	rBV2	262	146	0.01%	0.001%
33	5.532	1385	1397	1430	rBV	576447	1204308	67.09%	8.761%
34	5.985	1526	1538	1577	rBV	383306	799962	44.56%	5.819%
35	6.288	1629	1632	1634	rBV	399	235	0.01%	0.002%
36	6.329	1643	1645	1651	rVB2	310	273	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035428.D
 Acq On : 26 Apr 2024 15:40
 Operator : SY/MD
 Sample : P2269-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.355	1651	1653	1658	rVB4	438	326	0.02%	0.002%
38	6.384	1658	1662	1664	rBV	299	221	0.01%	0.002%
39	6.442	1675	1680	1682	rBV3	266	251	0.01%	0.002%
40	6.477	1689	1691	1695	rVB3	307	166	0.01%	0.001%
41	6.510	1697	1701	1706	rVB3	410	263	0.01%	0.002%
42	6.542	1709	1711	1712	rBV	196	63	0.00%	0.000%
43	6.680	1751	1754	1758	rBV2	419	337	0.02%	0.002%
44	6.722	1764	1767	1772	rVB2	154	125	0.01%	0.001%
45	6.744	1772	1774	1776	rBV	134	77	0.00%	0.001%
46	6.854	1806	1808	1811	rVB	215	121	0.01%	0.001%
47	6.911	1811	1826	1862	rBV	190619	374423	20.86%	2.724%
48	7.239	1917	1928	1961	rBV	761647	1381410	76.95%	10.049%
49	7.551	2016	2025	2060	rBV	130228	245866	13.70%	1.789%
50	7.815	2105	2107	2110	rBV	226	114	0.01%	0.001%
51	7.844	2115	2116	2119	rBV2	299	125	0.01%	0.001%
52	7.860	2119	2121	2123	rBV2	294	151	0.01%	0.001%
53	7.934	2142	2144	2147	rVB2	365	160	0.01%	0.001%
54	7.963	2151	2153	2154	rBV2	216	104	0.01%	0.001%
55	8.027	2164	2173	2230	rBV3	294991	755257	42.07%	5.494%
56	8.432	2297	2299	2303	rBV4	588	423	0.02%	0.003%
57	8.644	2363	2365	2366	rBV	361	163	0.01%	0.001%
58	8.699	2379	2382	2390	rVB3	306	318	0.02%	0.002%
59	8.783	2396	2408	2438	rBV	880667	1464792	81.60%	10.655%
60	9.146	2518	2521	2526	rVB3	495	361	0.02%	0.003%
61	9.275	2555	2561	2562	rBV2	502	503	0.03%	0.004%
62	9.336	2577	2580	2581	rBV2	223	127	0.01%	0.001%
63	9.378	2588	2593	2595	rBV2	234	162	0.01%	0.001%
64	9.390	2595	2597	2598	rBV	191	83	0.00%	0.001%
65	9.522	2636	2638	2641	rBV	344	186	0.01%	0.001%
66	9.561	2647	2650	2652	rBV	258	147	0.01%	0.001%
67	9.625	2668	2670	2675	rVB	185	135	0.01%	0.001%
68	9.651	2675	2678	2681	rBV2	279	186	0.01%	0.001%
69	9.792	2719	2722	2725	rBV2	316	209	0.01%	0.002%
70	9.834	2732	2735	2738	rVB2	217	108	0.01%	0.001%
71	9.940	2763	2768	2770	rBV2	336	270	0.02%	0.002%
72	10.017	2789	2792	2795	rBV2	293	219	0.01%	0.002%
73	10.066	2806	2807	2808	rBV2	123	39	0.00%	0.000%
74	10.149	2821	2833	2862	rBV	540843	857087	47.74%	6.235%
75	10.361	2895	2899	2900	rBV2	306	187	0.01%	0.001%
76	10.410	2911	2914	2918	rBV	277	135	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035428.D
 Acq On : 26 Apr 2024 15:40
 Operator : SY/MD
 Sample : P2269-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	10.509	2942	2945	2949	rBV	255	158	0.01%	0.001%
78	10.622	2973	2980	2981	rBV2	316	313	0.02%	0.002%
79	10.689	2999	3001	3004	rVB2	234	112	0.01%	0.001%
80	11.024	3102	3105	3108	rBV	274	150	0.01%	0.001%
81	11.040	3108	3110	3115	rBV2	213	215	0.01%	0.002%
82	11.133	3134	3139	3143	rBV3	897	1017	0.06%	0.007%
83	11.185	3143	3155	3189	rVV	784893	1254933	69.91%	9.129%
84	11.516	3251	3258	3259	rBV4	2556	2664	0.15%	0.019%
85	11.558	3260	3271	3296	rVV	738261	1171308	65.25%	8.520%
86	12.059	3425	3427	3430	rVB2	338	171	0.01%	0.001%
87	12.127	3447	3448	3449	rBB	86	45	0.00%	0.000%
88	12.278	3493	3495	3498	rBV	387	216	0.01%	0.002%
89	12.648	3607	3610	3613	rBV4	514	401	0.02%	0.003%
90	12.815	3660	3662	3663	rBV4	280	105	0.01%	0.001%
91	13.207	3777	3784	3794	rBV4	3659	5829	0.32%	0.042%
92	13.805	3967	3970	3972	rBV2	609	378	0.02%	0.003%
93	13.879	3989	3993	3995	rBV2	504	444	0.02%	0.003%

Sum of corrected areas: 13746972




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035428.D
Acq On : 26 Apr 2024 15:40
Operator : SY/MD
Sample : P2269-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

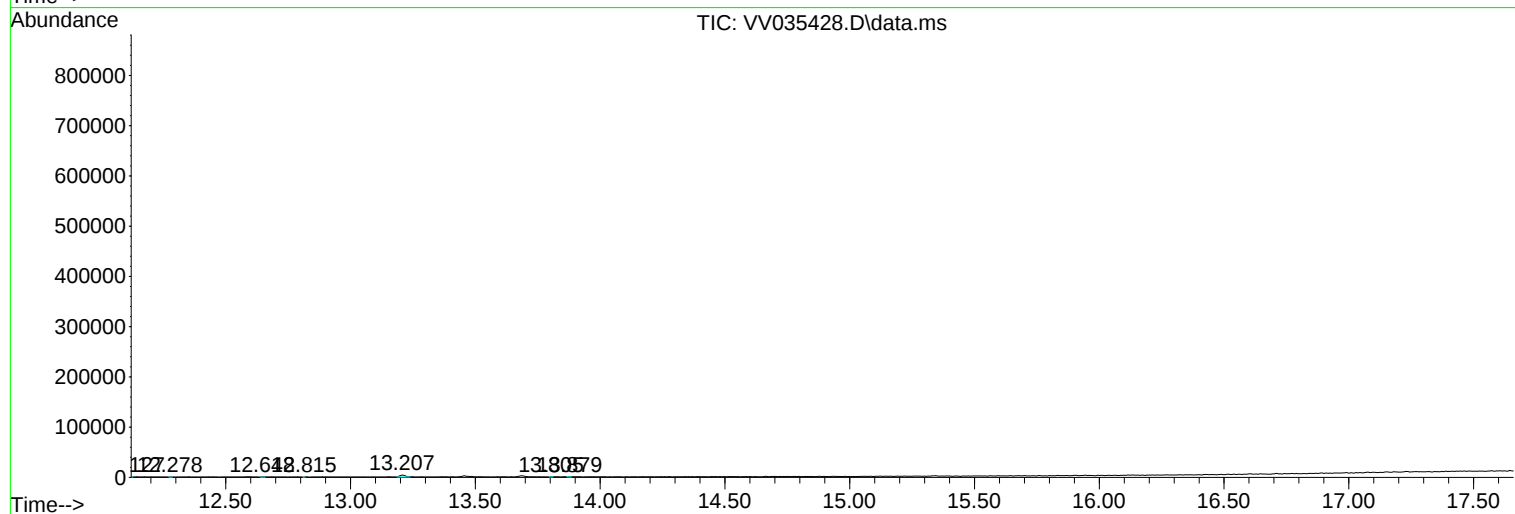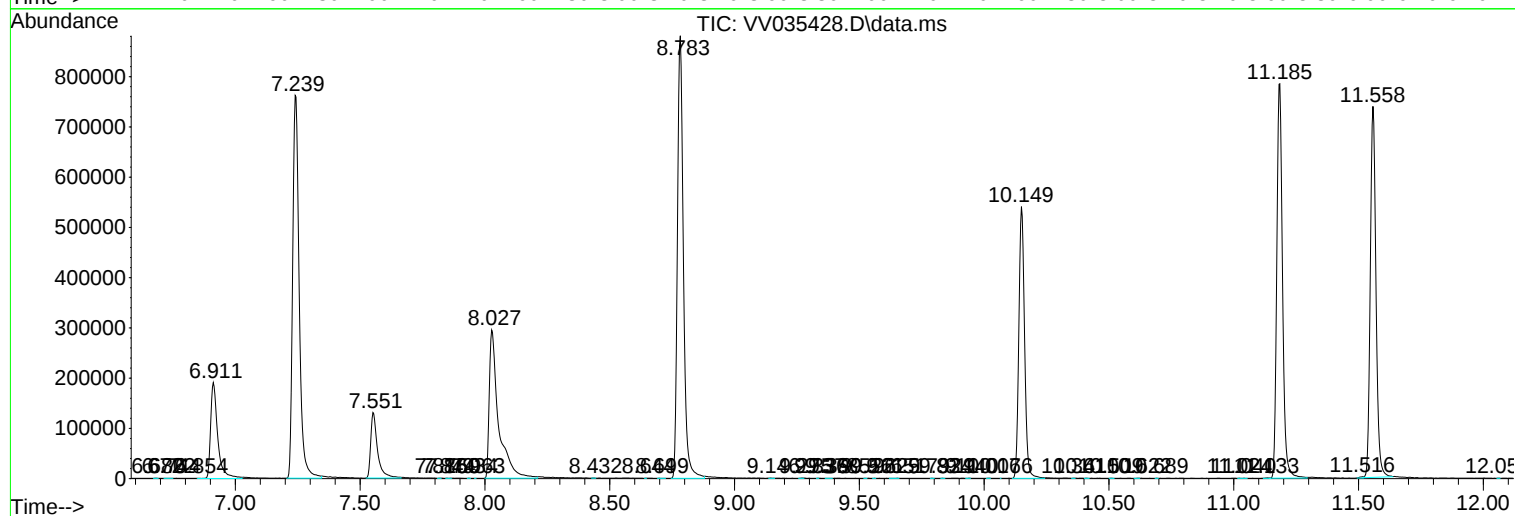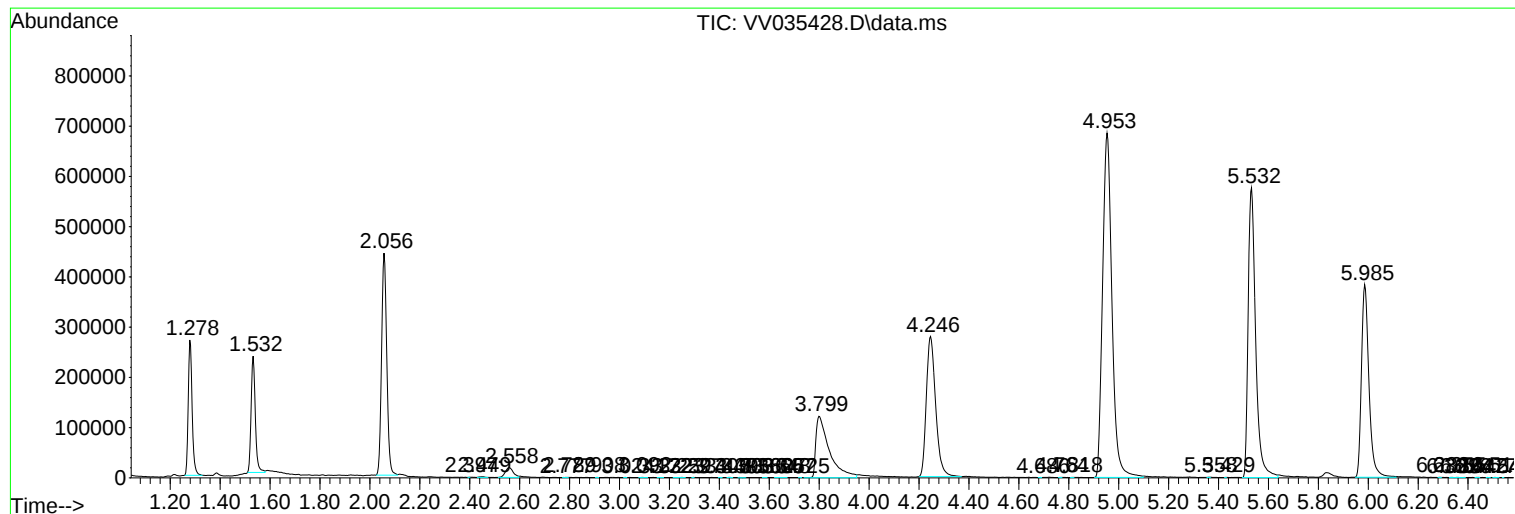

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035428.D
Acq On : 26 Apr 2024 15:40
Operator : SY/MD
Sample : P2269-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035428.D
Acq On : 26 Apr 2024 15:40
Operator : SY/MD
Sample : P2269-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------