

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035429.D
 Acq On : 26 Apr 2024 16:04
 Operator : SY/MD
 Sample : P2269-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M

Title : VOC Analysis

Signal : TIC: VV035429.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	42	46	50	rBV	2266	2246	0.02%	0.006%
2	1.214	51	54	58	rVV3	2262	2178	0.02%	0.006%
3	1.278	67	74	94	rVB	260567	284167	2.28%	0.740%
4	1.532	145	153	164	rBV	234604	269112	2.16%	0.701%
5	2.056	306	316	331	rBV	434830	627823	5.03%	1.634%
6	2.278	382	385	389	rVB2	327	279	0.00%	0.001%
7	2.449	429	438	445	rBV8	3285	5062	0.04%	0.013%
8	2.497	450	453	456	rBV2	536	390	0.00%	0.001%
9	2.513	456	458	464	rVB5	567	437	0.00%	0.001%
10	2.545	465	468	469	rBV	476	267	0.00%	0.001%
11	2.693	510	514	518	rVB2	465	419	0.00%	0.001%
12	3.092	633	638	641	rVV2	325	297	0.00%	0.001%
13	3.394	725	732	740	rBV2	462	539	0.00%	0.001%
14	3.497	761	764	767	rBV2	270	253	0.00%	0.001%
15	3.606	792	798	804	rBV2	326	354	0.00%	0.001%
16	3.667	806	817	821	rBV4	2187	3783	0.03%	0.010%
17	3.799	849	858	906	rBV	103561	350644	2.81%	0.913%
18	4.163	969	971	975	rBV2	319	289	0.00%	0.001%
19	4.246	982	997	1033	rBV	277245	713111	5.72%	1.856%
20	4.574	1097	1099	1102	rBV4	611	396	0.00%	0.001%
21	4.632	1113	1117	1120	rBV3	313	269	0.00%	0.001%
22	4.735	1137	1149	1160	rBV7	3675	8786	0.07%	0.023%
23	4.873	1188	1192	1199	rBV3	343	337	0.00%	0.001%
24	4.953	1201	1217	1226	rBV2	692432	1741001	13.96%	4.532%
25	5.320	1329	1331	1336	rBV4	578	502	0.00%	0.001%
26	5.404	1351	1357	1359	rVB4	463	465	0.00%	0.001%
27	5.532	1385	1397	1430	rBV	590276	1230382	9.86%	3.203%
28	5.767	1468	1470	1475	rVB	365	302	0.00%	0.001%
29	5.831	1481	1490	1507	rBV6	5702	12984	0.10%	0.034%
30	5.915	1513	1516	1520	rBV2	373	248	0.00%	0.001%
31	5.986	1525	1538	1567	rBV	381072	793637	6.36%	2.066%
32	6.211	1606	1608	1613	rVB4	775	448	0.00%	0.001%
33	6.240	1613	1617	1620	rBV3	504	461	0.00%	0.001%
34	6.413	1666	1671	1674	rBV2	472	399	0.00%	0.001%
35	6.429	1674	1676	1682	rVB2	386	317	0.00%	0.001%
36	6.677	1748	1753	1756	rBV2	335	268	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035429.D
 Acq On : 26 Apr 2024 16:04
 Operator : SY/MD
 Sample : P2269-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.818	1795	1797	1804	rVB2	317	264	0.00%	0.001%
38	6.912	1814	1826	1862	rBV	193487	377802	3.03%	0.984%
39	7.240	1914	1928	1968	rBV	792266	1401665	11.24%	3.649%
40	7.551	2014	2025	2054	rBV	131562	252668	2.03%	0.658%
41	7.805	2100	2104	2107	rBV2	510	348	0.00%	0.001%
42	7.825	2107	2110	2114	rVB2	608	481	0.00%	0.001%
43	7.876	2124	2126	2131	rVB2	375	305	0.00%	0.001%
44	7.902	2131	2134	2136	rBV2	523	401	0.00%	0.001%
45	8.027	2164	2173	2216	rBV2	316803	759062	6.09%	1.976%
46	8.561	2336	2339	2345	rVB4	555	618	0.00%	0.002%
47	8.677	2369	2375	2377	rBV3	281	313	0.00%	0.001%
48	8.809	2396	2416	2475	rBV2	6917397	12472570	100.00%	32.470%
49	9.294	2564	2567	2574	rBV4	533	456	0.00%	0.001%
50	9.522	2636	2638	2642	rVB3	627	340	0.00%	0.001%
51	9.706	2692	2695	2699	rVB3	407	302	0.00%	0.001%
52	9.731	2699	2703	2706	rBV2	428	293	0.00%	0.001%
53	9.838	2728	2736	2738	rBV2	320	374	0.00%	0.001%
54	9.850	2738	2740	2743	rVB2	549	288	0.00%	0.001%
55	9.873	2743	2747	2750	rBV2	500	417	0.00%	0.001%
56	9.911	2756	2759	2764	rVB2	304	270	0.00%	0.001%
57	9.944	2764	2769	2772	rBV	392	361	0.00%	0.001%
58	10.149	2821	2833	2866	rBV	556718	883520	7.08%	2.300%
59	10.329	2887	2889	2894	rVB4	468	288	0.00%	0.001%
60	10.381	2902	2905	2909	rVB2	762	510	0.00%	0.001%
61	10.416	2914	2916	2921	rVB3	378	305	0.00%	0.001%
62	10.455	2921	2928	2930	rBV3	254	312	0.00%	0.001%
63	10.490	2935	2939	2943	rVB2	469	356	0.00%	0.001%
64	10.548	2953	2957	2962	rVB2	288	316	0.00%	0.001%
65	10.789	3028	3032	3034	rBV2	426	311	0.00%	0.001%
66	10.953	3078	3083	3089	rVB3	409	472	0.00%	0.001%
67	11.043	3109	3111	3118	rVB3	303	312	0.00%	0.001%
68	11.114	3118	3133	3145	rBV	372849	591329	4.74%	1.539%
69	11.204	3145	3161	3193	rVB2	3490141	6677275	53.54%	17.383%
70	11.574	3259	3276	3308	rBV3	4480486	7800382	62.54%	20.307%
71	12.059	3422	3427	3429	rBV2	432	390	0.00%	0.001%
72	12.162	3455	3459	3462	rVB2	334	263	0.00%	0.001%
73	12.181	3462	3465	3467	rBV	374	271	0.00%	0.001%
74	12.355	3511	3519	3529	rVV7	2362	4187	0.03%	0.011%
75	12.526	3567	3572	3575	rBV3	611	541	0.00%	0.001%
76	12.596	3584	3594	3599	rBV8	1330	2437	0.02%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035429.D
 Acq On : 26 Apr 2024 16:04
 Operator : SY/MD
 Sample : P2269-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	12.693	3620	3624	3633	rVB4	1621	2263	0.02%	0.006%
78	12.767	3646	3647	3652	rVB2	436	282	0.00%	0.001%
79	12.831	3664	3667	3672	rBV5	540	457	0.00%	0.001%
80	12.944	3698	3702	3705	rBV2	385	313	0.00%	0.001%
81	12.985	3713	3715	3719	rVB2	390	261	0.00%	0.001%
82	13.066	3736	3740	3743	rBV2	295	249	0.00%	0.001%
83	13.091	3744	3748	3751	rVB4	533	444	0.00%	0.001%
84	13.143	3761	3764	3769	rVB3	431	393	0.00%	0.001%
85	13.194	3769	3780	3810	rBV	587618	921209	7.39%	2.398%
86	13.371	3831	3835	3839	rBV3	677	530	0.00%	0.001%
87	13.419	3846	3850	3851	rBV	405	262	0.00%	0.001%
88	13.448	3851	3859	3871	rVV6	2686	5085	0.04%	0.013%
89	13.558	3891	3893	3899	rVB4	518	391	0.00%	0.001%
90	13.680	3920	3931	3953	rBV	109367	179373	1.44%	0.467%
91	13.834	3977	3979	3984	rBV4	454	357	0.00%	0.001%
92	13.915	4001	4004	4006	rBV2	453	265	0.00%	0.001%
93	14.072	4050	4053	4055	rBV2	416	304	0.00%	0.001%
94	14.532	4194	4196	4199	rBV2	453	297	0.00%	0.001%
95	14.680	4239	4242	4244	rBV3	514	352	0.00%	0.001%
96	14.763	4264	4268	4277	rVB5	2823	3824	0.03%	0.010%
97	14.876	4297	4303	4307	rBV5	650	822	0.01%	0.002%
98	14.956	4325	4328	4331	rBV3	782	548	0.00%	0.001%
99	15.123	4377	4380	4382	rBV3	635	513	0.00%	0.001%
100	15.336	4441	4446	4460	rVB8	4173	7038	0.06%	0.018%




Sum of corrected areas: 38412059

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035429.D
Acq On : 26 Apr 2024 16:04
Operator : SY/MD
Sample : P2269-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

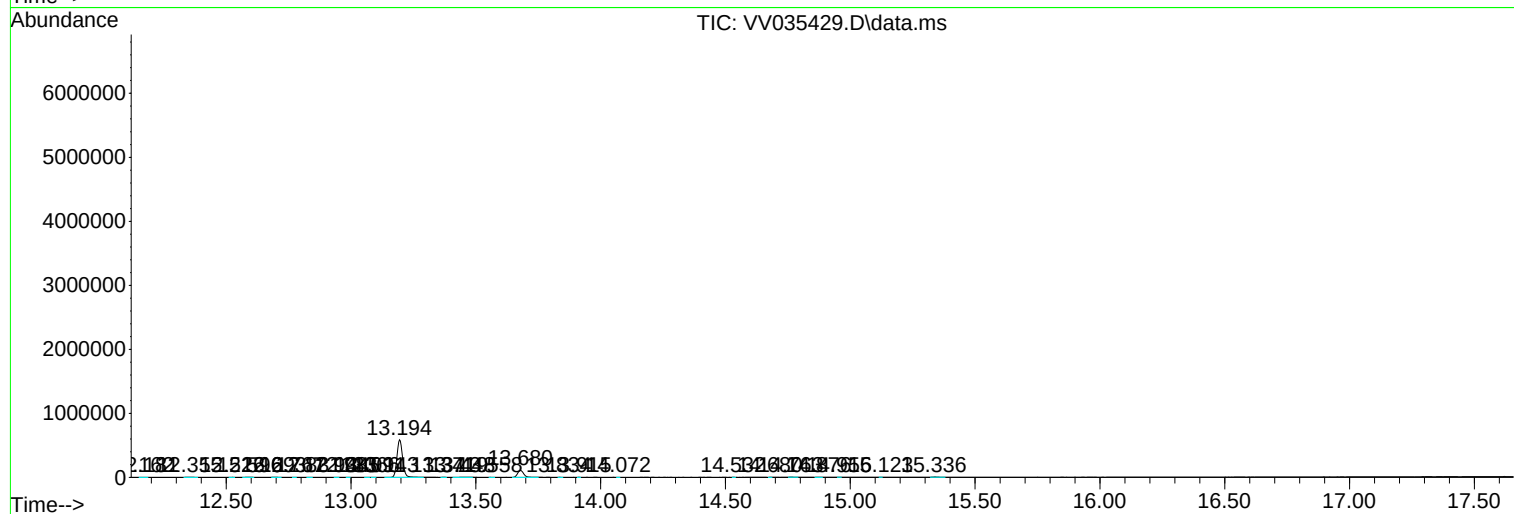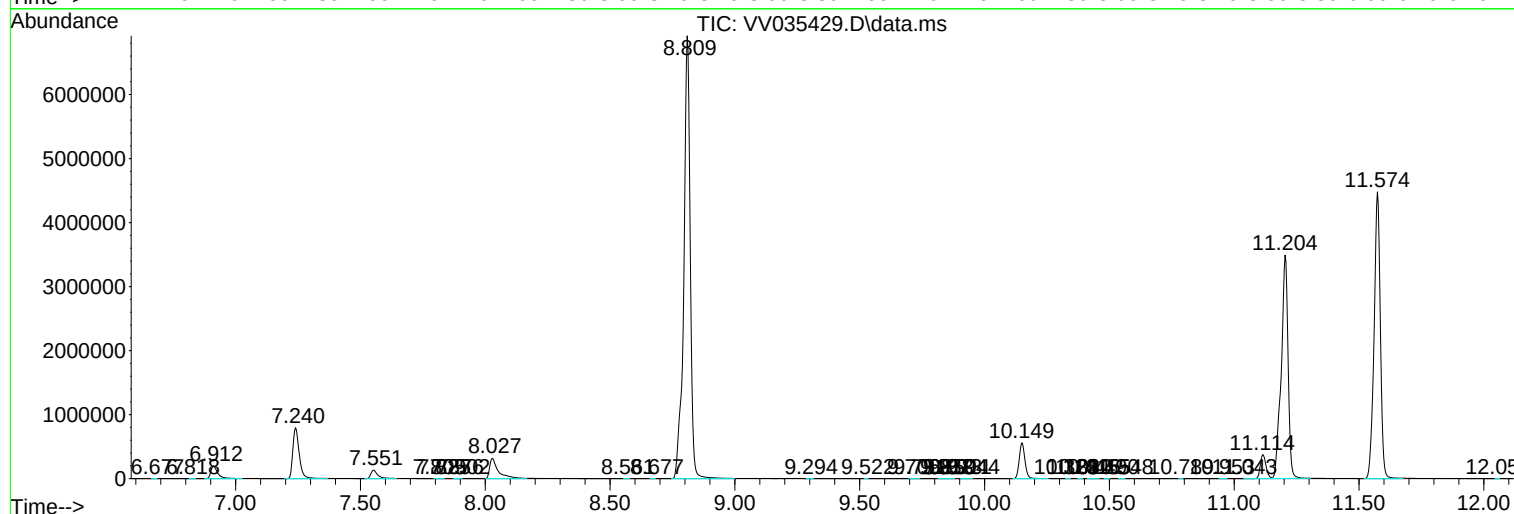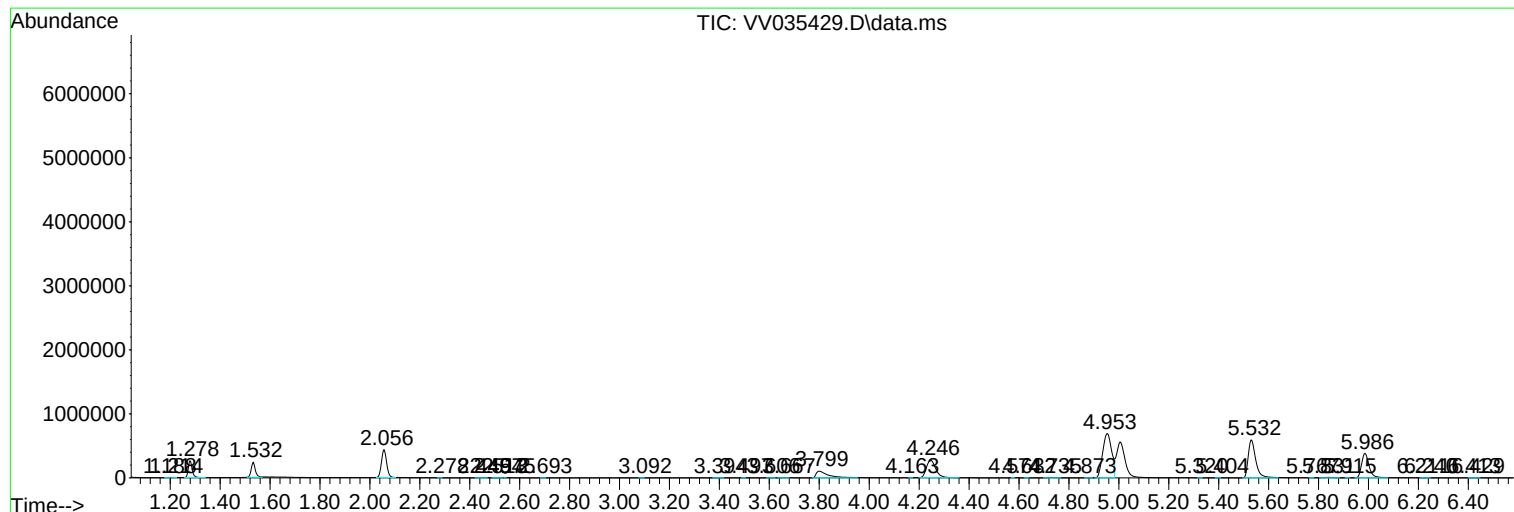

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035429.D
Acq On : 26 Apr 2024 16:04
Operator : SY/MD
Sample : P2269-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035429.D
Acq On : 26 Apr 2024 16:04
Operator : SY/MD
Sample : P2269-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
