

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035430.D
 Acq On : 26 Apr 2024 16:28
 Operator : SY/MD
 Sample : P2280-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08P7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035430.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.191	41	47	52	rBV2	22958	21660	1.18%	0.150%
2	1.281	68	75	93	rVB	274868	305030	16.58%	2.111%
3	1.532	146	153	166	rBV	228991	278414	15.13%	1.927%
4	2.056	307	316	333	rVB	453501	654052	35.55%	4.527%
5	2.953	593	595	597	rBV	160	108	0.01%	0.001%
6	2.995	603	608	611	rBV	193	172	0.01%	0.001%
7	3.050	618	625	627	rBV2	396	537	0.03%	0.004%
8	3.101	638	641	643	rBV2	201	91	0.00%	0.001%
9	3.272	690	694	698	rBV3	343	329	0.02%	0.002%
10	3.323	707	710	713	rVB2	286	176	0.01%	0.001%
11	3.355	713	720	722	rBV3	299	335	0.02%	0.002%
12	3.371	722	725	728	rVB	201	124	0.01%	0.001%
13	3.391	730	731	734	rBV	207	93	0.01%	0.001%
14	3.410	734	737	740	rBV2	138	100	0.01%	0.001%
15	3.439	744	746	749	rVB	259	154	0.01%	0.001%
16	3.471	752	756	762	rBV3	287	272	0.01%	0.002%
17	3.535	774	776	779	rBV	190	118	0.01%	0.001%
18	3.587	789	792	794	rBV2	362	264	0.01%	0.002%
19	3.703	824	828	833	rVB2	312	344	0.02%	0.002%
20	3.735	836	838	842	rVB3	260	116	0.01%	0.001%
21	3.767	842	848	850	rBV2	249	195	0.01%	0.001%
22	3.805	851	860	900	rBV2	103913	358949	19.51%	2.484%
23	4.246	983	997	1029	rBV2	298067	851411	46.27%	5.893%
24	4.699	1136	1138	1140	rBV	222	136	0.01%	0.001%
25	4.760	1154	1157	1160	rVB3	433	291	0.02%	0.002%
26	4.783	1160	1164	1165	rBV2	337	246	0.01%	0.002%
27	4.838	1178	1181	1184	rBV	253	154	0.01%	0.001%
28	4.953	1201	1217	1254	rBV2	699421	1840019	100.00%	12.735%
29	5.490	1382	1384	1386	rBV	356	142	0.01%	0.001%
30	5.532	1386	1397	1435	rBV	598044	1239495	67.36%	8.579%
31	5.838	1481	1492	1506	rBV4	9464	22634	1.23%	0.157%
32	5.985	1526	1538	1571	rBV	392562	820600	44.60%	5.680%
33	6.281	1626	1630	1633	rVB3	607	474	0.03%	0.003%
34	6.304	1633	1637	1642	rVB3	460	479	0.03%	0.003%
35	6.329	1642	1645	1646	rBV2	314	215	0.01%	0.001%
36	6.358	1650	1654	1656	rBV	368	356	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035430.D
 Acq On : 26 Apr 2024 16:28
 Operator : SY/MD
 Sample : P2280-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08P7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.400	1665	1667	1669	rBV2	158	98	0.01%	0.001%
38	6.442	1669	1680	1700	rVV	12733	26791	1.46%	0.185%
39	6.516	1700	1703	1705	rVB	530	272	0.01%	0.002%
40	6.571	1716	1720	1724	rBV3	408	334	0.02%	0.002%
41	6.629	1736	1738	1741	rBV2	303	174	0.01%	0.001%
42	6.667	1748	1750	1753	rVB2	268	147	0.01%	0.001%
43	6.690	1753	1757	1759	rBV2	95	89	0.00%	0.001%
44	6.702	1759	1761	1765	rVV	144	107	0.01%	0.001%
45	6.789	1785	1788	1790	rBV	142	91	0.00%	0.001%
46	6.870	1807	1813	1816	rVB	187	161	0.01%	0.001%
47	6.911	1816	1826	1853	rBV	197934	381627	20.74%	2.641%
48	7.239	1917	1928	1955	rBV	791420	1423215	77.35%	9.850%
49	7.551	2016	2025	2060	rBV	133952	261399	14.21%	1.809%
50	7.944	2146	2147	2150	rBV2	311	147	0.01%	0.001%
51	7.963	2150	2153	2159	rVB3	386	251	0.01%	0.002%
52	8.030	2165	2174	2213	rBV3	294904	762140	41.42%	5.275%
53	8.551	2332	2336	2337	rBV	385	270	0.01%	0.002%
54	8.622	2356	2358	2361	rBV3	258	113	0.01%	0.001%
55	8.654	2365	2368	2371	rBV2	310	212	0.01%	0.001%
56	8.712	2382	2386	2390	rBV2	357	313	0.02%	0.002%
57	8.731	2390	2392	2396	rVB2	344	223	0.01%	0.002%
58	8.783	2396	2408	2445	rBV	929030	1555961	84.56%	10.769%
59	9.217	2539	2543	2550	rVB4	401	508	0.03%	0.004%
60	9.255	2552	2555	2557	rBV	231	130	0.01%	0.001%
61	9.265	2557	2558	2562	rVB2	231	98	0.01%	0.001%
62	9.294	2564	2567	2568	rBV	354	144	0.01%	0.001%
63	9.339	2579	2581	2583	rBV2	218	108	0.01%	0.001%
64	9.416	2603	2605	2612	rVB2	288	273	0.01%	0.002%
65	9.452	2612	2616	2617	rBV	239	139	0.01%	0.001%
66	9.522	2636	2638	2642	rBV2	244	201	0.01%	0.001%
67	9.651	2675	2678	2680	rVB	260	110	0.01%	0.001%
68	9.760	2709	2712	2715	rVB2	191	130	0.01%	0.001%
69	9.815	2725	2729	2732	rBV2	280	263	0.01%	0.002%
70	9.850	2739	2740	2743	rVB	303	104	0.01%	0.001%
71	9.876	2746	2748	2753	rVV2	319	213	0.01%	0.001%
72	9.924	2761	2763	2766	rVB2	297	166	0.01%	0.001%
73	9.963	2772	2775	2777	rBV2	148	121	0.01%	0.001%
74	10.056	2802	2804	2807	rVB2	238	140	0.01%	0.001%
75	10.149	2821	2833	2862	rBV	562953	910630	49.49%	6.303%
76	10.345	2891	2894	2898	rBV4	422	315	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035430.D
 Acq On : 26 Apr 2024 16:28
 Operator : SY/MD
 Sample : P2280-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E08P7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	10.397	2907	2910	2912	rBV2	335	218	0.01%	0.002%
78	10.535	2950	2953	2955	rBV	183	108	0.01%	0.001%
79	10.558	2956	2960	2962	rBV	301	221	0.01%	0.002%
80	10.590	2969	2970	2974	rVB2	295	132	0.01%	0.001%
81	10.615	2974	2978	2984	rBV2	287	260	0.01%	0.002%
82	10.715	3003	3009	3015	rVB3	693	924	0.05%	0.006%
83	10.757	3020	3022	3026	rVB2	226	166	0.01%	0.001%
84	10.841	3044	3048	3051	rBV3	297	229	0.01%	0.002%
85	10.863	3051	3055	3056	rBV	259	136	0.01%	0.001%
86	10.918	3069	3072	3075	rBV2	191	128	0.01%	0.001%
87	10.956	3078	3084	3086	rBV2	541	565	0.03%	0.004%
88	11.053	3110	3114	3116	rBV2	296	232	0.01%	0.002%
89	11.095	3124	3127	3131	rBV	257	239	0.01%	0.002%
90	11.130	3131	3138	3143	rBV4	3744	5208	0.28%	0.036%
91	11.185	3144	3155	3182	rVV	837244	1368427	74.37%	9.471%
92	11.487	3246	3249	3251	rBV	387	255	0.01%	0.002%
93	11.558	3260	3271	3302	rBV	780536	1286798	69.93%	8.906%
94	12.294	3497	3500	3504	rVB3	383	296	0.02%	0.002%
95	12.506	3564	3566	3569	rBV	295	190	0.01%	0.001%
96	12.689	3621	3623	3625	rBV2	389	223	0.01%	0.002%
97	12.895	3685	3687	3690	rBV	278	155	0.01%	0.001%
98	13.094	3746	3749	3750	rBV2	347	227	0.01%	0.002%
99	13.201	3773	3782	3794	rBV2	28269	44978	2.44%	0.311%
100	13.683	3925	3932	3946	rVB4	6780	11704	0.64%	0.081%



Sum of corrected areas: 14448232

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035430.D
Acq On : 26 Apr 2024 16:28
Operator : SY/MD
Sample : P2280-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08P7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

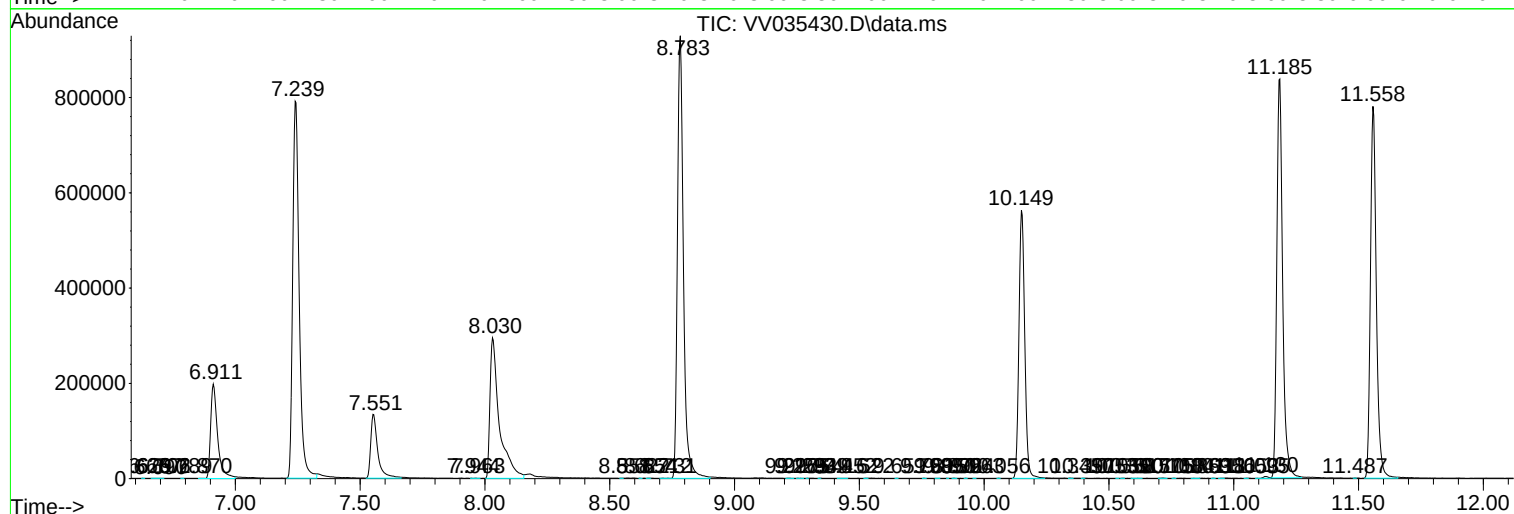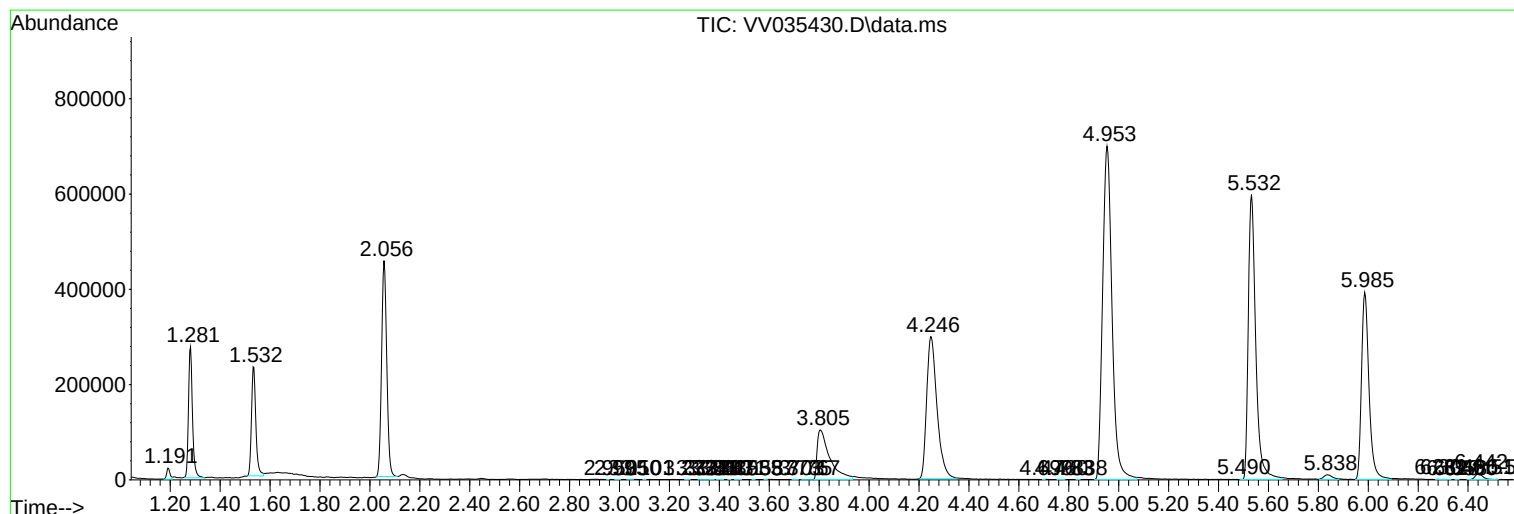

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035430.D
Acq On : 26 Apr 2024 16:28
Operator : SY/MD
Sample : P2280-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08P7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035430.D
Acq On : 26 Apr 2024 16:28
Operator : SY/MD
Sample : P2280-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E08P7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------