

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035433.D
 Acq On : 26 Apr 2024 17:39
 Operator : SY/MD
 Sample : P2204-03 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1CW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M

Title : VOC Analysis

Signal : TIC: VV035433.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	93	rBV	273361	297480	16.25%	2.141%
2	1.532	146	153	166	rBV	230428	271796	14.85%	1.956%
3	2.056	306	316	332	rVB	444709	645644	35.27%	4.646%
4	2.687	510	512	514	rBV2	257	140	0.01%	0.001%
5	2.847	560	562	563	rBV2	152	41	0.00%	0.000%
6	2.986	603	605	609	rBV2	218	159	0.01%	0.001%
7	3.002	609	610	613	rVB2	287	82	0.00%	0.001%
8	3.050	622	625	628	rBV	304	165	0.01%	0.001%
9	3.069	628	631	633	rBV	345	169	0.01%	0.001%
10	3.169	659	662	663	rBV	172	83	0.00%	0.001%
11	3.220	677	678	681	rVB2	287	105	0.01%	0.001%
12	3.333	710	713	715	rBV	172	88	0.00%	0.001%
13	3.349	715	718	723	rVV2	370	286	0.02%	0.002%
14	3.388	726	730	734	rBV2	291	297	0.02%	0.002%
15	3.474	755	757	760	rVB	181	95	0.01%	0.001%
16	3.494	760	763	765	rBV2	232	126	0.01%	0.001%
17	3.561	781	784	789	rVB	279	169	0.01%	0.001%
18	3.651	808	812	815	rBV3	265	244	0.01%	0.002%
19	3.735	835	838	840	rBV	196	109	0.01%	0.001%
20	3.751	840	843	844	rVB	147	78	0.00%	0.001%
21	3.761	844	846	848	rVB2	169	73	0.00%	0.001%
22	3.806	848	860	893	rBV	102088	359159	19.62%	2.584%
23	4.246	982	997	1026	rBV	284376	730877	39.93%	5.259%
24	4.680	1128	1132	1135	rVB3	384	283	0.02%	0.002%
25	4.857	1184	1187	1190	rBV2	401	309	0.02%	0.002%
26	4.953	1201	1217	1250	rBV2	697941	1830543	100.00%	13.172%
27	5.432	1362	1366	1370	rBV4	599	459	0.03%	0.003%
28	5.532	1385	1397	1439	rBV	563566	1189237	64.97%	8.557%
29	5.986	1525	1538	1570	rBV	391513	820964	44.85%	5.907%
30	6.281	1627	1630	1634	rBV3	509	419	0.02%	0.003%
31	6.304	1634	1637	1639	rBV	696	371	0.02%	0.003%
32	6.339	1639	1648	1651	rBV5	1409	2233	0.12%	0.016%
33	6.513	1700	1702	1703	rBV2	308	105	0.01%	0.001%
34	6.596	1725	1728	1731	rBV	268	200	0.01%	0.001%
35	6.613	1731	1733	1738	rVB2	423	273	0.01%	0.002%
36	6.664	1748	1749	1750	rBV	238	49	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035433.D
 Acq On : 26 Apr 2024 17:39
 Operator : SY/MD
 Sample : P2204-03 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1CW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.683	1753	1755	1757	rVV	238	107	0.01%	0.001%
38	6.703	1757	1761	1764	rVV2	401	302	0.02%	0.002%
39	6.735	1768	1771	1774	rVB2	372	235	0.01%	0.002%
40	6.754	1774	1777	1778	rBV	177	103	0.01%	0.001%
41	6.822	1796	1798	1800	rVB	251	57	0.00%	0.000%
42	6.834	1800	1802	1805	rVB2	237	105	0.01%	0.001%
43	6.912	1815	1826	1863	rBV	197199	385317	21.05%	2.773%
44	7.239	1917	1928	1959	rBV	790378	1417896	77.46%	10.203%
45	7.551	2016	2025	2054	rBV	135492	255465	13.96%	1.838%
46	7.870	2116	2124	2141	rVB2	5347	10247	0.56%	0.074%
47	7.934	2141	2144	2149	rVB2	641	463	0.03%	0.003%
48	7.960	2149	2152	2155	rBV2	248	157	0.01%	0.001%
49	8.030	2164	2174	2221	rBV2	309339	766970	41.90%	5.519%
50	8.632	2353	2361	2375	rVB6	3552	6584	0.36%	0.047%
51	8.783	2396	2408	2439	rBV	877049	1463177	79.93%	10.529%
52	9.188	2530	2534	2535	rBV2	397	283	0.02%	0.002%
53	9.210	2538	2541	2542	rBV	336	208	0.01%	0.001%
54	9.246	2550	2552	2556	rBV2	329	207	0.01%	0.001%
55	9.320	2570	2575	2578	rBV4	475	445	0.02%	0.003%
56	9.371	2589	2591	2595	rBV2	312	180	0.01%	0.001%
57	9.407	2599	2602	2605	rBV4	383	364	0.02%	0.003%
58	9.516	2633	2636	2637	rBV	210	114	0.01%	0.001%
59	9.526	2637	2639	2641	rVB2	210	97	0.01%	0.001%
60	9.628	2667	2671	2675	rVB3	445	373	0.02%	0.003%
61	9.683	2686	2688	2690	rVB	175	67	0.00%	0.000%
62	9.937	2764	2767	2768	rBV	170	92	0.01%	0.001%
63	9.982	2778	2781	2789	rBV2	263	236	0.01%	0.002%
64	10.069	2804	2808	2811	rBV	382	294	0.02%	0.002%
65	10.098	2814	2817	2819	rBV	212	111	0.01%	0.001%
66	10.149	2822	2833	2856	rBV	571183	909329	49.68%	6.543%
67	10.503	2940	2943	2945	rBV2	273	174	0.01%	0.001%
68	10.577	2963	2966	2969	rVB2	306	216	0.01%	0.002%
69	10.609	2974	2976	2981	rVB2	511	302	0.02%	0.002%
70	10.638	2981	2985	2987	rBV2	371	238	0.01%	0.002%
71	10.751	3017	3020	3022	rBV	296	128	0.01%	0.001%
72	10.783	3029	3030	3034	rVB	395	241	0.01%	0.002%
73	10.850	3050	3051	3052	rBV	159	50	0.00%	0.000%
74	10.944	3078	3080	3081	rBV	142	35	0.00%	0.000%
75	10.992	3092	3095	3097	rBV	401	234	0.01%	0.002%
76	11.066	3116	3118	3119	rBV	183	87	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035433.D
 Acq On : 26 Apr 2024 17:39
 Operator : SY/MD
 Sample : P2204-03 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E1CW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M

Title : VOC Analysis

77	11.075	3119	3121	3125	rVV2	394	219	0.01%	0.002%
78	11.181	3143	3154	3181	rBV	791966	1279248	69.88%	9.205%
79	11.558	3259	3271	3300	rBV	779415	1240791	67.78%	8.928%
80	11.918	3381	3383	3386	rBV2	359	203	0.01%	0.001%
81	12.815	3660	3662	3666	rVB2	462	291	0.02%	0.002%
82	12.837	3666	3669	3671	rBV2	219	151	0.01%	0.001%
83	12.988	3714	3716	3719	rBV2	294	175	0.01%	0.001%
84	13.210	3782	3785	3791	rVB4	1740	1559	0.09%	0.011%
85	14.902	4309	4311	4313	rBV	827	331	0.02%	0.002%




Sum of corrected areas: 13897168

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035433.D
Acq On : 26 Apr 2024 17:39
Operator : SY/MD
Sample : P2204-03 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1CW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

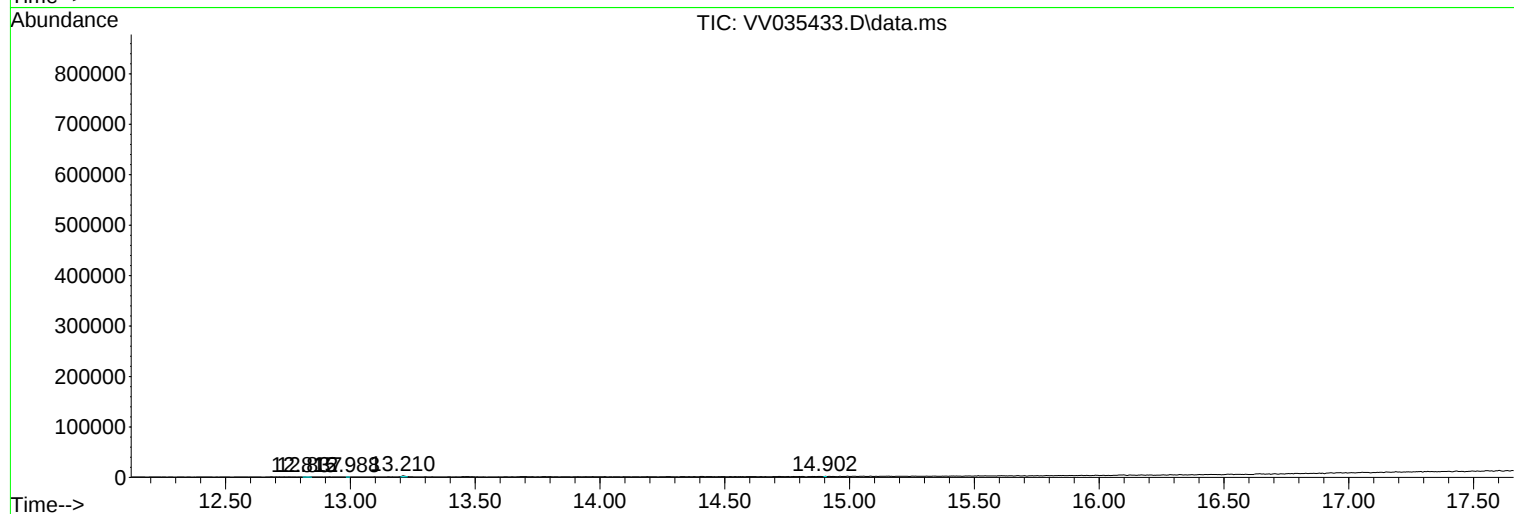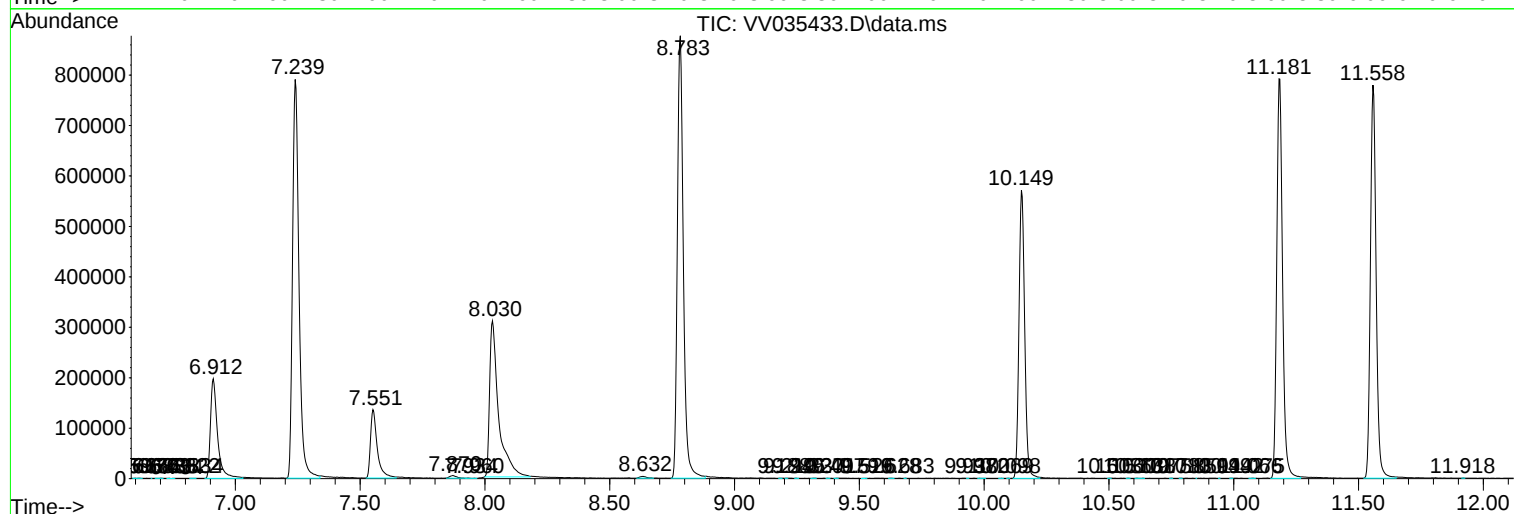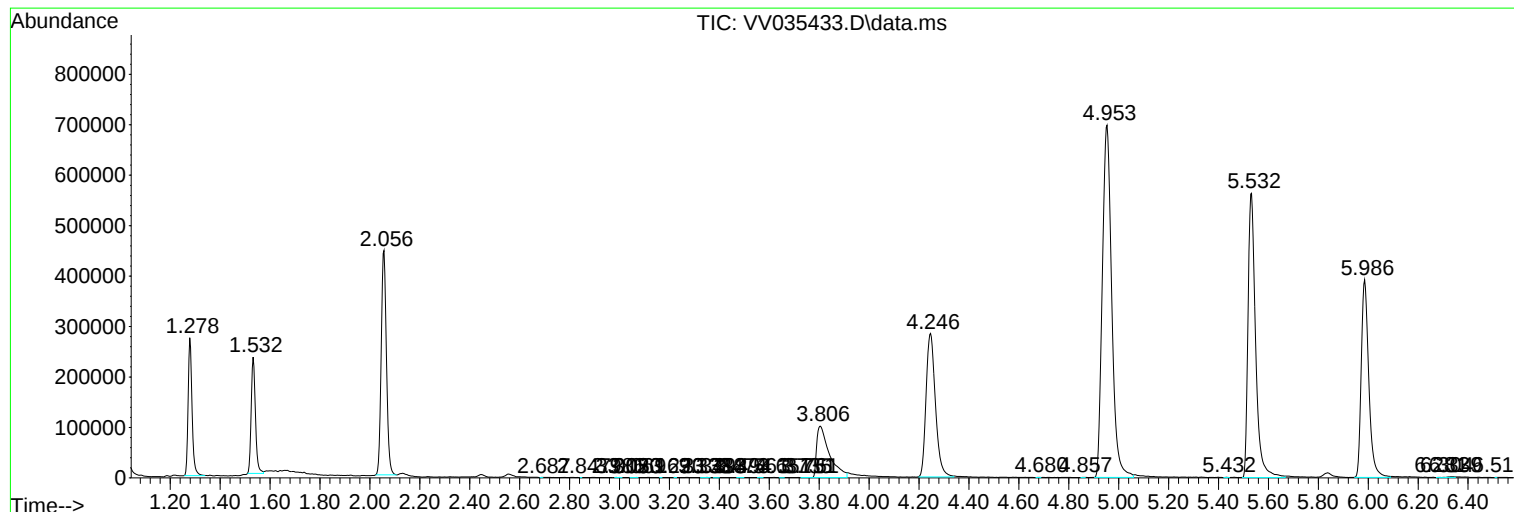

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035433.D
Acq On : 26 Apr 2024 17:39
Operator : SY/MD
Sample : P2204-03 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1CW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035433.D
Acq On : 26 Apr 2024 17:39
Operator : SY/MD
Sample : P2204-03 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E1CW8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc