

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035436.D
 Acq On : 26 Apr 2024 18:51
 Operator : SY/MD
 Sample : P2235-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	94	rVB	259846	282545	16.33%	2.161%
2	1.532	146	153	166	rBV	225683	257455	14.88%	1.969%
3	2.056	306	316	334	rBV	419539	610143	35.26%	4.666%
4	2.761	532	535	538	rBV	297	201	0.01%	0.002%
5	2.876	570	571	572	rBV	131	42	0.00%	0.000%
6	2.908	579	581	582	rBV	141	77	0.00%	0.001%
7	2.937	586	590	593	rBV2	302	290	0.02%	0.002%
8	3.060	625	628	630	rVB2	233	117	0.01%	0.001%
9	3.076	630	633	637	rBV2	244	200	0.01%	0.002%
10	3.156	654	658	660	rBV3	192	173	0.01%	0.001%
11	3.182	664	666	668	rBV	187	113	0.01%	0.001%
12	3.220	675	678	680	rBV	96	69	0.00%	0.001%
13	3.272	692	694	695	rBV	136	40	0.00%	0.000%
14	3.281	695	697	700	rVB2	236	107	0.01%	0.001%
15	3.320	705	709	712	rVB2	271	198	0.01%	0.002%
16	3.343	712	716	720	rVB	251	198	0.01%	0.002%
17	3.371	720	725	728	rBV2	297	287	0.02%	0.002%
18	3.439	741	746	750	rVB3	384	357	0.02%	0.003%
19	3.458	750	752	756	rBV2	69	42	0.00%	0.000%
20	3.490	758	762	766	rVB	250	222	0.01%	0.002%
21	3.513	766	769	772	rBV2	278	182	0.01%	0.001%
22	3.532	772	775	778	rBV	179	110	0.01%	0.001%
23	3.577	783	789	791	rBV2	146	131	0.01%	0.001%
24	3.597	791	795	799	rVB2	355	245	0.01%	0.002%
25	3.622	799	803	804	rBV2	298	192	0.01%	0.001%
26	3.648	809	811	815	rVB2	411	255	0.01%	0.002%
27	3.677	815	820	824	rBV2	204	200	0.01%	0.002%
28	3.699	824	827	829	rBV2	261	185	0.01%	0.001%
29	3.767	846	848	850	rVB	156	46	0.00%	0.000%
30	3.802	850	859	911	rBV	91339	324946	18.78%	2.485%
31	4.246	982	997	1027	rBV	264681	683928	39.52%	5.230%
32	4.860	1185	1188	1189	rBV	406	209	0.01%	0.002%
33	4.953	1200	1217	1264	rBV2	660246	1730390	100.00%	13.232%
34	5.288	1319	1321	1323	rBV	350	208	0.01%	0.002%
35	5.416	1359	1361	1364	rVB	454	212	0.01%	0.002%
36	5.432	1364	1366	1367	rBV	356	168	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035436.D
 Acq On : 26 Apr 2024 18:51
 Operator : SY/MD
 Sample : P2235-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	5.532	1386	1397	1424	rBV	550149	1146047	66.23%	8.764%
38	5.834	1481	1491	1509	rBV4	7972	19905	1.15%	0.152%
39	5.985	1526	1538	1573	rBV	367380	773353	44.69%	5.914%
40	6.362	1653	1655	1657	rBV2	306	158	0.01%	0.001%
41	6.387	1661	1663	1669	rVB3	340	213	0.01%	0.002%
42	6.448	1677	1682	1686	rVB2	296	323	0.02%	0.002%
43	6.481	1690	1692	1697	rVV	234	191	0.01%	0.001%
44	6.500	1697	1698	1701	rVV	237	89	0.01%	0.001%
45	6.513	1701	1702	1703	rVV	165	45	0.00%	0.000%
46	6.526	1704	1706	1711	rVV3	299	278	0.02%	0.002%
47	6.555	1712	1715	1720	rVB3	284	220	0.01%	0.002%
48	6.619	1732	1735	1739	rBV2	330	208	0.01%	0.002%
49	6.641	1739	1742	1745	rBV2	113	95	0.01%	0.001%
50	6.667	1748	1750	1751	rBV	158	69	0.00%	0.001%
51	6.690	1756	1757	1761	rVB2	306	121	0.01%	0.001%
52	6.709	1761	1763	1765	rVB2	120	49	0.00%	0.000%
53	6.725	1765	1768	1771	rBV2	312	203	0.01%	0.002%
54	6.841	1800	1804	1805	rBV	141	100	0.01%	0.001%
55	6.863	1809	1811	1813	rBV2	171	104	0.01%	0.001%
56	6.911	1816	1826	1861	rBV	177836	355489	20.54%	2.718%
57	7.239	1915	1928	1975	rBV	745879	1332374	77.00%	10.189%
58	7.551	2016	2025	2052	rBV	124120	236692	13.68%	1.810%
59	7.873	2122	2125	2128	rBV3	503	332	0.02%	0.003%
60	7.911	2134	2137	2138	rBV2	192	129	0.01%	0.001%
61	8.030	2165	2174	2217	rBV3	268003	688938	39.81%	5.268%
62	8.458	2304	2307	2311	rVB3	527	346	0.02%	0.003%
63	8.609	2352	2354	2357	rBV2	327	201	0.01%	0.002%
64	8.702	2379	2383	2386	rBV	316	309	0.02%	0.002%
65	8.783	2396	2408	2440	rBV	850270	1426424	82.43%	10.908%
66	9.236	2547	2549	2554	rVB3	503	300	0.02%	0.002%
67	9.436	2608	2611	2613	rBV2	229	108	0.01%	0.001%
68	9.490	2626	2628	2630	rBV2	228	108	0.01%	0.001%
69	9.500	2630	2631	2633	rVV	266	75	0.00%	0.001%
70	9.628	2667	2671	2675	rBV3	327	266	0.02%	0.002%
71	9.657	2678	2680	2682	rBV2	223	82	0.00%	0.001%
72	9.699	2691	2693	2696	rBV	208	100	0.01%	0.001%
73	9.725	2699	2701	2705	rVB2	266	128	0.01%	0.001%
74	9.767	2711	2714	2716	rBV2	363	186	0.01%	0.001%
75	9.802	2721	2725	2728	rBV	364	354	0.02%	0.003%
76	9.940	2765	2768	2769	rBV	159	88	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035436.D
 Acq On : 26 Apr 2024 18:51
 Operator : SY/MD
 Sample : P2235-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M

Title : VOC Analysis

77	10.149	2821	2833	2860	rBV	522067	842387	48.68%	6.442%
78	10.439	2919	2923	2927	rBV2	348	335	0.02%	0.003%
79	10.458	2927	2929	2932	rVB	291	117	0.01%	0.001%
80	10.500	2937	2942	2945	rBV2	621	514	0.03%	0.004%
81	10.812	3036	3039	3042	rBV2	190	123	0.01%	0.001%
82	10.988	3091	3094	3095	rBV	204	100	0.01%	0.001%
83	11.117	3131	3134	3135	rBV2	372	207	0.01%	0.002%
84	11.181	3144	3154	3186	rBV	772235	1219576	70.48%	9.326%
85	11.558	3259	3271	3296	rBV	703405	1133173	65.49%	8.665%
86	12.185	3463	3466	3470	rBV2	420	411	0.02%	0.003%
87	12.252	3485	3487	3490	rBV2	393	220	0.01%	0.002%
88	12.281	3495	3496	3498	rBV2	260	81	0.00%	0.001%
89	12.599	3593	3595	3598	rBV2	271	178	0.01%	0.001%
90	13.101	3749	3751	3756	rVB2	464	335	0.02%	0.003%




Sum of corrected areas: 13077040

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035436.D
Acq On : 26 Apr 2024 18:51
Operator : SY/MD
Sample : P2235-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

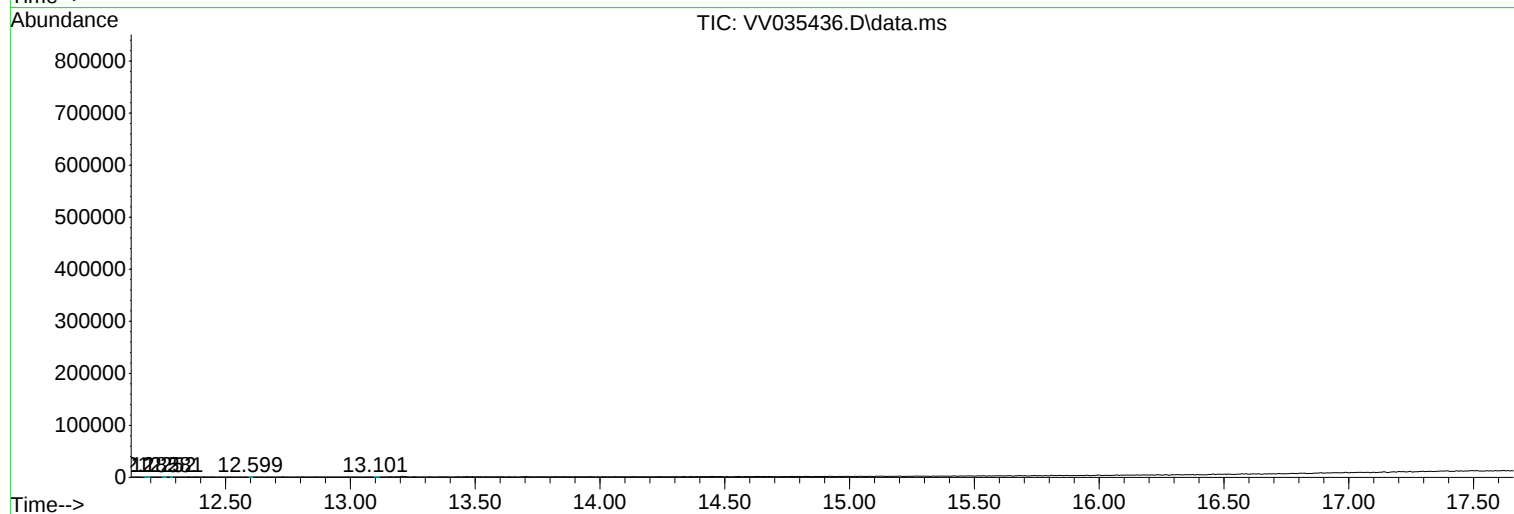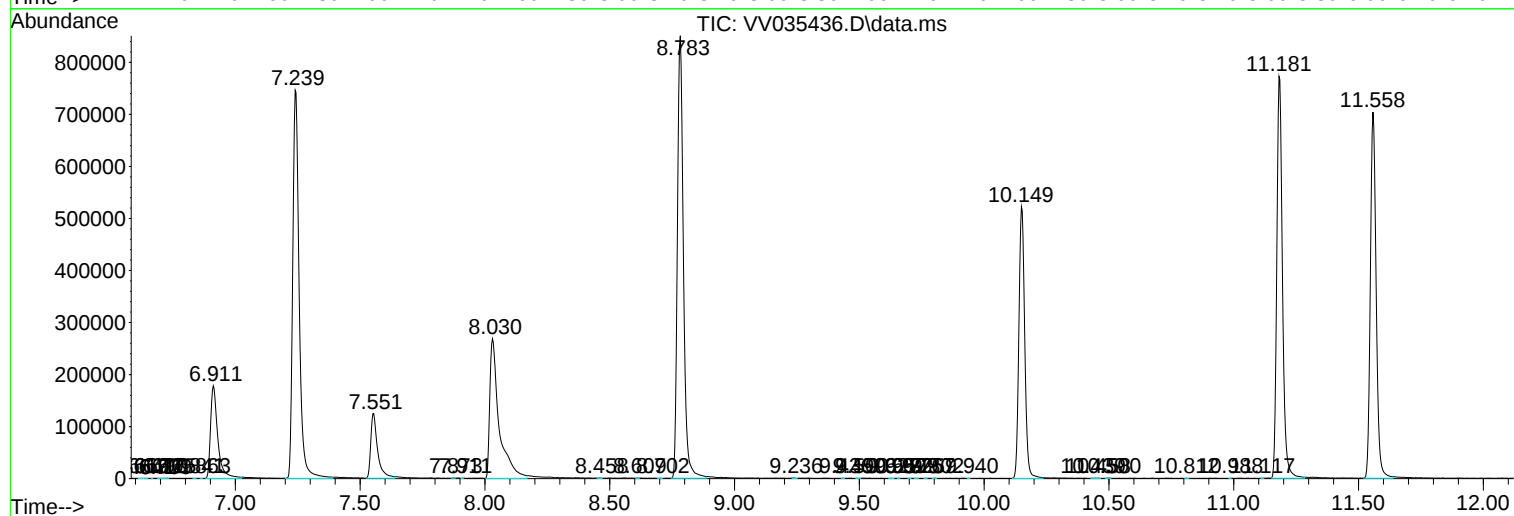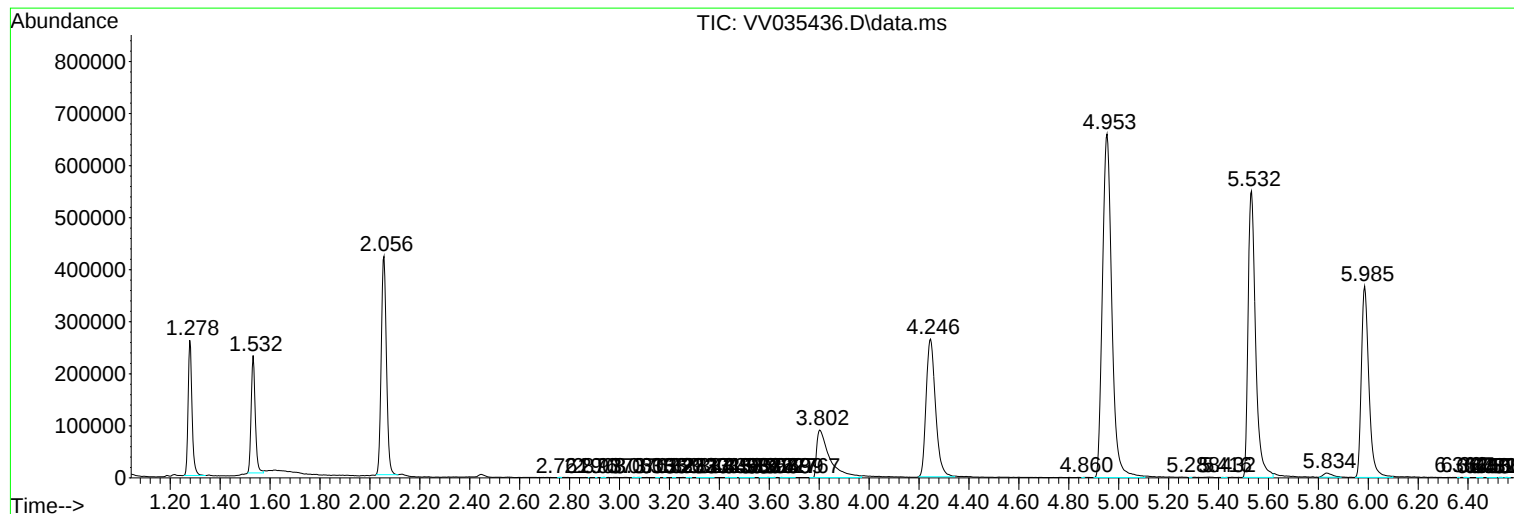

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035436.D
Acq On : 26 Apr 2024 18:51
Operator : SY/MD
Sample : P2235-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035436.D
Acq On : 26 Apr 2024 18:51
Operator : SY/MD
Sample : P2235-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
