

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035440.D
 Acq On : 26 Apr 2024 21:14
 Operator : SY/MD
 Sample : VV0426WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK278

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M

Title : VOC Analysis

Signal : TIC: VV035440.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	88	rVB	275783	300872	16.59%	2.170%
2	1.526	146	151	165	rVB	185023	205216	11.31%	1.480%
3	2.053	305	315	330	rBV	446638	647190	35.68%	4.668%
4	2.754	531	533	537	rBV2	263	180	0.01%	0.001%
5	2.835	554	558	560	rBV2	413	306	0.02%	0.002%
6	2.851	560	563	565	rVV2	249	153	0.01%	0.001%
7	2.921	582	585	587	rBV2	276	199	0.01%	0.001%
8	2.950	592	594	595	rBV	248	91	0.01%	0.001%
9	2.976	600	602	603	rBV	307	113	0.01%	0.001%
10	3.011	610	613	618	rVB3	302	191	0.01%	0.001%
11	3.101	639	641	643	rBV	256	169	0.01%	0.001%
12	3.153	655	657	660	rVB	178	84	0.00%	0.001%
13	3.172	660	663	666	rBV2	398	273	0.02%	0.002%
14	3.217	674	677	679	rBV	197	136	0.01%	0.001%
15	3.246	683	686	690	rBV3	295	268	0.01%	0.002%
16	3.265	690	692	696	rVV2	274	178	0.01%	0.001%
17	3.298	700	702	706	rBV2	292	170	0.01%	0.001%
18	3.359	717	721	725	rVB	243	186	0.01%	0.001%
19	3.384	725	729	735	rBV3	258	342	0.02%	0.002%
20	3.410	735	737	739	rBV	181	93	0.01%	0.001%
21	3.487	758	761	763	rBV2	176	134	0.01%	0.001%
22	3.539	775	777	778	rBV2	230	101	0.01%	0.001%
23	3.574	786	788	792	rVB	255	164	0.01%	0.001%
24	3.606	795	798	800	rBV3	211	109	0.01%	0.001%
25	3.674	816	819	824	rVB2	390	303	0.02%	0.002%
26	3.706	824	829	831	rBV	197	198	0.01%	0.001%
27	3.719	831	833	835	rVB2	225	80	0.00%	0.001%
28	3.796	848	857	904	rBV	117361	380593	20.98%	2.745%
29	4.246	982	997	1031	rBV	278092	717227	39.54%	5.173%
30	4.648	1119	1122	1128	rBV4	620	590	0.03%	0.004%
31	4.738	1148	1150	1154	rVB2	398	255	0.01%	0.002%
32	4.761	1154	1157	1159	rBV2	239	191	0.01%	0.001%
33	4.873	1189	1192	1194	rVB2	270	137	0.01%	0.001%
34	4.953	1201	1217	1262	rBV2	694536	1813735	100.00%	13.083%
35	5.346	1337	1339	1341	rBV	454	259	0.01%	0.002%
36	5.416	1358	1361	1367	rBV3	454	395	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035440.D
 Acq On : 26 Apr 2024 21:14
 Operator : SY/MD
 Sample : VV0426WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK278

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	5.532	1386	1397	1437	rBV	577160	1217501	67.13%	8.782%
38	5.838	1481	1492	1518	rVB4	9198	24419	1.35%	0.176%
39	5.934	1519	1522	1525	rBV3	771	647	0.04%	0.005%
40	5.986	1526	1538	1566	rBV	389054	802382	44.24%	5.788%
41	6.291	1630	1633	1636	rBV	223	150	0.01%	0.001%
42	6.307	1636	1638	1641	rVB2	286	154	0.01%	0.001%
43	6.346	1648	1650	1652	rBV	298	138	0.01%	0.001%
44	6.362	1654	1655	1656	rVV	365	111	0.01%	0.001%
45	6.384	1660	1662	1664	rVB2	227	108	0.01%	0.001%
46	6.420	1669	1673	1676	rBV2	417	272	0.01%	0.002%
47	6.458	1681	1685	1687	rBV2	221	162	0.01%	0.001%
48	6.490	1693	1695	1701	rVB2	175	129	0.01%	0.001%
49	6.539	1706	1710	1711	rBV2	372	198	0.01%	0.001%
50	6.619	1732	1735	1739	rBV2	162	145	0.01%	0.001%
51	6.642	1740	1742	1744	rBV	175	74	0.00%	0.001%
52	6.741	1770	1773	1775	rBV	271	168	0.01%	0.001%
53	6.876	1810	1815	1816	rBV	153	121	0.01%	0.001%
54	6.912	1816	1826	1851	rBV	190120	369205	20.36%	2.663%
55	7.240	1916	1928	1966	rBV	776072	1396484	76.99%	10.073%
56	7.551	2017	2025	2057	rBV	129337	244311	13.47%	1.762%
57	7.754	2086	2088	2090	rBV2	592	365	0.02%	0.003%
58	7.809	2102	2105	2106	rBV2	269	170	0.01%	0.001%
59	7.892	2129	2131	2134	rVB2	334	155	0.01%	0.001%
60	7.908	2134	2136	2138	rBV3	369	225	0.01%	0.002%
61	7.921	2138	2140	2145	rVB4	590	498	0.03%	0.004%
62	7.944	2145	2147	2151	rBV2	310	281	0.02%	0.002%
63	7.992	2158	2162	2163	rBV2	400	202	0.01%	0.001%
64	8.031	2165	2174	2219	rBV2	326163	801090	44.17%	5.778%
65	8.545	2332	2334	2335	rBV	410	152	0.01%	0.001%
66	8.635	2360	2362	2365	rBV2	294	145	0.01%	0.001%
67	8.674	2372	2374	2375	rBV	223	80	0.00%	0.001%
68	8.712	2383	2386	2387	rVB	399	158	0.01%	0.001%
69	8.783	2396	2408	2446	rBV	905931	1488396	82.06%	10.736%
70	9.227	2545	2546	2549	rVB2	280	110	0.01%	0.001%
71	9.249	2551	2553	2557	rBV2	357	260	0.01%	0.002%
72	9.301	2567	2569	2576	rBV2	142	160	0.01%	0.001%
73	9.333	2578	2579	2581	rBV2	291	74	0.00%	0.001%
74	9.381	2591	2594	2598	rBV2	131	119	0.01%	0.001%
75	9.407	2599	2602	2604	rBV2	255	159	0.01%	0.001%
76	9.461	2616	2619	2620	rBV2	177	104	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035440.D
 Acq On : 26 Apr 2024 21:14
 Operator : SY/MD
 Sample : VV0426WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK278

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	9.513	2631	2635	2639	rVB3	528	453	0.02%	0.003%
78	9.535	2639	2642	2644	rBV2	544	383	0.02%	0.003%
79	10.069	2803	2808	2810	rBV2	335	282	0.02%	0.002%
80	10.149	2822	2833	2861	rBV	572624	914547	50.42%	6.597%
81	10.387	2905	2907	2911	rVB2	379	235	0.01%	0.002%
82	10.474	2930	2934	2935	rBV	363	224	0.01%	0.002%
83	10.522	2947	2949	2959	rBV2	264	437	0.02%	0.003%
84	10.815	3038	3040	3043	rBV	204	129	0.01%	0.001%
85	10.924	3071	3074	3078	rBV2	326	274	0.02%	0.002%
86	11.008	3097	3100	3106	rBV2	222	206	0.01%	0.001%
87	11.185	3144	3155	3185	rBV	821865	1301651	71.77%	9.389%
88	11.558	3259	3271	3296	rBV	740405	1186212	65.40%	8.556%
89	11.915	3380	3382	3386	rBV2	327	169	0.01%	0.001%
90	11.989	3402	3405	3408	rBV2	359	313	0.02%	0.002%
91	12.246	3483	3485	3490	rVB2	479	316	0.02%	0.002%
92	12.278	3490	3495	3496	rBV2	374	286	0.02%	0.002%
93	12.329	3508	3511	3516	rBV2	333	262	0.01%	0.002%
94	12.390	3528	3530	3532	rBV	260	126	0.01%	0.001%
95	12.590	3587	3592	3597	rBV4	1340	1849	0.10%	0.013%
96	12.690	3621	3623	3626	rBV2	303	137	0.01%	0.001%
97	13.066	3735	3740	3746	rBV3	475	602	0.03%	0.004%
98	13.210	3779	3785	3801	rVB5	3886	6706	0.37%	0.048%
99	13.445	3851	3858	3872	rBV2	11091	19645	1.08%	0.142%
100	13.683	3925	3932	3942	rBV5	4689	7557	0.42%	0.055%




Sum of corrected areas: 13863664

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035440.D
Acq On : 26 Apr 2024 21:14
Operator : SY/MD
Sample : VV0426WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK278

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

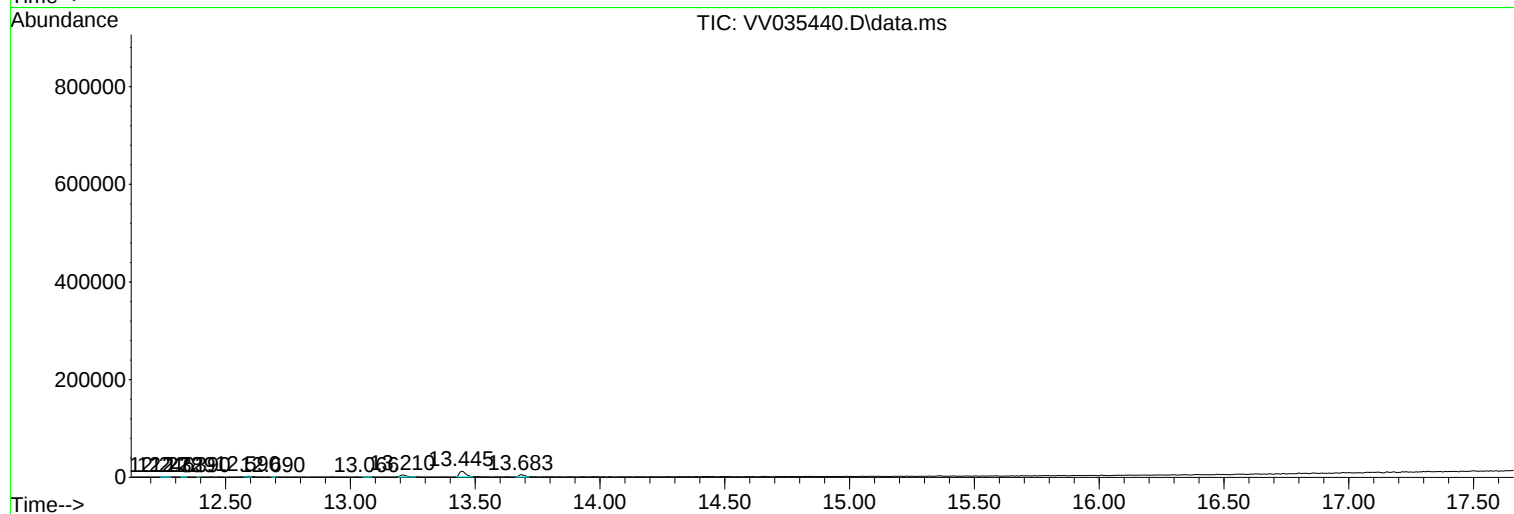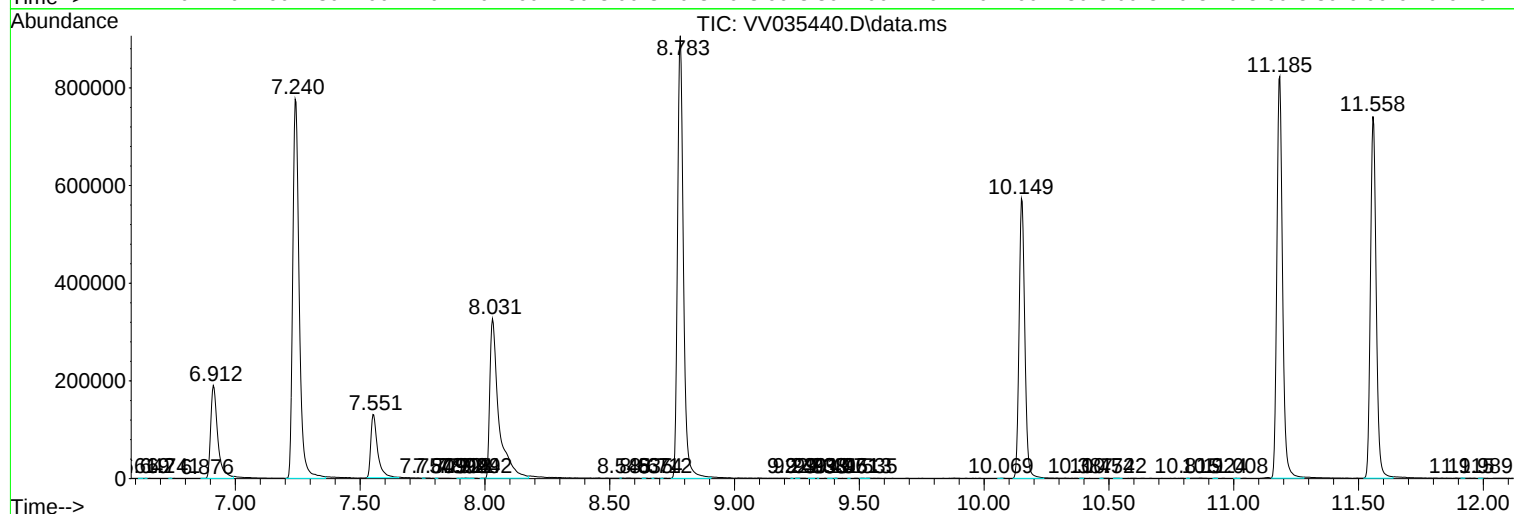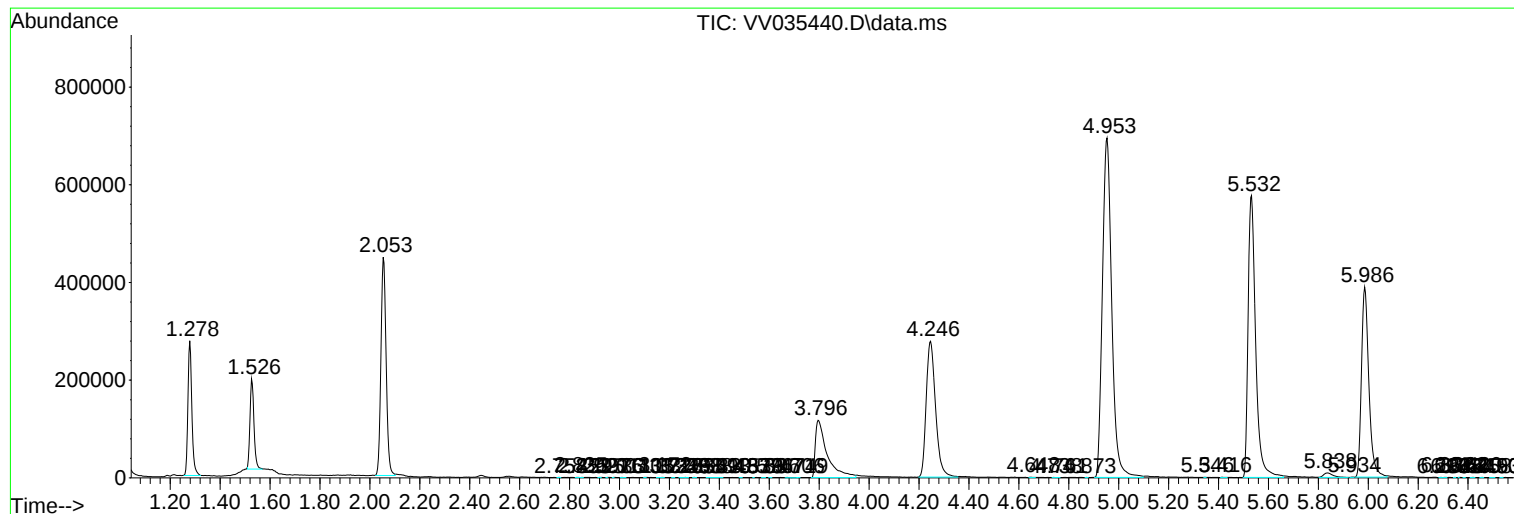

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035440.D
Acq On : 26 Apr 2024 21:14
Operator : SY/MD
Sample : VV0426WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK278

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035440.D
Acq On : 26 Apr 2024 21:14
Operator : SY/MD
Sample : VV0426WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK278

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------