

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035441.D
 Acq On : 26 Apr 2024 21:37
 Operator : SY/MD
 Sample : P2279-01 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M

Title : VOC Analysis

Signal : TIC: VV035441.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	93	rVB	256379	279382	15.91%	2.083%
2	1.529	146	152	167	rVB	178194	199990	11.39%	1.491%
3	2.053	306	315	332	rBV	418220	605249	34.47%	4.513%
4	2.748	526	531	534	rBV2	292	256	0.01%	0.002%
5	2.796	543	546	548	rBV	176	115	0.01%	0.001%
6	2.809	548	550	552	rBV	243	122	0.01%	0.001%
7	2.838	557	559	561	rVB2	170	72	0.00%	0.001%
8	3.063	626	629	632	rVB	255	182	0.01%	0.001%
9	3.082	632	635	637	rBV2	339	169	0.01%	0.001%
10	3.146	653	655	658	rVV2	209	128	0.01%	0.001%
11	3.166	658	661	665	rVB2	425	320	0.02%	0.002%
12	3.304	701	704	709	rBV2	224	203	0.01%	0.002%
13	3.339	713	715	717	rBV	282	138	0.01%	0.001%
14	3.487	756	761	764	rVB3	305	278	0.02%	0.002%
15	3.529	769	774	777	rBV3	454	347	0.02%	0.003%
16	3.619	799	802	804	rBV3	232	146	0.01%	0.001%
17	3.657	810	814	817	rBV3	207	145	0.01%	0.001%
18	3.722	830	834	837	rBV2	348	316	0.02%	0.002%
19	3.799	849	858	910	rBV	112958	383206	21.82%	2.857%
20	4.246	982	997	1032	rBV	271155	697781	39.74%	5.203%
21	4.532	1084	1086	1087	rBV2	362	106	0.01%	0.001%
22	4.577	1096	1100	1104	rBV2	595	635	0.04%	0.005%
23	4.635	1115	1118	1123	rBV2	285	326	0.02%	0.002%
24	4.770	1158	1160	1162	rVB	221	76	0.00%	0.001%
25	4.792	1162	1167	1173	rBV4	316	477	0.03%	0.004%
26	4.863	1186	1189	1192	rBV	298	225	0.01%	0.002%
27	4.953	1199	1217	1259	rBV2	669535	1756028	100.00%	13.094%
28	5.381	1346	1350	1352	rBV2	369	236	0.01%	0.002%
29	5.532	1386	1397	1429	rBV	570860	1184574	67.46%	8.833%
30	5.985	1526	1538	1581	rBV	371992	786104	44.77%	5.862%
31	6.439	1675	1679	1681	rBV3	457	267	0.02%	0.002%
32	6.468	1686	1688	1691	rBV3	319	167	0.01%	0.001%
33	6.538	1708	1710	1711	rBB	66	46	0.00%	0.000%
34	6.657	1741	1747	1750	rBV3	371	269	0.02%	0.002%
35	6.722	1764	1767	1770	rBV2	166	132	0.01%	0.001%
36	6.741	1770	1773	1778	rVB3	207	204	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042624\
 Data File : VW035441.D
 Acq On : 26 Apr 2024 21:37
 Operator : SY/MD
 Sample : P2279-01 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.770	1778	1782	1787	rBV2	319	318	0.02%	0.002%
38	6.821	1795	1798	1799	rBV2	162	83	0.00%	0.001%
39	6.911	1816	1826	1870	rBV	182589	368190	20.97%	2.745%
40	7.243	1917	1929	1969	rBV	741361	1333247	75.92%	9.942%
41	7.554	2017	2026	2061	rBV	126421	242315	13.80%	1.807%
42	7.918	2134	2139	2143	rBV4	421	354	0.02%	0.003%
43	7.940	2144	2146	2147	rBV4	317	106	0.01%	0.001%
44	7.988	2158	2161	2165	rBV3	418	293	0.02%	0.002%
45	8.030	2165	2174	2221	rBV3	320838	791028	45.05%	5.898%
46	8.664	2369	2371	2374	rBV2	347	165	0.01%	0.001%
47	8.783	2396	2408	2444	rBV	879899	1487735	84.72%	11.094%
48	9.168	2526	2528	2529	rBV	325	109	0.01%	0.001%
49	9.217	2541	2543	2545	rBV2	475	242	0.01%	0.002%
50	9.377	2591	2593	2595	rVV	357	174	0.01%	0.001%
51	9.406	2599	2602	2604	rVB2	471	233	0.01%	0.002%
52	9.471	2619	2622	2626	rBV3	217	186	0.01%	0.001%
53	9.632	2669	2672	2673	rBV	239	120	0.01%	0.001%
54	9.664	2679	2682	2684	rBV2	217	97	0.01%	0.001%
55	9.677	2684	2686	2688	rBV	218	90	0.01%	0.001%
56	9.693	2688	2691	2692	rBV2	261	149	0.01%	0.001%
57	9.712	2695	2697	2701	rVV2	208	104	0.01%	0.001%
58	9.799	2722	2724	2728	rVB2	349	228	0.01%	0.002%
59	9.873	2744	2747	2752	rBV3	380	453	0.03%	0.003%
60	9.947	2767	2770	2773	rBV	195	131	0.01%	0.001%
61	9.963	2773	2775	2780	rVB2	294	169	0.01%	0.001%
62	10.059	2802	2805	2807	rBV	157	94	0.01%	0.001%
63	10.075	2807	2810	2814	rVV2	286	195	0.01%	0.001%
64	10.152	2822	2834	2859	rBV	565754	890137	50.69%	6.637%
65	10.426	2916	2919	2920	rBV2	198	110	0.01%	0.001%
66	10.439	2920	2923	2926	rVB2	408	258	0.01%	0.002%
67	10.516	2945	2947	2950	rVB2	444	158	0.01%	0.001%
68	10.558	2958	2960	2963	rVB	243	105	0.01%	0.001%
69	10.664	2991	2993	2997	rVB3	194	123	0.01%	0.001%
70	10.795	3031	3034	3039	rBV2	407	278	0.02%	0.002%
71	10.850	3049	3051	3053	rBV	278	154	0.01%	0.001%
72	10.963	3082	3086	3088	rBV	270	164	0.01%	0.001%
73	11.075	3118	3121	3123	rBV2	167	106	0.01%	0.001%
74	11.136	3132	3140	3144	rBV4	1131	1725	0.10%	0.013%
75	11.184	3144	3155	3182	rBV	787218	1247671	71.05%	9.303%
76	11.557	3260	3271	3300	rBV	707248	1129770	64.34%	8.424%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035441.D
Acq On : 26 Apr 2024 21:37
Operator : SY/MD
Sample : P2279-01 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Title : VOC Analysis

77	12.445	3544	3547	3550	rBV	338	277	0.02%	0.002%
78	12.586	3588	3591	3592	rBV2	627	367	0.02%	0.003%
79	12.824	3663	3665	3667	rBV	225	120	0.01%	0.001%
80	13.210	3781	3785	3791	rBV3	1874	2219	0.13%	0.017%
81	13.451	3848	3860	3876	rBV2	5895	12051	0.69%	0.090%




Sum of corrected areas: 13410818

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035441.D
Acq On : 26 Apr 2024 21:37
Operator : SY/MD
Sample : P2279-01 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

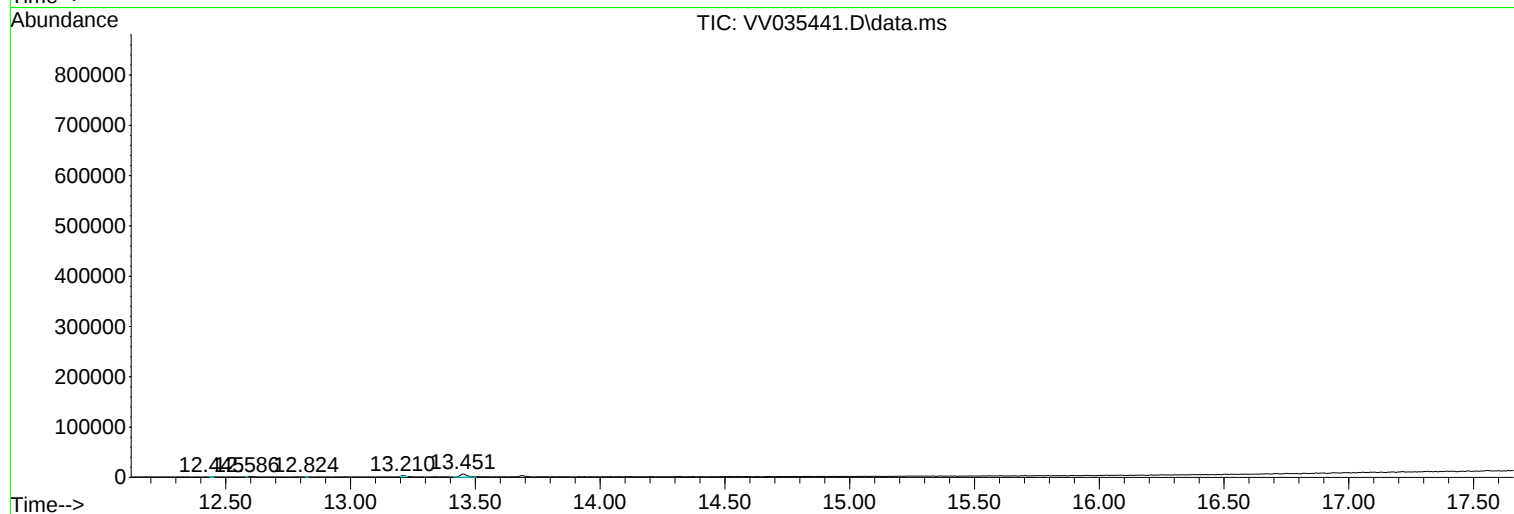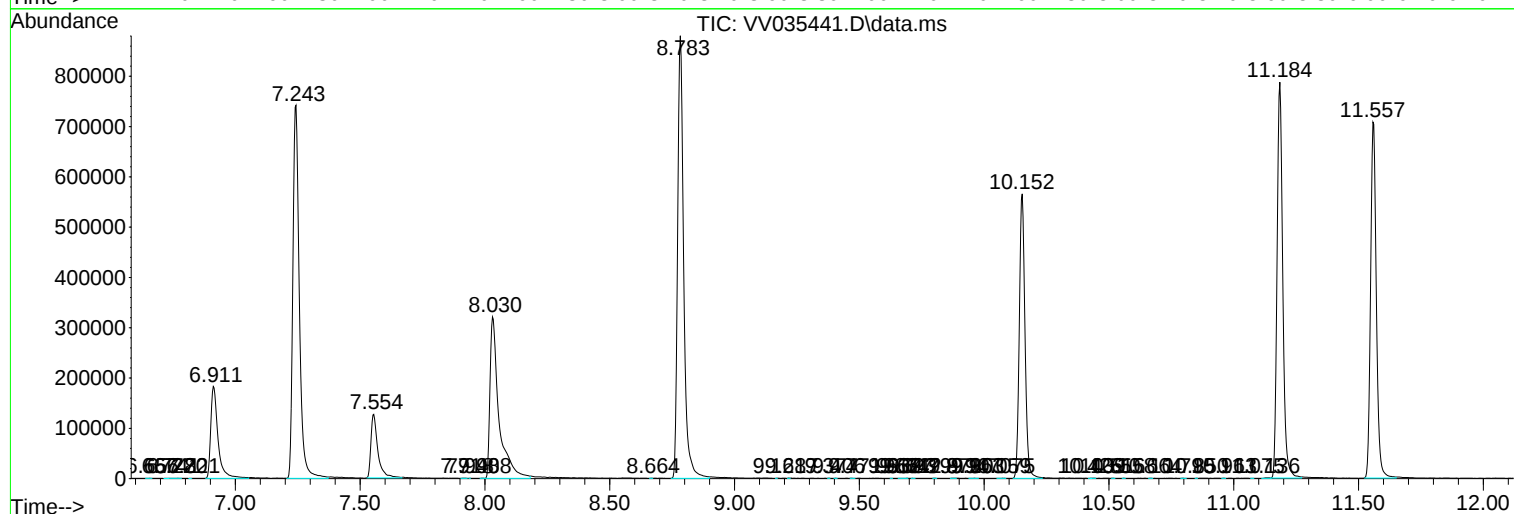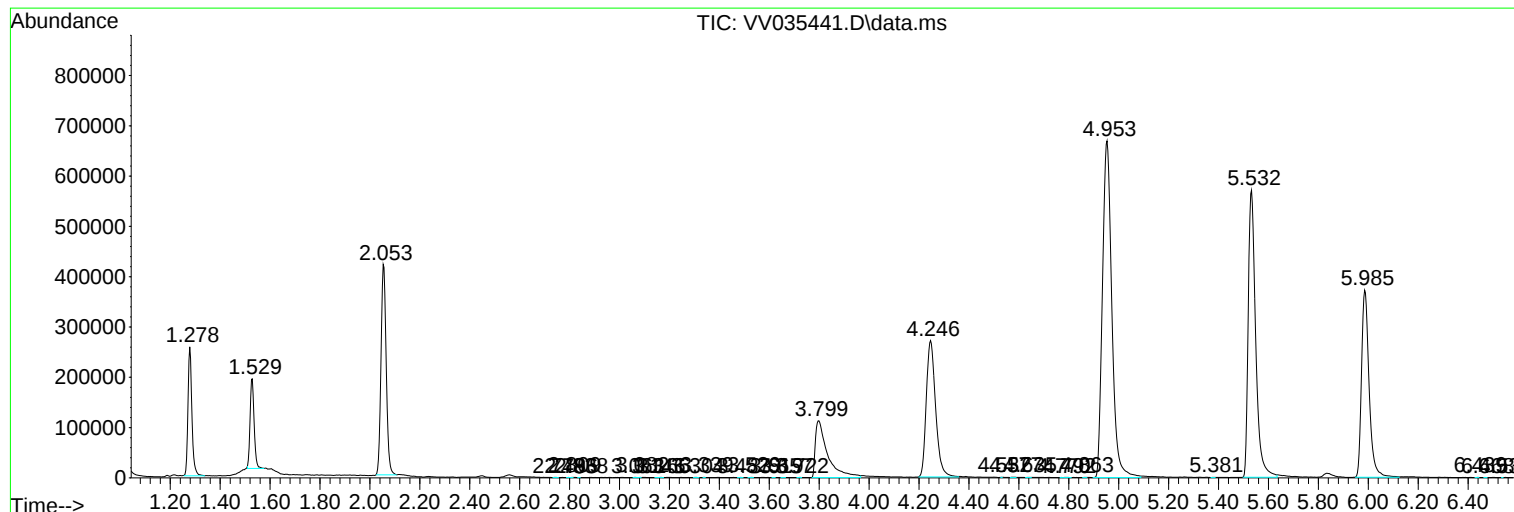

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035441.D
Acq On : 26 Apr 2024 21:37
Operator : SY/MD
Sample : P2279-01 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035441.D
Acq On : 26 Apr 2024 21:37
Operator : SY/MD
Sample : P2279-01 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc