

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035443.D
 Acq On : 26 Apr 2024 22:25
 Operator : SY/MD
 Sample : P2279-03 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035443.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	93	rVB	255454	278270	15.54%	2.099%
2	1.526	146	151	164	rVB	184242	204551	11.42%	1.543%
3	2.053	306	315	335	rBV	404546	587696	32.82%	4.433%
4	2.748	529	531	532	rBV	350	146	0.01%	0.001%
5	2.854	562	564	567	rVB2	283	126	0.01%	0.001%
6	2.963	594	598	601	rBV3	482	405	0.02%	0.003%
7	2.998	607	609	612	rVB3	379	223	0.01%	0.002%
8	3.027	616	618	621	rVB	266	111	0.01%	0.001%
9	3.130	648	650	656	rBV	311	242	0.01%	0.002%
10	3.297	698	702	704	rBV2	269	175	0.01%	0.001%
11	3.336	708	714	720	rBV3	462	574	0.03%	0.004%
12	3.487	759	761	764	rBV2	163	106	0.01%	0.001%
13	3.526	768	773	781	rBV3	313	431	0.02%	0.003%
14	3.564	781	785	787	rVB2	235	160	0.01%	0.001%
15	3.587	787	792	796	rBV2	258	243	0.01%	0.002%
16	3.632	796	806	811	rBV2	369	489	0.03%	0.004%
17	3.719	830	833	837	rBV	151	105	0.01%	0.001%
18	3.738	837	839	844	rVB	307	217	0.01%	0.002%
19	3.764	844	847	848	rBV	179	108	0.01%	0.001%
20	3.796	848	857	896	rBV	126109	415023	23.18%	3.130%
21	4.246	983	997	1036	rVB	277326	715966	39.99%	5.400%
22	4.558	1092	1094	1096	rBV2	528	319	0.02%	0.002%
23	4.629	1114	1116	1119	rVB2	360	203	0.01%	0.002%
24	4.953	1201	1217	1260	rBV2	677901	1790506	100.00%	13.505%
25	5.416	1359	1361	1363	rBV	277	156	0.01%	0.001%
26	5.532	1386	1397	1427	rBV	538739	1127673	62.98%	8.505%
27	5.985	1525	1538	1567	rBV	391952	813400	45.43%	6.135%
28	6.320	1639	1642	1645	rVB3	449	251	0.01%	0.002%
29	6.336	1645	1647	1650	rBV3	384	238	0.01%	0.002%
30	6.400	1666	1667	1670	rVB2	136	78	0.00%	0.001%
31	6.420	1670	1673	1676	rVB2	235	118	0.01%	0.001%
32	6.445	1679	1681	1682	rVB	195	60	0.00%	0.000%
33	6.497	1692	1697	1700	rBV3	186	151	0.01%	0.001%
34	6.513	1700	1702	1706	rVB	183	80	0.00%	0.001%
35	6.625	1733	1737	1739	rBV2	162	113	0.01%	0.001%
36	6.651	1743	1745	1747	rBV	147	56	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035443.D
 Acq On : 26 Apr 2024 22:25
 Operator : SY/MD
 Sample : P2279-03 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.661	1747	1748	1750	rVB	209	57	0.00%	0.000%
38	6.674	1750	1752	1755	rBV2	190	103	0.01%	0.001%
39	6.770	1780	1782	1784	rBV2	196	85	0.00%	0.001%
40	6.783	1784	1786	1788	rVB2	118	49	0.00%	0.000%
41	6.815	1793	1796	1797	rBV	238	116	0.01%	0.001%
42	6.911	1815	1826	1849	rBV	188799	365693	20.42%	2.758%
43	7.120	1888	1891	1894	rVB2	614	324	0.02%	0.002%
44	7.243	1918	1929	1961	rBV	728550	1292966	72.21%	9.752%
45	7.551	2016	2025	2053	rBV	129083	248413	13.87%	1.874%
46	7.847	2115	2117	2120	rBV2	284	142	0.01%	0.001%
47	7.879	2125	2127	2131	rVV3	373	203	0.01%	0.002%
48	7.921	2137	2140	2143	rVB2	418	279	0.02%	0.002%
49	7.940	2143	2146	2147	rBV	218	105	0.01%	0.001%
50	7.953	2147	2150	2153	rBV	214	210	0.01%	0.002%
51	7.998	2161	2164	2165	rBV	275	106	0.01%	0.001%
52	8.030	2165	2174	2225	rBV2	335501	843937	47.13%	6.365%
53	8.487	2314	2316	2319	rBV2	606	330	0.02%	0.002%
54	8.673	2373	2374	2377	rBV2	235	156	0.01%	0.001%
55	8.741	2393	2395	2397	rVB	236	77	0.00%	0.001%
56	8.783	2397	2408	2452	rBV	823619	1366192	76.30%	10.304%
57	9.127	2511	2515	2518	rBV	478	394	0.02%	0.003%
58	9.188	2531	2534	2536	rBV3	287	173	0.01%	0.001%
59	9.281	2562	2563	2565	rVB	413	148	0.01%	0.001%
60	9.374	2590	2592	2598	rBV2	230	171	0.01%	0.001%
61	9.471	2620	2622	2625	rVB	171	51	0.00%	0.000%
62	9.490	2625	2628	2631	rBV2	194	121	0.01%	0.001%
63	9.538	2642	2643	2644	rBV2	149	46	0.00%	0.000%
64	9.641	2672	2675	2679	rBV2	344	282	0.02%	0.002%
65	9.734	2702	2704	2706	rVB	216	74	0.00%	0.001%
66	9.751	2707	2709	2712	rBV2	243	119	0.01%	0.001%
67	9.780	2716	2718	2719	rBV	179	65	0.00%	0.000%
68	9.837	2731	2736	2741	rBV3	256	268	0.01%	0.002%
69	9.915	2758	2760	2762	rBV2	166	81	0.00%	0.001%
70	9.927	2762	2764	2765	rBV	192	84	0.00%	0.001%
71	10.024	2791	2794	2796	rBV2	233	156	0.01%	0.001%
72	10.037	2796	2798	2800	rVB	300	99	0.01%	0.001%
73	10.069	2805	2808	2810	rBV	198	90	0.01%	0.001%
74	10.152	2820	2834	2864	rBV	579219	936329	52.29%	7.062%
75	10.419	2914	2917	2921	rBV	299	177	0.01%	0.001%
76	10.435	2921	2922	2926	rVB	223	110	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035443.D
 Acq On : 26 Apr 2024 22:25
 Operator : SY/MD
 Sample : P2279-03 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	10.455	2926	2928	2930	rBV	155	58	0.00%	0.000%
78	10.493	2937	2940	2943	rVB2	312	258	0.01%	0.002%
79	10.516	2943	2947	2950	rBV	147	139	0.01%	0.001%
80	10.873	3053	3058	3059	rBV2	289	248	0.01%	0.002%
81	10.947	3079	3081	3085	rVB2	266	132	0.01%	0.001%
82	10.985	3091	3093	3095	rBV2	162	94	0.01%	0.001%
83	11.027	3104	3106	3107	rBV2	216	94	0.01%	0.001%
84	11.185	3144	3155	3184	rBV	720934	1141689	63.76%	8.611%
85	11.493	3247	3251	3255	rBV3	591	644	0.04%	0.005%
86	11.558	3259	3271	3301	rBV	694113	1111820	62.10%	8.386%
87	11.847	3359	3361	3363	rBV2	357	196	0.01%	0.001%
88	11.937	3386	3389	3392	rBV2	555	443	0.02%	0.003%
89	12.088	3434	3436	3439	rBV3	309	157	0.01%	0.001%
90	12.307	3501	3504	3506	rBV	379	234	0.01%	0.002%
91	12.905	3688	3690	3692	rBV2	497	290	0.02%	0.002%
92	13.451	3854	3860	3873	rBV3	2244	4500	0.25%	0.034%




Sum of corrected areas: 13258346

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035443.D
Acq On : 26 Apr 2024 22:25
Operator : SY/MD
Sample : P2279-03 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

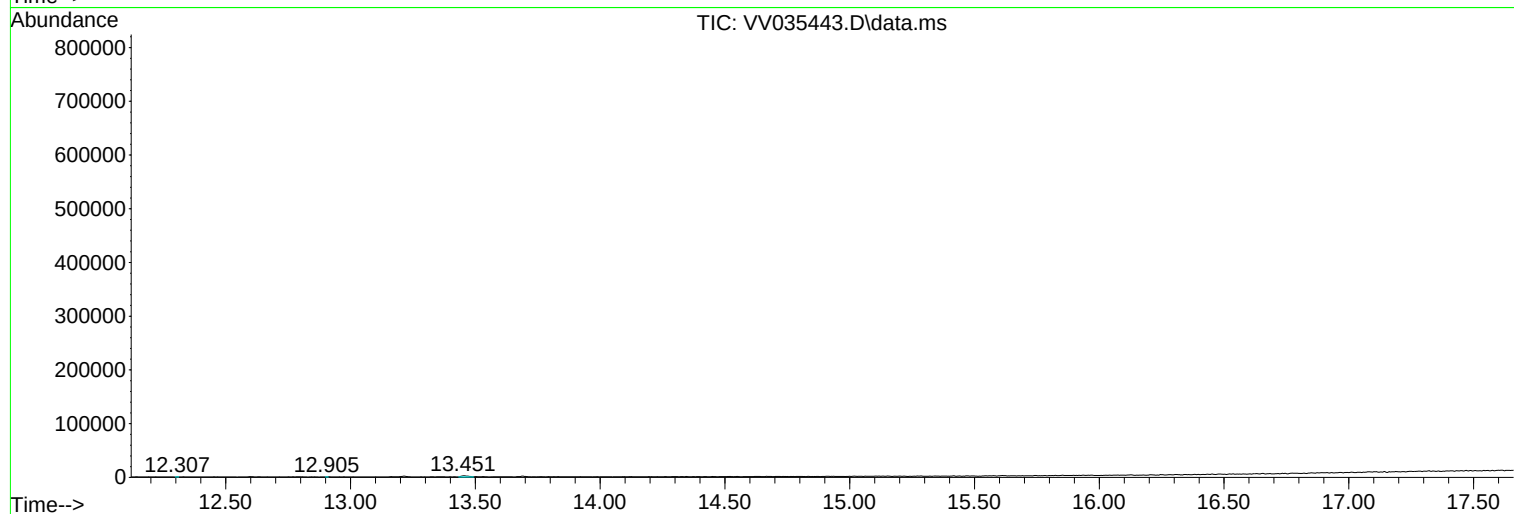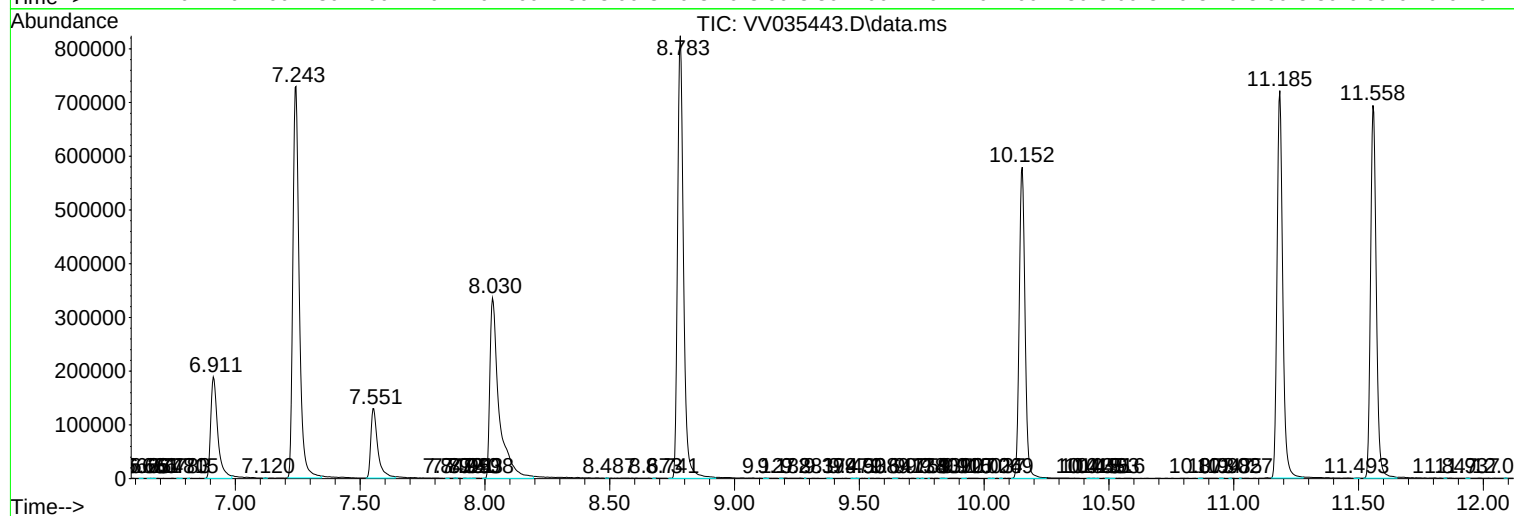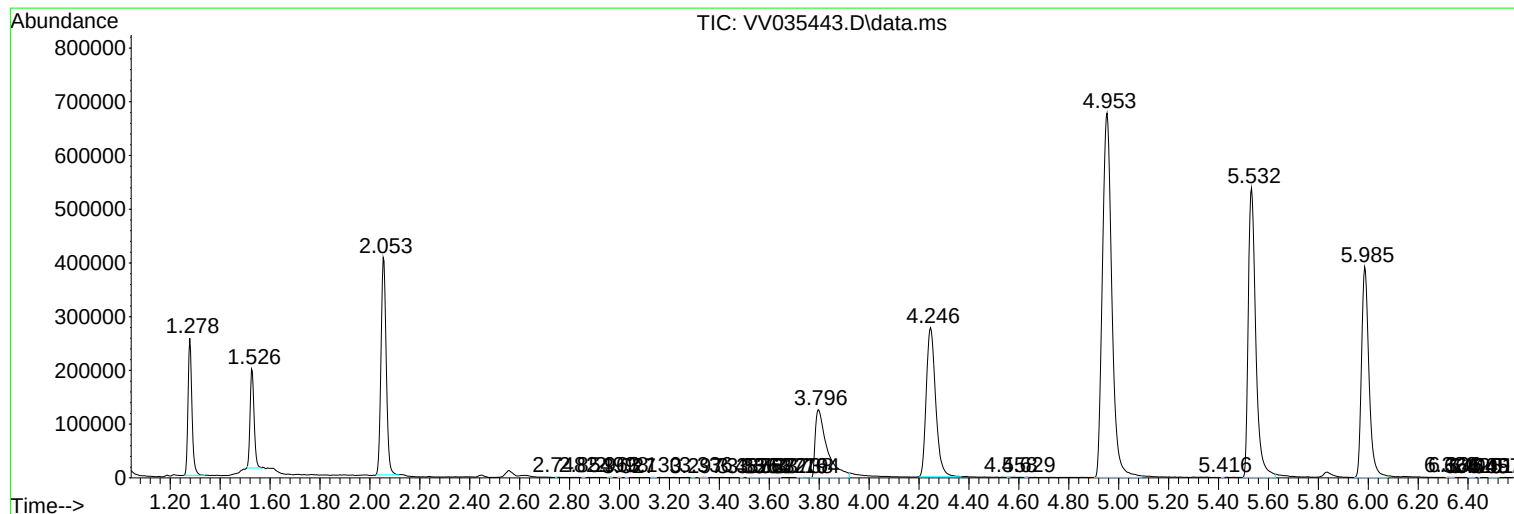

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035443.D
Acq On : 26 Apr 2024 22:25
Operator : SY/MD
Sample : P2279-03 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035443.D
Acq On : 26 Apr 2024 22:25
Operator : SY/MD
Sample : P2279-03 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------