

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035445.D
 Acq On : 26 Apr 2024 23:13
 Operator : SY/MD
 Sample : P2279-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M

Title : VOC Analysis

Signal : TIC: VV035445.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	93	rVB	252274	277406	15.76%	2.092%
2	1.529	146	152	165	rVB	173500	196785	11.18%	1.484%
3	2.053	306	315	331	rVB	412107	591699	33.62%	4.463%
4	2.282	383	386	390	rVB3	786	524	0.03%	0.004%
5	2.445	430	437	445	rVB2	2672	3899	0.22%	0.029%
6	2.851	559	563	564	rBV	235	160	0.01%	0.001%
7	2.880	570	572	574	rBV	287	106	0.01%	0.001%
8	2.908	579	581	583	rBV	215	127	0.01%	0.001%
9	3.021	613	616	618	rBV2	234	152	0.01%	0.001%
10	3.153	654	657	659	rBV2	177	116	0.01%	0.001%
11	3.169	659	662	666	rVV3	305	227	0.01%	0.002%
12	3.188	666	668	670	rVV	211	107	0.01%	0.001%
13	3.201	670	672	673	rVB	175	50	0.00%	0.000%
14	3.262	687	691	693	rBV	323	262	0.01%	0.002%
15	3.294	699	701	703	rBV	169	55	0.00%	0.000%
16	3.368	723	724	725	rBV	249	84	0.00%	0.001%
17	3.407	732	736	740	rBV3	264	234	0.01%	0.002%
18	3.490	760	762	769	rBV2	164	138	0.01%	0.001%
19	3.523	769	772	775	rBV3	336	314	0.02%	0.002%
20	3.587	789	792	796	rVB	212	136	0.01%	0.001%
21	3.661	813	815	818	rVB	150	74	0.00%	0.001%
22	3.683	818	822	823	rBV	152	98	0.01%	0.001%
23	3.728	834	836	837	rBV	188	68	0.00%	0.001%
24	3.799	849	858	919	rBV	114559	404993	23.01%	3.055%
25	4.246	982	997	1029	rBV	271059	700207	39.79%	5.281%
26	4.732	1146	1148	1152	rBV2	246	150	0.01%	0.001%
27	4.767	1156	1159	1160	rBV	254	175	0.01%	0.001%
28	4.953	1199	1217	1264	rBV2	670869	1759772	100.00%	13.273%
29	5.532	1386	1397	1429	rBV	554981	1166051	66.26%	8.795%
30	5.834	1482	1491	1517	rVB3	9849	22318	1.27%	0.168%
31	5.986	1525	1538	1575	rBV	377572	789535	44.87%	5.955%
32	6.339	1644	1648	1652	rBV3	543	395	0.02%	0.003%
33	6.359	1652	1654	1656	rVV	170	106	0.01%	0.001%
34	6.387	1660	1663	1667	rVB3	384	255	0.01%	0.002%
35	6.432	1674	1677	1680	rVB3	306	188	0.01%	0.001%
36	6.468	1686	1688	1690	rBV	293	123	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035445.D
 Acq On : 26 Apr 2024 23:13
 Operator : SY/MD
 Sample : P2279-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.481	1690	1692	1694	rVV2	246	115	0.01%	0.001%
38	6.506	1698	1700	1703	rBV	95	58	0.00%	0.000%
39	6.532	1706	1708	1710	rBV2	90	57	0.00%	0.000%
40	6.551	1710	1714	1717	rBV2	309	274	0.02%	0.002%
41	6.587	1723	1725	1728	rBV3	342	161	0.01%	0.001%
42	6.603	1728	1730	1733	rVB2	206	96	0.01%	0.001%
43	6.622	1734	1736	1739	rVB2	195	84	0.00%	0.001%
44	6.641	1739	1742	1743	rBV	169	80	0.00%	0.001%
45	6.754	1774	1777	1780	rBV2	105	64	0.00%	0.000%
46	6.773	1781	1783	1785	rVB	271	89	0.01%	0.001%
47	6.796	1788	1790	1792	rBV	155	48	0.00%	0.000%
48	6.912	1815	1826	1864	rBV	182123	360877	20.51%	2.722%
49	7.243	1918	1929	1972	rBV	732973	1312337	74.57%	9.898%
50	7.555	2016	2026	2051	rBV	127968	242300	13.77%	1.827%
51	7.863	2117	2122	2128	rBV3	503	634	0.04%	0.005%
52	7.937	2142	2145	2146	rBV	246	149	0.01%	0.001%
53	7.969	2153	2155	2158	rBV2	421	217	0.01%	0.002%
54	8.034	2164	2175	2221	rBV2	314099	799550	45.43%	6.030%
55	8.606	2350	2353	2354	rBV2	359	196	0.01%	0.001%
56	8.638	2361	2363	2365	rBV3	281	141	0.01%	0.001%
57	8.722	2387	2389	2393	rBV3	280	190	0.01%	0.001%
58	8.783	2397	2408	2436	rBV	847552	1414722	80.39%	10.670%
59	9.175	2526	2530	2531	rBV2	346	217	0.01%	0.002%
60	9.204	2538	2539	2542	rVB	256	96	0.01%	0.001%
61	9.246	2551	2552	2556	rVB	255	127	0.01%	0.001%
62	9.288	2563	2565	2568	rBV	237	157	0.01%	0.001%
63	9.310	2569	2572	2578	rVB4	407	358	0.02%	0.003%
64	9.346	2581	2583	2590	rVB3	330	211	0.01%	0.002%
65	9.400	2594	2600	2602	rBV2	277	265	0.02%	0.002%
66	9.577	2651	2655	2656	rBV	194	132	0.01%	0.001%
67	9.648	2675	2677	2682	rBV3	192	131	0.01%	0.001%
68	9.722	2697	2700	2705	rVB2	196	133	0.01%	0.001%
69	9.754	2705	2710	2715	rBV	347	351	0.02%	0.003%
70	9.792	2719	2722	2727	rBV2	215	263	0.01%	0.002%
71	9.918	2758	2761	2763	rBV2	140	96	0.01%	0.001%
72	10.001	2785	2787	2788	rBV	165	46	0.00%	0.000%
73	10.088	2811	2814	2817	rBV2	202	130	0.01%	0.001%
74	10.108	2817	2820	2822	rBV2	414	240	0.01%	0.002%
75	10.153	2822	2834	2863	rVV	558441	900966	51.20%	6.795%
76	10.407	2911	2913	2917	rBV	348	246	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035445.D
 Acq On : 26 Apr 2024 23:13
 Operator : SY/MD
 Sample : P2279-05 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	10.474	2932	2934	2938	rBV2	321	155	0.01%	0.001%
78	10.503	2941	2943	2945	rBV	191	82	0.00%	0.001%
79	10.574	2963	2965	2970	rBV	179	118	0.01%	0.001%
80	10.603	2971	2974	2977	rVV	199	122	0.01%	0.001%
81	10.648	2985	2988	2989	rBV	132	79	0.00%	0.001%
82	10.786	3029	3031	3033	rBV2	246	142	0.01%	0.001%
83	10.821	3039	3042	3047	rBV	232	219	0.01%	0.002%
84	10.857	3047	3053	3055	rBV2	401	409	0.02%	0.003%
85	10.927	3070	3075	3080	rBV2	372	515	0.03%	0.004%
86	11.008	3097	3100	3104	rBV	274	294	0.02%	0.002%
87	11.104	3128	3130	3133	rBV	187	96	0.01%	0.001%
88	11.185	3144	3155	3189	rBV	771307	1194774	67.89%	9.011%
89	11.497	3249	3252	3256	rBV3	465	389	0.02%	0.003%
90	11.558	3260	3271	3305	rVV	690671	1105016	62.79%	8.334%
91	11.924	3383	3385	3390	rBV2	256	241	0.01%	0.002%
92	12.181	3463	3465	3468	rVB2	327	133	0.01%	0.001%
93	12.400	3531	3533	3536	rBV2	271	171	0.01%	0.001%
94	12.558	3579	3582	3587	rBV	370	312	0.02%	0.002%
95	12.596	3590	3594	3597	rBV2	514	448	0.03%	0.003%
96	12.632	3603	3605	3606	rBV	305	94	0.01%	0.001%
97	12.860	3673	3676	3677	rBV2	275	166	0.01%	0.001%
98	13.066	3737	3740	3746	rBV3	494	410	0.02%	0.003%
99	13.162	3767	3770	3772	rBV2	313	215	0.01%	0.002%
100	13.204	3780	3783	3784	rBV3	635	356	0.02%	0.003%



Sum of corrected areas: 13258649

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035445.D
Acq On : 26 Apr 2024 23:13
Operator : SY/MD
Sample : P2279-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

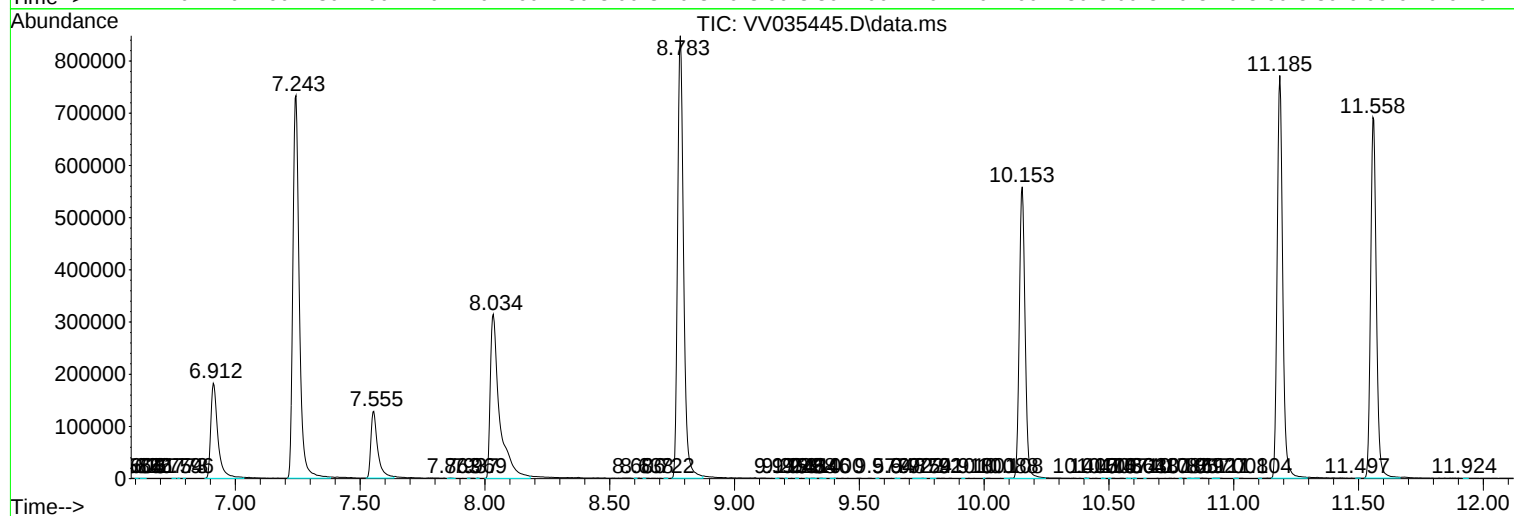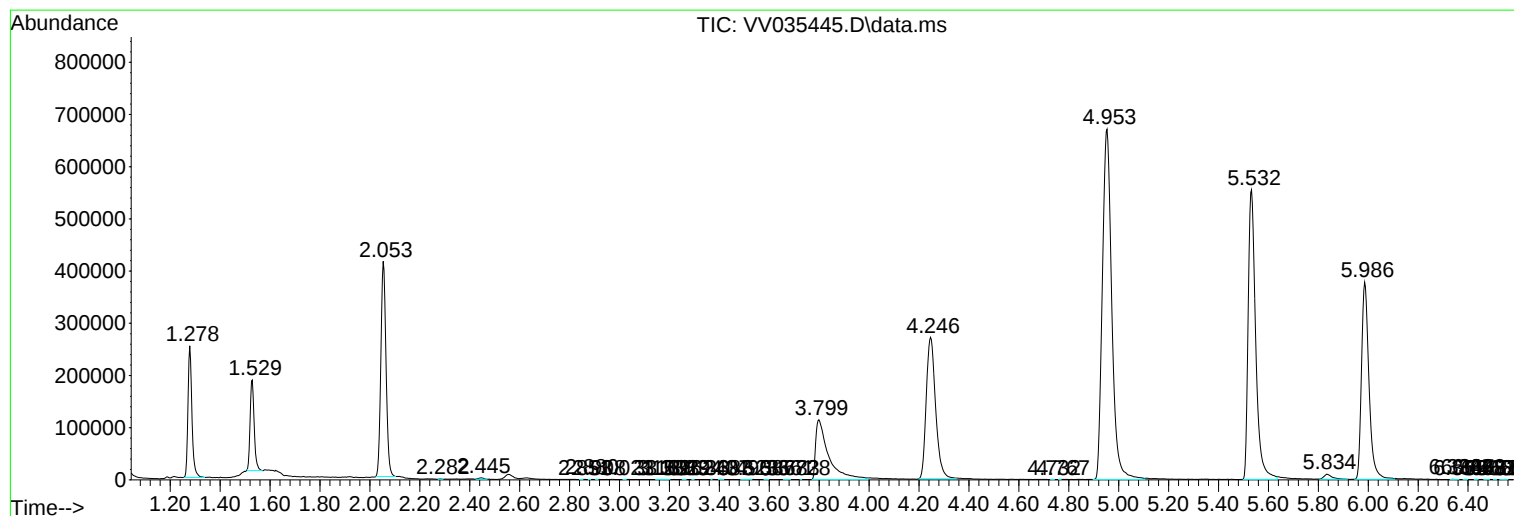

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035445.D
Acq On : 26 Apr 2024 23:13
Operator : SY/MD
Sample : P2279-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035445.D
Acq On : 26 Apr 2024 23:13
Operator : SY/MD
Sample : P2279-05 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc