

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035446.D
 Acq On : 26 Apr 2024 23:37
 Operator : SY/MD
 Sample : P2279-06 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035446.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	91	rVB	246006	266848	15.53%	2.085%
2	1.526	146	151	168	rVB	171016	193243	11.24%	1.510%
3	2.053	306	315	332	rVB	394586	567163	33.00%	4.431%
4	2.558	463	472	486	rBV	8192	16519	0.96%	0.129%
5	2.954	590	595	597	rBV2	274	281	0.02%	0.002%
6	3.021	614	616	620	rBV	261	163	0.01%	0.001%
7	3.044	621	623	625	rBV3	225	121	0.01%	0.001%
8	3.092	634	638	641	rBV	412	262	0.02%	0.002%
9	3.159	656	659	663	rBV2	343	319	0.02%	0.002%
10	3.185	665	667	670	rVV2	210	135	0.01%	0.001%
11	3.288	697	699	702	rBV	208	122	0.01%	0.001%
12	3.307	703	705	708	rVV2	220	134	0.01%	0.001%
13	3.323	708	710	712	rVV2	236	92	0.01%	0.001%
14	3.339	712	715	721	rVV2	239	262	0.02%	0.002%
15	3.397	728	733	737	rBV2	320	311	0.02%	0.002%
16	3.487	759	761	764	rVB	163	77	0.00%	0.001%
17	3.535	773	776	780	rBV3	249	196	0.01%	0.002%
18	3.606	796	798	799	rVB	155	36	0.00%	0.000%
19	3.622	799	803	807	rBV	170	151	0.01%	0.001%
20	3.642	808	809	811	rVB	85	34	0.00%	0.000%
21	3.706	826	829	832	rVB	355	203	0.01%	0.002%
22	3.725	832	835	836	rBV2	146	81	0.00%	0.001%
23	3.741	836	840	846	rVB2	199	199	0.01%	0.002%
24	3.799	849	858	903	rBV	115349	391733	22.79%	3.061%
25	4.246	981	997	1032	rBV	267051	697250	40.57%	5.448%
26	4.709	1139	1141	1145	rVB4	353	232	0.01%	0.002%
27	4.773	1158	1161	1164	rBV2	320	242	0.01%	0.002%
28	4.953	1201	1217	1253	rBV2	651250	1718806	100.00%	13.429%
29	5.429	1363	1365	1368	rVB	402	158	0.01%	0.001%
30	5.452	1368	1372	1375	rBV4	234	227	0.01%	0.002%
31	5.532	1386	1397	1433	rBV	526456	1099125	63.95%	8.588%
32	5.834	1483	1491	1513	rVB5	10114	25212	1.47%	0.197%
33	5.986	1525	1538	1577	rBV	372912	784657	45.65%	6.131%
34	6.317	1639	1641	1644	rVB2	325	131	0.01%	0.001%
35	6.333	1644	1646	1647	rVB2	237	67	0.00%	0.001%
36	6.349	1647	1651	1653	rBV2	337	275	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035446.D
 Acq On : 26 Apr 2024 23:37
 Operator : SY/MD
 Sample : P2279-06 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.445	1677	1681	1683	rBV3	254	177	0.01%	0.001%
38	6.503	1696	1699	1703	rVB2	326	175	0.01%	0.001%
39	6.574	1718	1721	1725	rBV	281	231	0.01%	0.002%
40	6.686	1753	1756	1758	rBV2	146	88	0.01%	0.001%
41	6.699	1758	1760	1764	rVV3	196	124	0.01%	0.001%
42	6.751	1774	1776	1778	rVB	311	122	0.01%	0.001%
43	6.764	1778	1780	1783	rBV	149	71	0.00%	0.001%
44	6.844	1801	1805	1809	rBV2	326	283	0.02%	0.002%
45	6.912	1816	1826	1863	rBV	178194	354896	20.65%	2.773%
46	7.243	1917	1929	1970	rBV	697510	1254033	72.96%	9.798%
47	7.551	2016	2025	2058	rBV	121517	238651	13.88%	1.865%
48	7.912	2133	2137	2140	rBB2	403	266	0.02%	0.002%
49	7.928	2140	2142	2144	rBV	384	135	0.01%	0.001%
50	7.976	2155	2157	2161	rBV	381	196	0.01%	0.002%
51	8.030	2165	2174	2217	rBV2	304892	792729	46.12%	6.194%
52	8.506	2320	2322	2326	rVB3	671	295	0.02%	0.002%
53	8.558	2335	2338	2341	rBV2	511	347	0.02%	0.003%
54	8.609	2352	2354	2356	rBV3	280	142	0.01%	0.001%
55	8.699	2380	2382	2386	rVB3	564	269	0.02%	0.002%
56	8.719	2386	2388	2391	rBV	327	183	0.01%	0.001%
57	8.738	2391	2394	2397	rBV2	344	277	0.02%	0.002%
58	8.783	2397	2408	2437	rBV	801143	1326559	77.18%	10.365%
59	9.281	2560	2563	2568	rVB3	431	267	0.02%	0.002%
60	9.313	2570	2573	2574	rBV	263	136	0.01%	0.001%
61	9.358	2584	2587	2589	rVB	314	125	0.01%	0.001%
62	9.407	2598	2602	2604	rBV2	334	255	0.01%	0.002%
63	9.500	2626	2631	2633	rBV	329	260	0.02%	0.002%
64	9.606	2662	2664	2665	rBV	186	62	0.00%	0.000%
65	9.674	2683	2685	2688	rVB	307	142	0.01%	0.001%
66	9.757	2709	2711	2717	rVB3	494	431	0.03%	0.003%
67	9.815	2723	2729	2731	rBV2	278	276	0.02%	0.002%
68	9.928	2762	2764	2765	rBV2	330	98	0.01%	0.001%
69	10.014	2789	2791	2792	rBV	153	50	0.00%	0.000%
70	10.153	2821	2834	2860	rBV	554800	899332	52.32%	7.027%
71	10.500	2939	2942	2944	rBV	300	133	0.01%	0.001%
72	10.513	2944	2946	2947	rBV2	247	76	0.00%	0.001%
73	10.558	2959	2960	2963	rVB	159	58	0.00%	0.000%
74	10.744	3016	3018	3020	rVB2	271	126	0.01%	0.001%
75	10.780	3027	3029	3030	rBV	148	43	0.00%	0.000%
76	10.796	3031	3034	3038	rVV2	392	285	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035446.D
 Acq On : 26 Apr 2024 23:37
 Operator : SY/MD
 Sample : P2279-06 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0RQ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M

Title : VOC Analysis

77	11.101	3127	3129	3132	rBV	235	118	0.01%	0.001%
78	11.185	3143	3155	3185	rBV	699352	1103864	64.22%	8.625%
79	11.490	3248	3250	3256	rVB4	366	228	0.01%	0.002%
80	11.558	3260	3271	3294	rBV	661639	1054618	61.36%	8.240%
81	11.886	3371	3373	3378	rBV2	487	320	0.02%	0.003%
82	12.062	3427	3428	3430	rBV	240	96	0.01%	0.001%
83	12.680	3618	3620	3623	rBV2	312	161	0.01%	0.001%
84	12.860	3674	3676	3679	rBV	269	168	0.01%	0.001%
85	13.217	3782	3787	3789	rBV3	746	720	0.04%	0.006%
86	13.548	3887	3890	3895	rBV3	535	540	0.03%	0.004%
87	14.480	4177	4180	4183	rBV	584	471	0.03%	0.004%




Sum of corrected areas: 12798775

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035446.D
Acq On : 26 Apr 2024 23:37
Operator : SY/MD
Sample : P2279-06 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

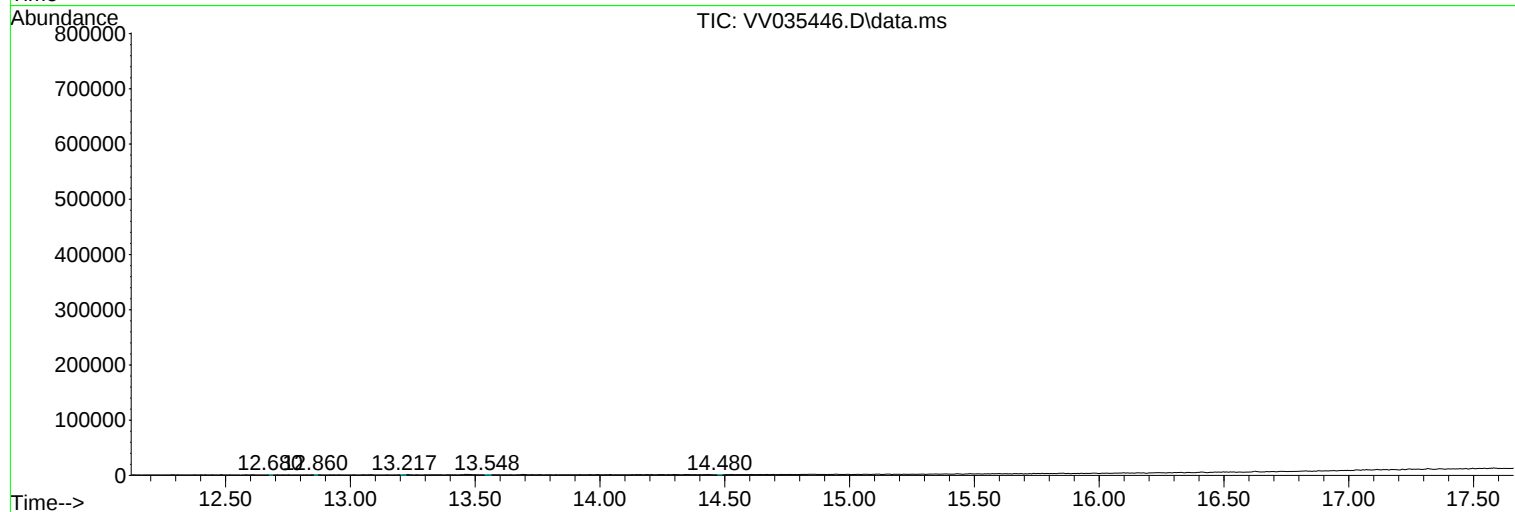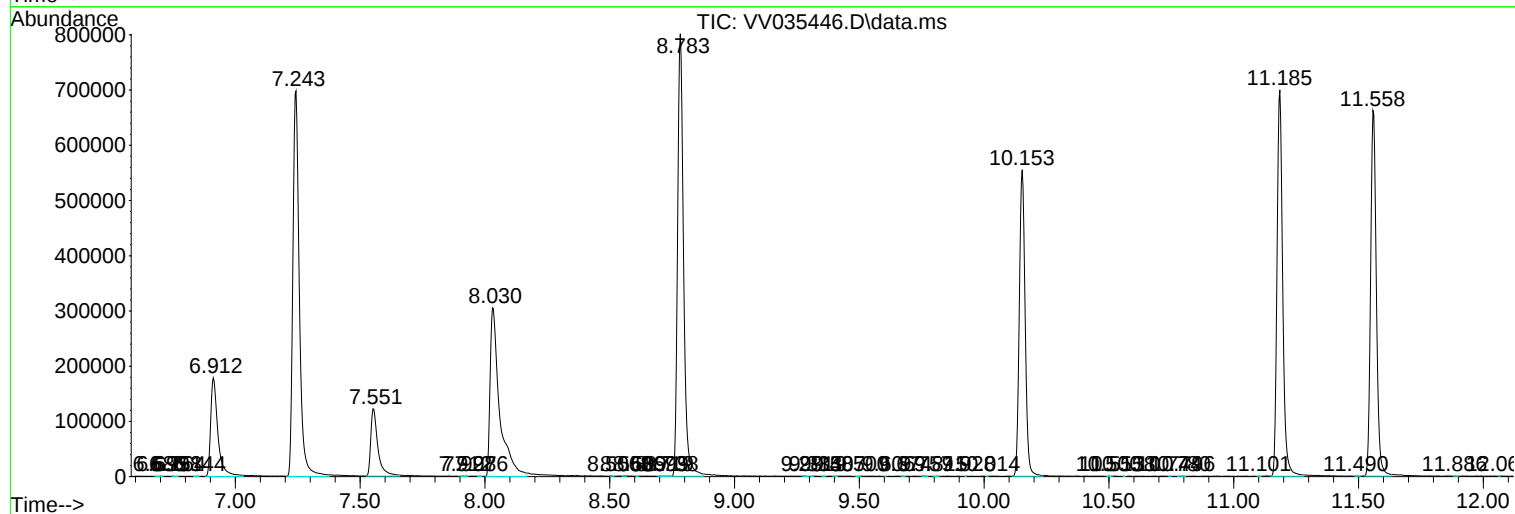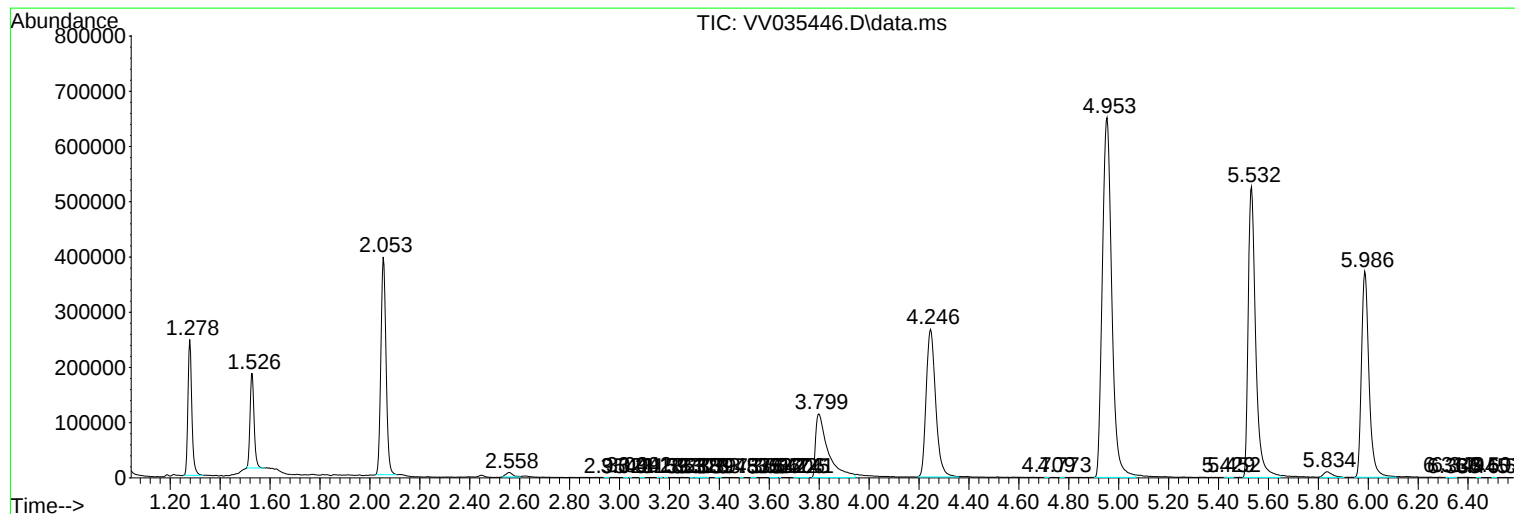

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035446.D
Acq On : 26 Apr 2024 23:37
Operator : SY/MD
Sample : P2279-06 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035446.D
Acq On : 26 Apr 2024 23:37
Operator : SY/MD
Sample : P2279-06 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RQ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------