

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035447.D
 Acq On : 27 Apr 2024 00:00
 Operator : SY/MD
 Sample : P2279-07 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035447.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	41	46	50	rBV	3483	3529	0.21%	0.028%
2	1.217	50	55	62	rVV2	2869	4140	0.25%	0.033%
3	1.278	67	74	88	rVB	233627	258711	15.59%	2.081%
4	1.529	145	152	167	rVB	164106	189443	11.42%	1.524%
5	2.053	305	315	334	rBV	375548	546773	32.95%	4.398%
6	2.230	369	370	373	rBV2	471	316	0.02%	0.003%
7	2.288	385	388	390	rBV3	523	316	0.02%	0.003%
8	2.446	431	437	447	rVB4	4079	6492	0.39%	0.052%
9	2.558	459	472	484	rBV	14347	31670	1.91%	0.255%
10	2.812	548	551	556	rVV	342	251	0.02%	0.002%
11	3.063	626	629	633	rBV3	420	205	0.01%	0.002%
12	3.098	637	640	645	rVB3	318	219	0.01%	0.002%
13	3.153	652	657	661	rBV2	249	201	0.01%	0.002%
14	3.188	661	668	671	rBV2	280	258	0.02%	0.002%
15	3.291	697	700	704	rBV2	340	271	0.02%	0.002%
16	3.526	768	773	777	rBV2	218	199	0.01%	0.002%
17	3.581	787	790	795	rVV	315	244	0.01%	0.002%
18	3.651	809	812	815	rVB	280	190	0.01%	0.002%
19	3.802	849	859	911	rBV	112442	406162	24.48%	3.267%
20	4.246	981	997	1030	rBV	260025	675273	40.70%	5.432%
21	4.571	1096	1098	1102	rVB2	336	229	0.01%	0.002%
22	4.597	1102	1106	1108	rBV3	313	209	0.01%	0.002%
23	4.703	1133	1139	1142	rBV	436	471	0.03%	0.004%
24	4.728	1145	1147	1151	rVV2	486	328	0.02%	0.003%
25	4.953	1200	1217	1254	rBV2	626222	1659333	100.00%	13.347%
26	5.198	1289	1293	1297	rBV4	685	624	0.04%	0.005%
27	5.278	1315	1318	1322	rBV2	279	199	0.01%	0.002%
28	5.388	1348	1352	1355	rBV4	308	235	0.01%	0.002%
29	5.494	1381	1385	1386	rBV2	378	229	0.01%	0.002%
30	5.532	1386	1397	1432	rBV	514071	1080742	65.13%	8.693%
31	5.757	1465	1467	1478	rVB4	1094	1329	0.08%	0.011%
32	5.838	1480	1492	1514	rVB3	8892	22778	1.37%	0.183%
33	5.986	1526	1538	1570	rBV	358678	755008	45.50%	6.073%
34	6.224	1609	1612	1615	rBV2	474	362	0.02%	0.003%
35	6.240	1615	1617	1619	rVB2	404	208	0.01%	0.002%
36	6.487	1692	1694	1699	rVB2	280	220	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042624\
 Data File : VW035447.D
 Acq On : 27 Apr 2024 00:00
 Operator : SY/MD
 Sample : P2279-07 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.551	1712	1714	1720	rVB2	304	263	0.02%	0.002%
38	6.687	1753	1756	1758	rBV2	275	190	0.01%	0.002%
39	6.912	1816	1826	1862	rBV	169391	341383	20.57%	2.746%
40	7.243	1917	1929	1958	rBV	664288	1185039	71.42%	9.532%
41	7.555	2017	2026	2055	rBV	120064	228754	13.79%	1.840%
42	7.838	2109	2114	2116	rBV3	380	338	0.02%	0.003%
43	7.889	2128	2130	2134	rVB	345	211	0.01%	0.002%
44	7.944	2144	2147	2149	rBV2	317	228	0.01%	0.002%
45	7.979	2154	2158	2161	rVB4	314	277	0.02%	0.002%
46	8.034	2165	2175	2215	rBV3	298633	774208	46.66%	6.228%
47	8.513	2322	2324	2328	rBV2	521	341	0.02%	0.003%
48	8.783	2397	2408	2439	rBV	787016	1301120	78.41%	10.466%
49	8.998	2473	2475	2479	rVB4	464	250	0.02%	0.002%
50	9.021	2479	2482	2485	rVB3	451	293	0.02%	0.002%
51	9.117	2510	2512	2515	rVB2	417	235	0.01%	0.002%
52	9.153	2520	2523	2525	rVB2	463	232	0.01%	0.002%
53	9.191	2532	2535	2537	rBV	305	224	0.01%	0.002%
54	9.249	2551	2553	2560	rVV2	303	291	0.02%	0.002%
55	9.281	2560	2563	2567	rVV2	618	380	0.02%	0.003%
56	9.320	2573	2575	2580	rVB3	337	280	0.02%	0.002%
57	9.349	2580	2584	2590	rBV4	296	321	0.02%	0.003%
58	9.410	2600	2603	2607	rVB	442	337	0.02%	0.003%
59	9.657	2677	2680	2682	rBV2	391	205	0.01%	0.002%
60	9.725	2697	2701	2708	rVV	272	198	0.01%	0.002%
61	9.886	2747	2751	2756	rBV	318	279	0.02%	0.002%
62	10.005	2784	2788	2791	rBV2	266	277	0.02%	0.002%
63	10.092	2811	2815	2819	rVB2	273	218	0.01%	0.002%
64	10.153	2819	2834	2861	rBV	543081	878209	52.93%	7.064%
65	10.288	2873	2876	2879	rBV3	396	219	0.01%	0.002%
66	10.381	2902	2905	2909	rVB2	542	395	0.02%	0.003%
67	10.439	2919	2923	2926	rVV3	327	264	0.02%	0.002%
68	10.461	2927	2930	2935	rVB	362	192	0.01%	0.002%
69	10.635	2981	2984	2987	rVB3	382	231	0.01%	0.002%
70	10.657	2987	2991	2994	rBV2	269	224	0.01%	0.002%
71	10.677	2994	2997	3000	rBV2	262	196	0.01%	0.002%
72	11.040	3108	3110	3115	rVB2	436	217	0.01%	0.002%
73	11.130	3135	3138	3142	rBV3	608	513	0.03%	0.004%
74	11.185	3143	3155	3183	rBV	685977	1064825	64.17%	8.565%
75	11.506	3252	3255	3259	rVB3	441	282	0.02%	0.002%
76	11.558	3259	3271	3293	rBV	620819	994390	59.93%	7.999%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035447.D
 Acq On : 27 Apr 2024 00:00
 Operator : SY/MD
 Sample : P2279-07 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	11.812	3347	3350	3354	rVV2	351	308	0.02%	0.002%
78	11.944	3388	3391	3395	rBV2	285	207	0.01%	0.002%
79	11.976	3398	3401	3406	rVB3	336	333	0.02%	0.003%
80	12.095	3433	3438	3440	rBV2	404	298	0.02%	0.002%
81	12.153	3453	3456	3457	rBV2	334	195	0.01%	0.002%
82	12.484	3556	3559	3563	rBV3	488	314	0.02%	0.003%
83	12.506	3563	3566	3569	rBV2	301	205	0.01%	0.002%
84	12.673	3615	3618	3621	rBV	413	230	0.01%	0.002%
85	12.718	3626	3632	3634	rBV3	301	310	0.02%	0.002%
86	12.895	3686	3687	3693	rVB2	458	320	0.02%	0.003%
87	12.927	3693	3697	3699	rBV2	500	423	0.03%	0.003%
88	13.217	3783	3787	3788	rBV	813	512	0.03%	0.004%
89	13.329	3819	3822	3827	rVB3	459	432	0.03%	0.003%
90	13.432	3852	3854	3857	rBV	411	263	0.02%	0.002%
91	13.458	3859	3862	3868	rVV4	633	551	0.03%	0.004%
92	13.680	3929	3931	3936	rBV3	483	395	0.02%	0.003%
93	13.824	3974	3976	3980	rBV3	352	234	0.01%	0.002%
94	13.847	3980	3983	3986	rVB2	311	220	0.01%	0.002%
95	14.368	4142	4145	4150	rVB3	801	639	0.04%	0.005%
96	14.503	4184	4187	4192	rVB3	462	323	0.02%	0.003%
97	14.525	4192	4194	4197	rBV2	394	231	0.01%	0.002%
98	14.689	4242	4245	4247	rBV2	708	398	0.02%	0.003%
99	14.783	4271	4274	4277	rBV2	645	513	0.03%	0.004%
100	14.812	4281	4283	4285	rVB3	671	321	0.02%	0.003%




Sum of corrected areas: 12432071

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035447.D
Acq On : 27 Apr 2024 00:00
Operator : SY/MD
Sample : P2279-07 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CORR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

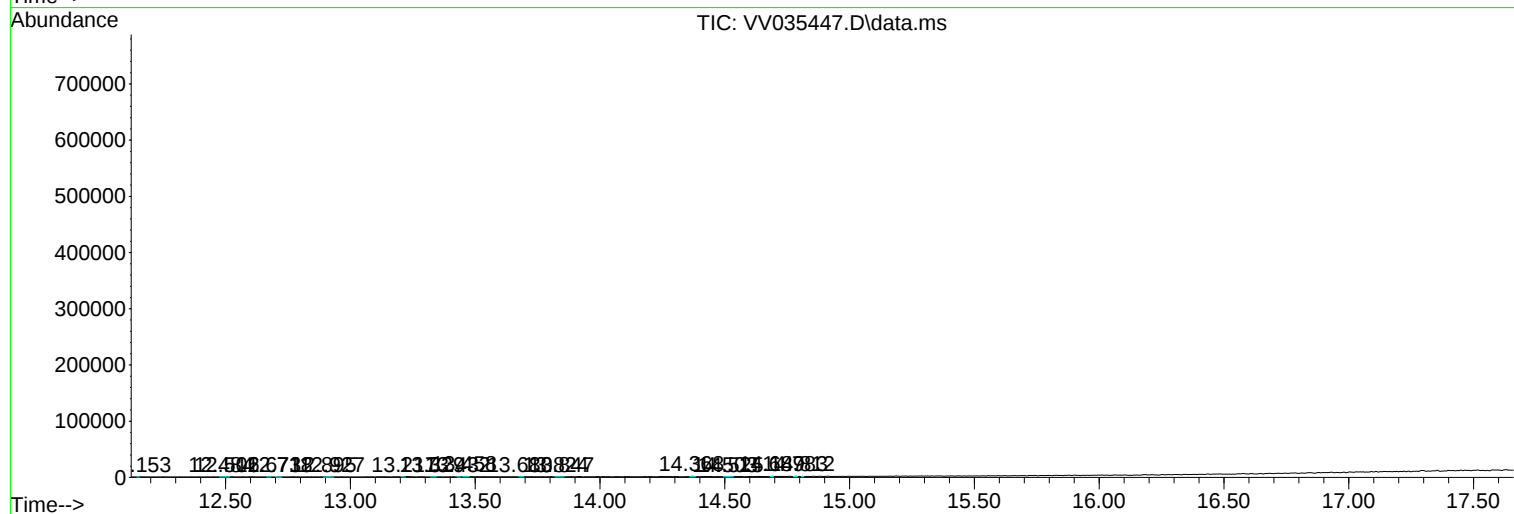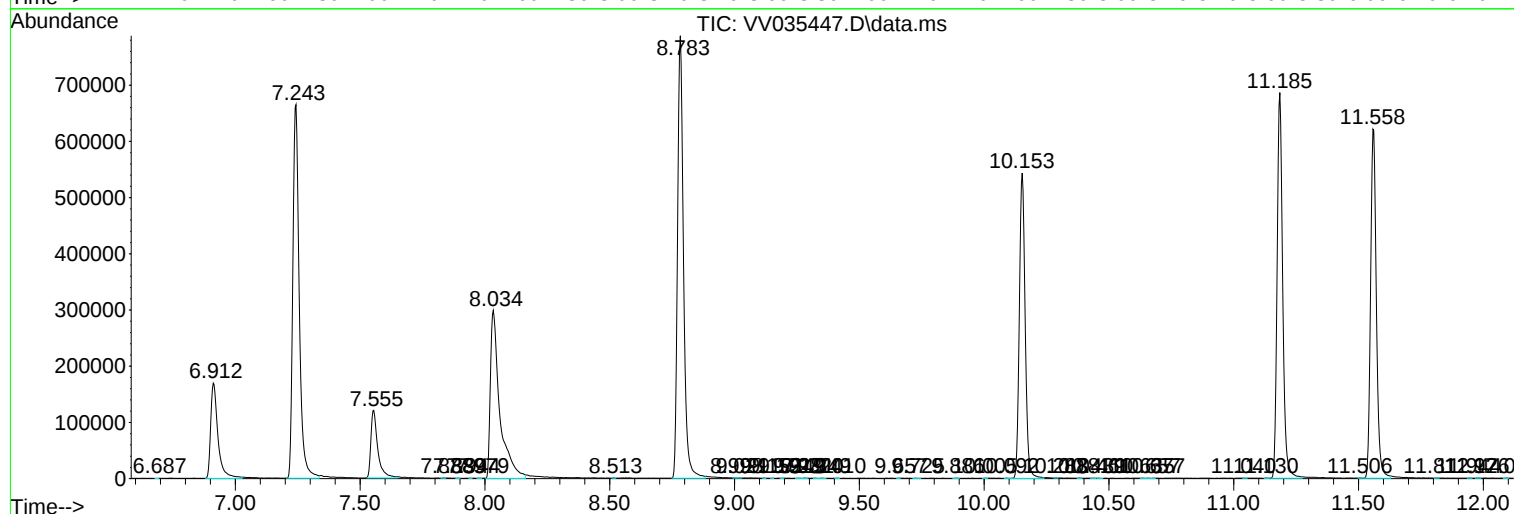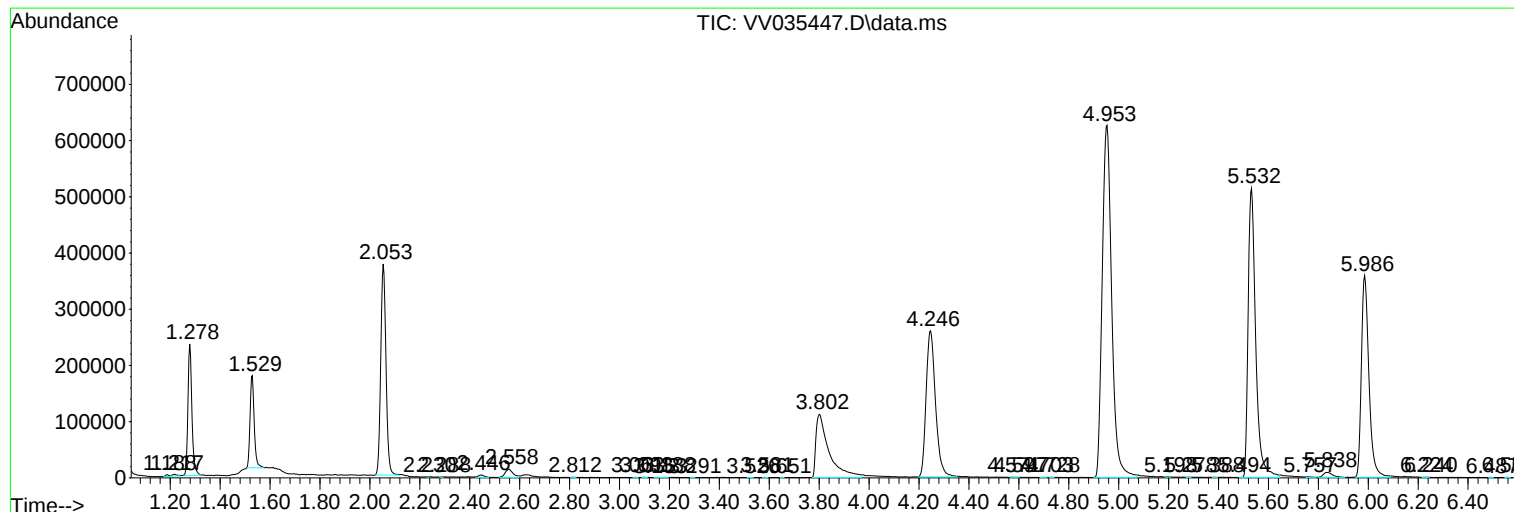

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035447.D
Acq On : 27 Apr 2024 00:00
Operator : SY/MD
Sample : P2279-07 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035447.D
Acq On : 27 Apr 2024 00:00
Operator : SY/MD
Sample : P2279-07 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------