

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035448.D
 Acq On : 27 Apr 2024 00:24
 Operator : SY/MD
 Sample : P2279-08 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035448.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	41	46	49	rBV	3481	3036	0.18%	0.024%
2	1.214	50	54	58	rBV2	2353	2622	0.16%	0.021%
3	1.278	67	74	96	rVB	236894	262673	15.89%	2.105%
4	1.526	145	151	161	rBV	161058	180397	10.91%	1.446%
5	2.053	305	315	332	rBV	374242	544141	32.91%	4.361%
6	2.449	430	438	449	rVB4	3104	5672	0.34%	0.045%
7	2.491	449	451	456	rBV	387	258	0.02%	0.002%
8	2.561	460	473	484	rBV	10471	24094	1.46%	0.193%
9	3.134	649	651	654	rVV	379	190	0.01%	0.002%
10	3.191	666	669	674	rVB3	296	271	0.02%	0.002%
11	3.359	718	721	725	rVV2	202	191	0.01%	0.002%
12	3.516	767	770	773	rBV	287	207	0.01%	0.002%
13	3.597	789	795	800	rBV2	335	231	0.01%	0.002%
14	3.645	806	810	812	rBV2	277	223	0.01%	0.002%
15	3.796	848	857	920	rBV	109483	395616	23.93%	3.170%
16	4.246	981	997	1034	rBV	259147	666384	40.30%	5.340%
17	4.548	1087	1091	1098	rBV3	345	371	0.02%	0.003%
18	4.953	1200	1217	1256	rBV2	627234	1653413	100.00%	13.250%
19	5.262	1311	1313	1318	rBV2	435	319	0.02%	0.003%
20	5.317	1328	1330	1334	rVB	452	274	0.02%	0.002%
21	5.375	1344	1348	1352	rVB4	449	274	0.02%	0.002%
22	5.394	1352	1354	1359	rVB3	755	435	0.03%	0.003%
23	5.423	1359	1363	1365	rBV	447	391	0.02%	0.003%
24	5.452	1369	1372	1377	rVB3	304	236	0.01%	0.002%
25	5.532	1385	1397	1431	rBV	524697	1104075	66.78%	8.848%
26	5.838	1480	1492	1505	rBV5	8734	20140	1.22%	0.161%
27	5.934	1519	1522	1523	rBV2	571	254	0.02%	0.002%
28	5.986	1523	1538	1576	rVV	362543	757954	45.84%	6.074%
29	6.204	1603	1606	1610	rBV3	388	259	0.02%	0.002%
30	6.249	1618	1620	1623	rBV2	496	239	0.01%	0.002%
31	6.281	1627	1630	1635	rVB5	474	517	0.03%	0.004%
32	6.310	1635	1639	1641	rBV	431	291	0.02%	0.002%
33	6.330	1641	1645	1649	rBV3	520	427	0.03%	0.003%
34	6.384	1660	1662	1667	rVB	461	345	0.02%	0.003%
35	6.433	1674	1677	1682	rVB2	446	278	0.02%	0.002%
36	6.481	1687	1692	1694	rBV	306	310	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042624\
 Data File : VW035448.D
 Acq On : 27 Apr 2024 00:24
 Operator : SY/MD
 Sample : P2279-08 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.523	1703	1705	1709	rVB2	315	214	0.01%	0.002%
38	6.912	1816	1826	1860	rBV	171555	338517	20.47%	2.713%
39	7.243	1918	1929	1957	rBV	657907	1178763	71.29%	9.446%
40	7.555	2016	2026	2052	rBV	116924	225031	13.61%	1.803%
41	7.873	2122	2125	2127	rBV2	212	194	0.01%	0.002%
42	7.918	2137	2139	2143	rBV2	308	208	0.01%	0.002%
43	8.031	2165	2174	2226	rBV4	290920	767251	46.40%	6.149%
44	8.355	2272	2275	2276	rBV3	715	304	0.02%	0.002%
45	8.490	2315	2317	2320	rBV4	259	197	0.01%	0.002%
46	8.555	2334	2337	2338	rBV	392	237	0.01%	0.002%
47	8.744	2392	2396	2397	rBV3	268	208	0.01%	0.002%
48	8.783	2397	2408	2449	rBV	812348	1339559	81.02%	10.735%
49	9.021	2480	2482	2487	rVB5	450	328	0.02%	0.003%
50	9.066	2494	2496	2500	rVB2	516	270	0.02%	0.002%
51	9.085	2500	2502	2504	rBV3	382	199	0.01%	0.002%
52	9.207	2536	2540	2542	rBV3	508	282	0.02%	0.002%
53	9.223	2542	2545	2547	rBV2	262	212	0.01%	0.002%
54	9.442	2609	2613	2614	rBV	439	243	0.01%	0.002%
55	9.555	2643	2648	2652	rBV	228	242	0.01%	0.002%
56	9.638	2671	2674	2679	rVB2	261	227	0.01%	0.002%
57	9.883	2749	2750	2755	rVB2	271	193	0.01%	0.002%
58	10.153	2822	2834	2863	rBV	544745	867334	52.46%	6.951%
59	10.329	2886	2889	2891	rBV2	268	192	0.01%	0.002%
60	10.387	2905	2907	2910	rVB2	403	226	0.01%	0.002%
61	10.416	2910	2916	2919	rBV3	426	393	0.02%	0.003%
62	10.616	2974	2978	2981	rBV2	288	272	0.02%	0.002%
63	10.709	3003	3007	3013	rVB	379	270	0.02%	0.002%
64	10.747	3013	3019	3020	rBV2	425	343	0.02%	0.003%
65	10.815	3038	3040	3043	rBV	244	196	0.01%	0.002%
66	11.136	3136	3140	3143	rBV3	545	497	0.03%	0.004%
67	11.185	3143	3155	3184	rBV	691807	1104491	66.80%	8.851%
68	11.558	3259	3271	3301	rBV	625494	1006997	60.90%	8.070%
69	11.786	3338	3342	3345	rVB3	659	581	0.04%	0.005%
70	11.828	3352	3355	3360	rVB4	665	531	0.03%	0.004%
71	11.882	3370	3372	3376	rVB3	267	202	0.01%	0.002%
72	12.011	3408	3412	3414	rBV2	459	299	0.02%	0.002%
73	12.095	3434	3438	3440	rBV2	307	224	0.01%	0.002%
74	12.185	3463	3466	3468	rBV	321	260	0.02%	0.002%
75	12.288	3495	3498	3501	rVV	299	218	0.01%	0.002%
76	12.345	3512	3516	3521	rBV2	366	253	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035448.D
 Acq On : 27 Apr 2024 00:24
 Operator : SY/MD
 Sample : P2279-08 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	12.413	3534	3537	3541	rBV	280	262	0.02%	0.002%
78	12.558	3578	3582	3586	rVB3	284	246	0.01%	0.002%
79	12.776	3648	3650	3656	rVB2	360	294	0.02%	0.002%
80	12.808	3656	3660	3663	rBV2	221	244	0.01%	0.002%
81	13.021	3722	3726	3729	rBV2	280	262	0.02%	0.002%
82	13.104	3747	3752	3755	rVB2	269	206	0.01%	0.002%
83	13.220	3783	3788	3794	rVB2	740	770	0.05%	0.006%
84	13.246	3794	3796	3799	rBV2	419	235	0.01%	0.002%
85	13.323	3816	3820	3825	rBV2	462	441	0.03%	0.004%
86	13.378	3835	3837	3840	rVB	515	236	0.01%	0.002%
87	13.397	3840	3843	3846	rBV	294	221	0.01%	0.002%
88	13.448	3856	3859	3860	rBV	368	207	0.01%	0.002%
89	13.593	3902	3904	3905	rBV	498	214	0.01%	0.002%
90	13.683	3930	3932	3936	rBV2	486	438	0.03%	0.004%
91	13.976	4020	4023	4025	rBV2	334	239	0.01%	0.002%
92	13.995	4027	4029	4031	rBV2	356	195	0.01%	0.002%
93	14.101	4060	4062	4067	rVB2	534	381	0.02%	0.003%
94	14.265	4111	4113	4116	rVB3	444	285	0.02%	0.002%
95	14.387	4148	4151	4155	rBV4	527	404	0.02%	0.003%
96	14.506	4183	4188	4190	rBV2	447	418	0.03%	0.003%
97	14.554	4199	4203	4205	rBV3	415	382	0.02%	0.003%
98	14.847	4292	4294	4300	rVB3	683	506	0.03%	0.004%
99	15.143	4382	4386	4388	rBV4	661	483	0.03%	0.004%
100	16.156	4697	4701	4708	rVB	8559	7127	0.43%	0.057%




Sum of corrected areas: 12478362

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035448.D
Acq On : 27 Apr 2024 00:24
Operator : SY/MD
Sample : P2279-08 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CORR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

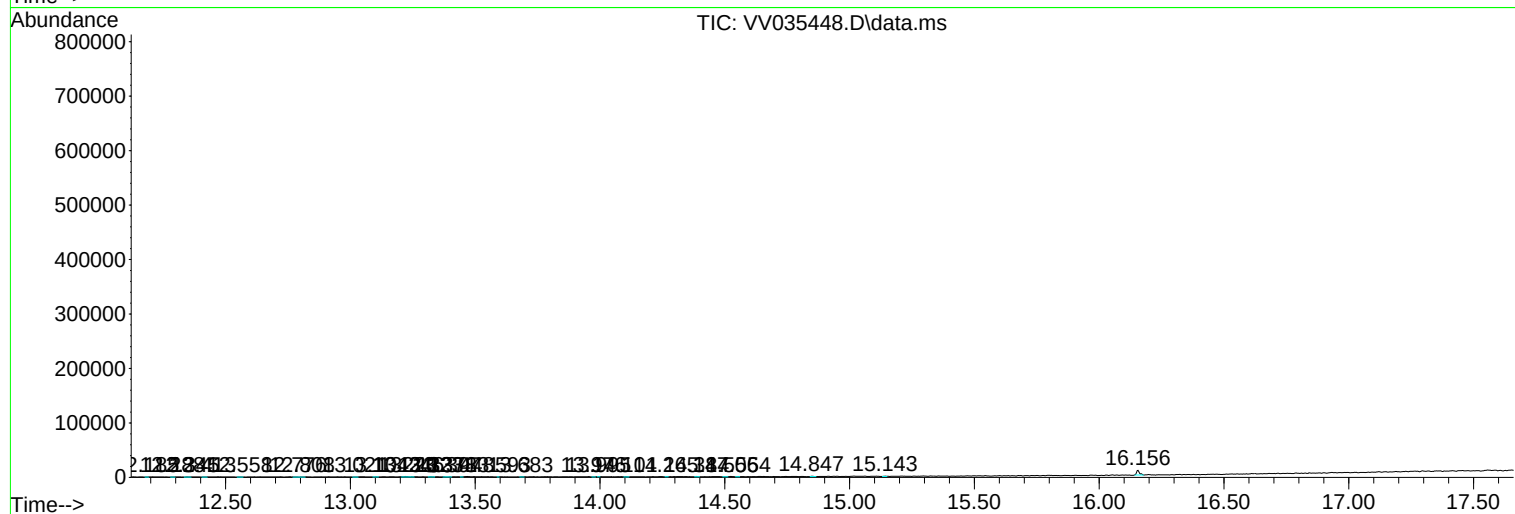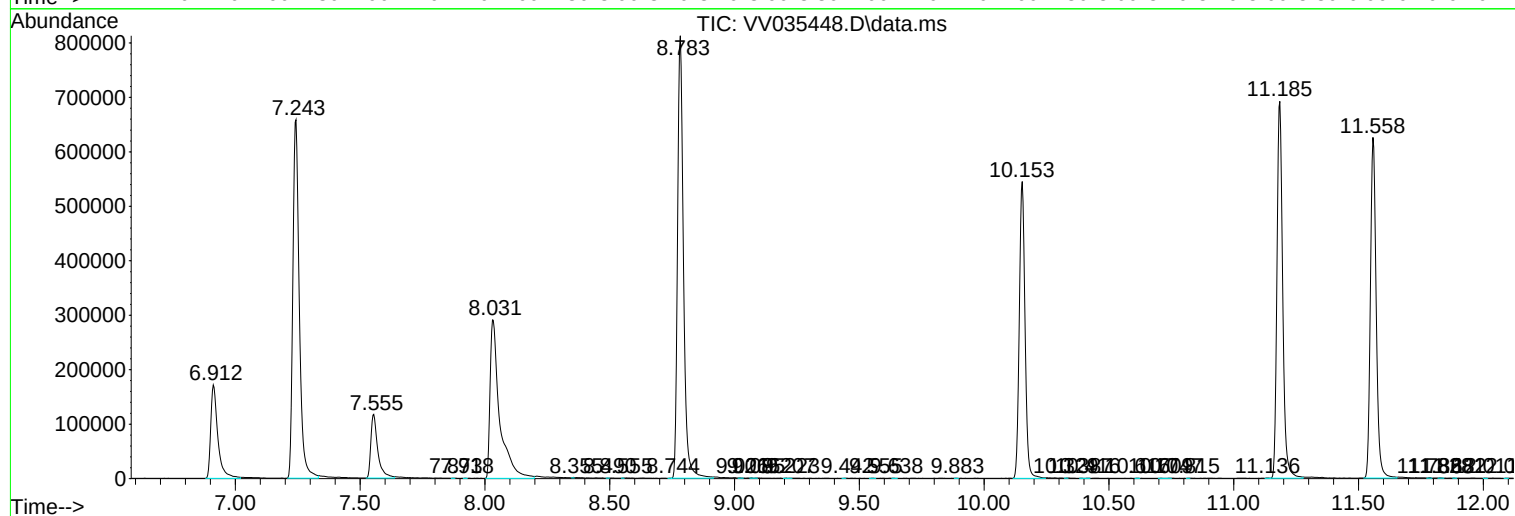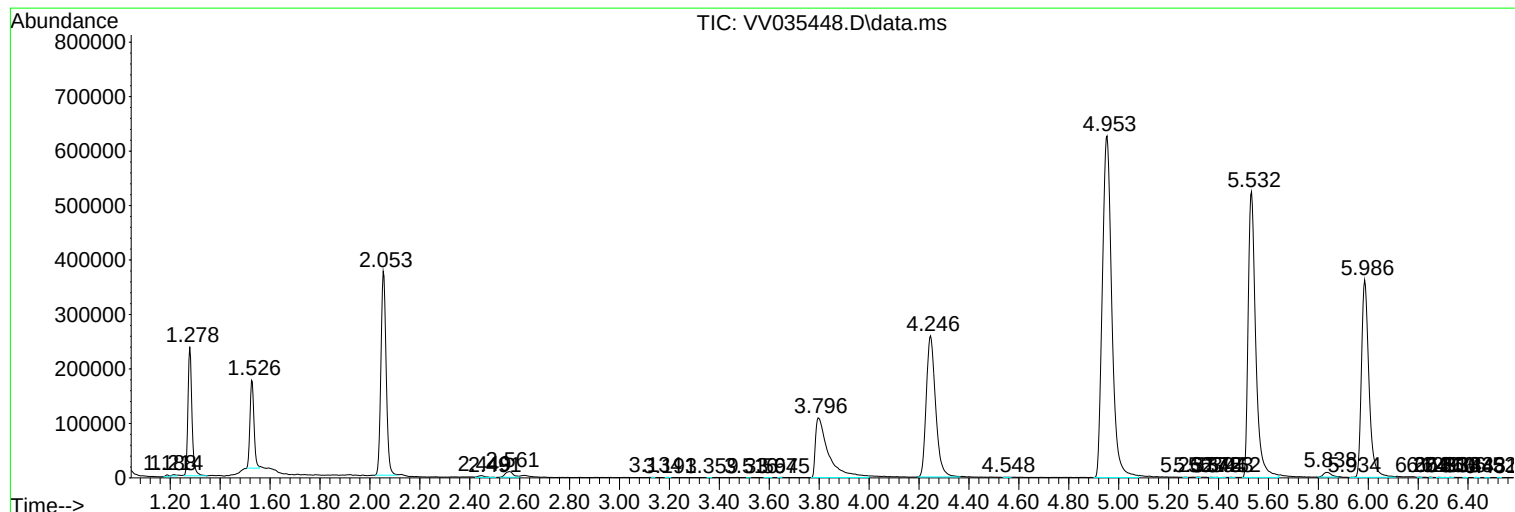

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035448.D
Acq On : 27 Apr 2024 00:24
Operator : SY/MD
Sample : P2279-08 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035448.D
Acq On : 27 Apr 2024 00:24
Operator : SY/MD
Sample : P2279-08 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc