

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035449.D
 Acq On : 27 Apr 2024 00:48
 Operator : SY/MD
 Sample : P2279-09 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M

Title : VOC Analysis

Signal : TIC: VV035449.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	42	46	50	rBV	2487	2568	0.16%	0.021%
2	1.278	67	74	92	rVB	239403	256276	15.67%	2.098%
3	1.529	145	152	166	rBV	158879	182387	11.16%	1.493%
4	2.053	304	315	333	rBV	369931	542665	33.19%	4.442%
5	2.233	369	371	373	rBV	433	174	0.01%	0.001%
6	2.297	389	391	394	rBV2	479	283	0.02%	0.002%
7	2.336	400	403	406	rBV3	408	337	0.02%	0.003%
8	2.445	431	437	447	rVB3	3397	5219	0.32%	0.043%
9	2.555	457	471	484	rBV2	10921	26509	1.62%	0.217%
10	2.989	603	606	610	rVB2	293	218	0.01%	0.002%
11	3.310	702	706	708	rBV2	382	250	0.02%	0.002%
12	3.387	727	730	735	rVB2	299	233	0.01%	0.002%
13	3.442	740	747	751	rVB3	334	382	0.02%	0.003%
14	3.519	766	771	775	rBV3	337	316	0.02%	0.003%
15	3.574	787	788	793	rVB2	297	182	0.01%	0.001%
16	3.613	793	800	807	rBV3	419	709	0.04%	0.006%
17	3.699	824	827	831	rBV3	334	240	0.01%	0.002%
18	3.754	841	844	848	rBV2	251	243	0.01%	0.002%
19	3.799	848	858	908	rBV	111318	391778	23.96%	3.207%
20	4.191	975	980	981	rBV2	530	518	0.03%	0.004%
21	4.246	981	997	1035	rVV	255490	665291	40.69%	5.446%
22	4.641	1117	1120	1122	rBV2	344	241	0.01%	0.002%
23	4.741	1146	1151	1152	rBV	373	317	0.02%	0.003%
24	4.831	1176	1179	1182	rVV4	282	196	0.01%	0.002%
25	4.953	1201	1217	1252	rBV2	619052	1634984	100.00%	13.383%
26	5.285	1318	1320	1323	rVB3	486	234	0.01%	0.002%
27	5.346	1336	1339	1341	rVV3	255	178	0.01%	0.001%
28	5.423	1361	1363	1367	rBV2	350	251	0.02%	0.002%
29	5.448	1369	1371	1373	rBV2	303	174	0.01%	0.001%
30	5.532	1386	1397	1438	rBV	500155	1051568	64.32%	8.607%
31	5.838	1481	1492	1507	rBV5	9477	20848	1.28%	0.171%
32	5.944	1519	1525	1526	rBV3	325	285	0.02%	0.002%
33	5.985	1526	1538	1574	rVV	360853	745356	45.59%	6.101%
34	6.194	1601	1603	1605	rBV2	439	222	0.01%	0.002%
35	6.371	1654	1658	1659	rBV2	350	230	0.01%	0.002%
36	6.574	1717	1721	1725	rVB2	254	203	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035449.D
 Acq On : 27 Apr 2024 00:48
 Operator : SY/MD
 Sample : P2279-09 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.616	1730	1734	1736	rBV	262	236	0.01%	0.002%
38	6.911	1816	1826	1862	rBV	170683	337003	20.61%	2.758%
39	7.140	1894	1897	1899	rBV	293	240	0.01%	0.002%
40	7.188	1909	1912	1916	rBV3	361	297	0.02%	0.002%
41	7.243	1916	1929	1966	rBV	644447	1164078	71.20%	9.528%
42	7.555	2016	2026	2063	rBV	116106	224630	13.74%	1.839%
43	7.747	2084	2086	2092	rVB4	540	417	0.03%	0.003%
44	7.834	2110	2113	2117	rVB4	367	282	0.02%	0.002%
45	7.870	2122	2124	2126	rVB2	443	205	0.01%	0.002%
46	7.915	2132	2138	2143	rBV4	365	437	0.03%	0.004%
47	7.963	2151	2153	2155	rVB	335	170	0.01%	0.001%
48	7.982	2155	2159	2162	rBV2	377	290	0.02%	0.002%
49	8.034	2165	2175	2220	rBV3	292400	760201	46.50%	6.222%
50	8.362	2275	2277	2284	rBV3	437	669	0.04%	0.005%
51	8.413	2288	2293	2301	rVB5	668	900	0.06%	0.007%
52	8.461	2307	2308	2313	rVB3	567	304	0.02%	0.002%
53	8.500	2316	2320	2323	rBV2	405	379	0.02%	0.003%
54	8.554	2335	2337	2339	rBV	365	181	0.01%	0.001%
55	8.599	2350	2351	2354	rVB3	454	228	0.01%	0.002%
56	8.619	2354	2357	2360	rBV2	383	259	0.02%	0.002%
57	8.706	2381	2384	2387	rBV2	379	256	0.02%	0.002%
58	8.783	2397	2408	2450	rBV	763763	1271009	77.74%	10.403%
59	9.008	2475	2478	2481	rBV3	507	361	0.02%	0.003%
60	9.069	2495	2497	2501	rBV3	493	321	0.02%	0.003%
61	9.178	2529	2531	2534	rVB2	356	196	0.01%	0.002%
62	9.198	2534	2537	2540	rBV3	390	313	0.02%	0.003%
63	9.214	2540	2542	2546	rBV3	348	267	0.02%	0.002%
64	9.278	2558	2562	2564	rBV2	316	241	0.01%	0.002%
65	9.516	2633	2636	2638	rBV	336	190	0.01%	0.002%
66	9.532	2639	2641	2645	rVV	310	209	0.01%	0.002%
67	9.554	2645	2648	2651	rVV	325	223	0.01%	0.002%
68	9.599	2659	2662	2670	rVV2	201	267	0.02%	0.002%
69	9.651	2674	2678	2679	rVV2	290	188	0.01%	0.002%
70	9.950	2765	2771	2774	rBV2	349	307	0.02%	0.003%
71	10.101	2815	2818	2821	rBV2	303	214	0.01%	0.002%
72	10.152	2821	2834	2862	rVV	533139	862177	52.73%	7.057%
73	10.333	2888	2890	2893	rVB2	349	190	0.01%	0.002%
74	10.654	2986	2990	2994	rBV	313	314	0.02%	0.003%
75	10.754	3016	3021	3028	rVB3	400	417	0.03%	0.003%
76	11.088	3121	3125	3129	rBV	209	184	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035449.D
 Acq On : 27 Apr 2024 00:48
 Operator : SY/MD
 Sample : P2279-09 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	11.185	3144	3155	3184	rBV	662693	1054541	64.50%	8.632%
78	11.397	3219	3221	3223	rBV2	363	207	0.01%	0.002%
79	11.484	3246	3248	3250	rBV	405	229	0.01%	0.002%
80	11.558	3259	3271	3299	rBV	613600	993419	60.76%	8.131%
81	11.863	3363	3366	3369	rBV3	419	257	0.02%	0.002%
82	11.908	3373	3380	3382	rBV2	385	459	0.03%	0.004%
83	12.040	3419	3421	3423	rVV	371	215	0.01%	0.002%
84	12.082	3432	3434	3439	rVB3	516	335	0.02%	0.003%
85	12.127	3439	3448	3451	rBV4	403	510	0.03%	0.004%
86	12.213	3474	3475	3483	rVB3	282	248	0.02%	0.002%
87	12.268	3488	3492	3495	rBV	477	311	0.02%	0.003%
88	12.496	3560	3563	3565	rBV	420	336	0.02%	0.003%
89	12.583	3588	3590	3593	rVB2	386	217	0.01%	0.002%
90	12.606	3593	3597	3599	rBV2	524	335	0.02%	0.003%
91	12.622	3599	3602	3606	rVB	290	262	0.02%	0.002%
92	12.760	3642	3645	3647	rVB2	356	197	0.01%	0.002%
93	12.847	3668	3672	3677	rBV2	378	378	0.02%	0.003%
94	13.117	3752	3756	3759	rBV	383	345	0.02%	0.003%
95	13.284	3806	3808	3811	rBV2	299	198	0.01%	0.002%
96	13.326	3816	3821	3826	rBV4	316	469	0.03%	0.004%
97	13.644	3918	3920	3925	rVB	448	314	0.02%	0.003%
98	13.693	3931	3935	3941	rBV3	755	850	0.05%	0.007%
99	14.689	4243	4245	4251	rVB3	656	357	0.02%	0.003%
100	15.043	4350	4355	4360	rBV5	778	879	0.05%	0.007%




Sum of corrected areas: 12217183

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035449.D
Acq On : 27 Apr 2024 00:48
Operator : SY/MD
Sample : P2279-09 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CORR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

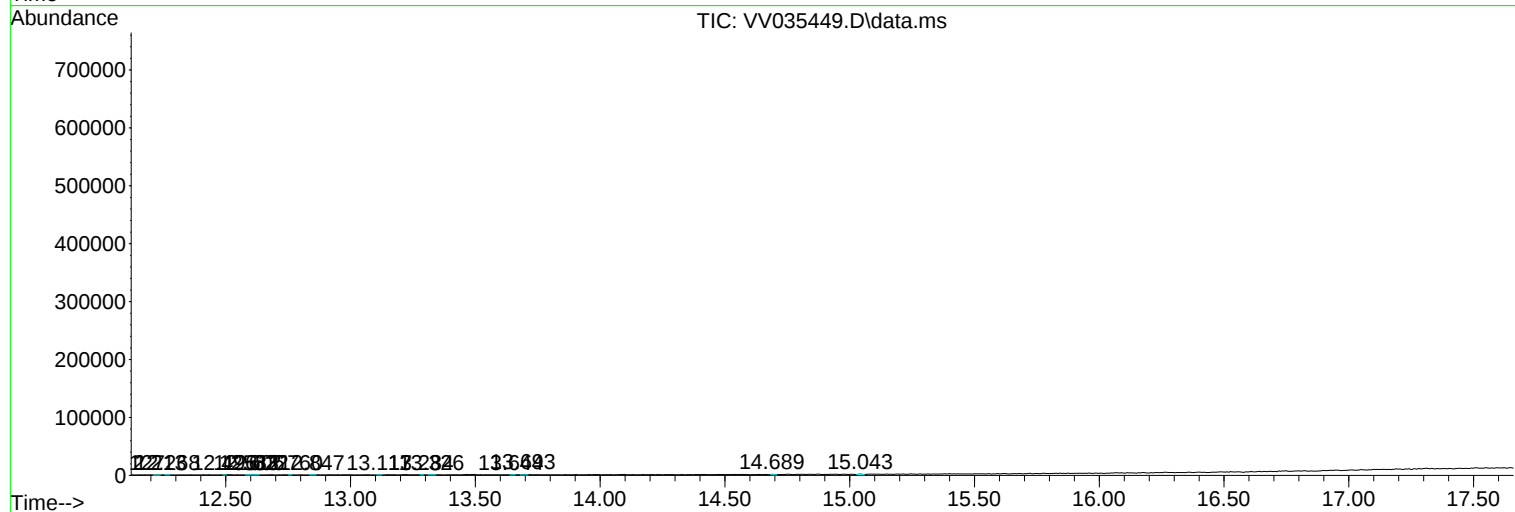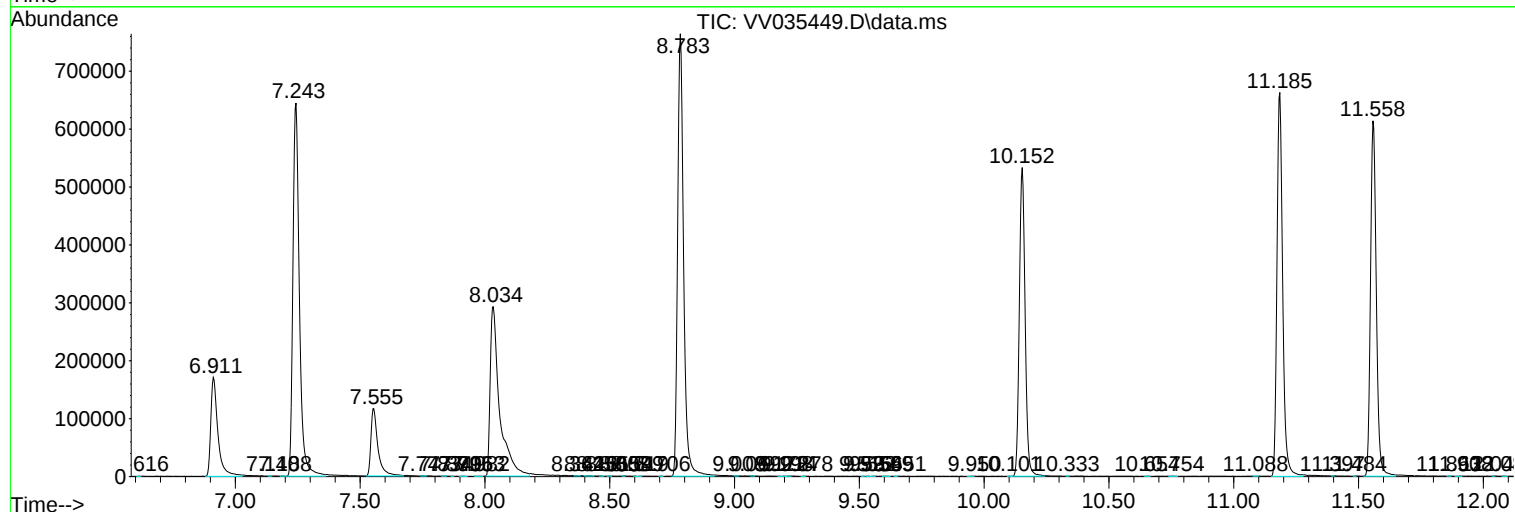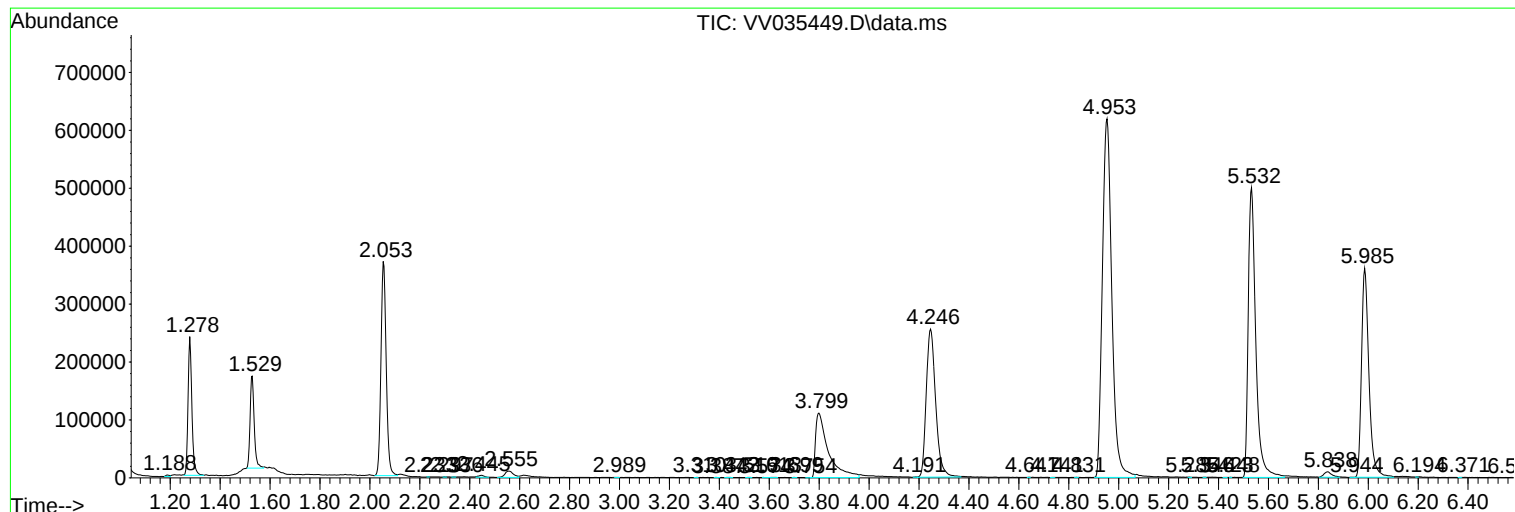

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035449.D
Acq On : 27 Apr 2024 00:48
Operator : SY/MD
Sample : P2279-09 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035449.D
Acq On : 27 Apr 2024 00:48
Operator : SY/MD
Sample : P2279-09 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc