

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035450.D
 Acq On : 27 Apr 2024 01:12
 Operator : SY/MD
 Sample : P2279-10 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035450.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	40	46	50	rBV	4204	4095	0.24%	0.033%
2	1.211	50	53	59	rVV	3249	3477	0.21%	0.028%
3	1.278	67	74	90	rVB	236563	258903	15.35%	2.072%
4	1.529	145	152	168	rBV	172902	195636	11.60%	1.566%
5	2.053	305	315	333	rBV	379411	546441	32.39%	4.374%
6	2.237	368	372	375	rBV4	770	525	0.03%	0.004%
7	2.343	403	405	410	rBV5	428	361	0.02%	0.003%
8	2.446	429	437	449	rVB4	3994	6923	0.41%	0.055%
9	2.558	461	472	483	rVV2	5940	12618	0.75%	0.101%
10	2.809	547	550	556	rBV3	229	244	0.01%	0.002%
11	3.137	648	652	658	rVB3	298	290	0.02%	0.002%
12	3.343	709	716	720	rBV3	224	249	0.01%	0.002%
13	3.401	732	734	741	rVB3	216	229	0.01%	0.002%
14	3.497	758	764	768	rBV2	311	363	0.02%	0.003%
15	3.799	849	858	909	rBV	110765	394018	23.36%	3.154%
16	4.246	981	997	1026	rBV	262640	683103	40.50%	5.468%
17	4.529	1082	1085	1092	rVB4	426	482	0.03%	0.004%
18	4.725	1139	1146	1148	rBV2	202	268	0.02%	0.002%
19	4.783	1158	1164	1168	rBV2	294	386	0.02%	0.003%
20	4.954	1201	1217	1261	rBV2	634929	1686876	100.00%	13.503%
21	5.243	1306	1307	1310	rVB2	389	192	0.01%	0.002%
22	5.304	1324	1326	1331	rVB4	442	282	0.02%	0.002%
23	5.532	1384	1397	1440	rBV	510554	1079214	63.98%	8.639%
24	5.831	1479	1490	1508	rBV2	9820	23893	1.42%	0.191%
25	5.986	1525	1538	1570	rBV	364993	766392	45.43%	6.135%
26	6.288	1630	1632	1636	rVB3	259	192	0.01%	0.002%
27	6.420	1670	1673	1676	rBV3	330	213	0.01%	0.002%
28	6.436	1676	1678	1684	rVB2	476	390	0.02%	0.003%
29	6.468	1684	1688	1692	rBV2	492	399	0.02%	0.003%
30	6.497	1693	1697	1703	rVB2	350	418	0.02%	0.003%
31	6.545	1706	1712	1716	rBV2	228	306	0.02%	0.002%
32	6.719	1764	1766	1771	rVB2	297	205	0.01%	0.002%
33	6.744	1771	1774	1777	rBV2	304	212	0.01%	0.002%
34	6.806	1790	1793	1798	rBV2	241	231	0.01%	0.002%
35	6.854	1802	1808	1813	rVB2	256	225	0.01%	0.002%
36	6.912	1815	1826	1863	rBV	176769	347479	20.60%	2.781%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035450.D
 Acq On : 27 Apr 2024 01:12
 Operator : SY/MD
 Sample : P2279-10 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	7.108	1885	1887	1891	rVB4	620	300	0.02%	0.002%
38	7.240	1917	1928	1960	rBV	658540	1192763	70.71%	9.547%
39	7.551	2016	2025	2047	rBV	121772	231569	13.73%	1.854%
40	7.783	2095	2097	2100	rVB2	387	190	0.01%	0.002%
41	7.812	2103	2106	2113	rBV4	490	636	0.04%	0.005%
42	7.863	2120	2122	2126	rVB3	547	322	0.02%	0.003%
43	7.896	2126	2132	2135	rBV2	661	543	0.03%	0.004%
44	8.034	2164	2175	2225	rBV4	293902	786873	46.65%	6.298%
45	8.400	2287	2289	2292	rVB2	485	216	0.01%	0.002%
46	8.523	2324	2327	2329	rBV2	345	231	0.01%	0.002%
47	8.555	2335	2337	2340	rBV2	462	374	0.02%	0.003%
48	8.609	2350	2354	2355	rBV2	513	311	0.02%	0.002%
49	8.677	2366	2375	2377	rBV4	395	461	0.03%	0.004%
50	8.712	2383	2386	2388	rVV3	383	247	0.01%	0.002%
51	8.783	2397	2408	2440	rBV	775606	1295650	76.81%	10.371%
52	9.059	2492	2494	2498	rVV2	362	230	0.01%	0.002%
53	9.082	2498	2501	2504	rVB3	545	298	0.02%	0.002%
54	9.098	2504	2506	2509	rBV3	377	216	0.01%	0.002%
55	9.114	2509	2511	2517	rVB	429	337	0.02%	0.003%
56	9.214	2540	2542	2546	rVB3	429	280	0.02%	0.002%
57	9.246	2549	2552	2557	rVB	333	235	0.01%	0.002%
58	9.278	2557	2562	2565	rBV2	393	273	0.02%	0.002%
59	9.297	2565	2568	2569	rBV2	279	193	0.01%	0.002%
60	9.519	2633	2637	2643	rBV	214	220	0.01%	0.002%
61	9.715	2695	2698	2703	rVB2	195	191	0.01%	0.002%
62	9.744	2703	2707	2710	rBV2	291	201	0.01%	0.002%
63	9.776	2714	2717	2719	rBV2	309	207	0.01%	0.002%
64	10.153	2821	2834	2859	rBV	552676	890910	52.81%	7.131%
65	10.310	2881	2883	2888	rBV3	235	207	0.01%	0.002%
66	10.532	2945	2952	2956	rVB2	202	279	0.02%	0.002%
67	10.918	3066	3072	3075	rVB2	265	214	0.01%	0.002%
68	10.953	3078	3083	3086	rBV	246	217	0.01%	0.002%
69	11.120	3131	3135	3137	rBV3	332	233	0.01%	0.002%
70	11.185	3144	3155	3188	rBV	674773	1059998	62.84%	8.485%
71	11.432	3228	3232	3234	rBV3	283	206	0.01%	0.002%
72	11.468	3239	3243	3245	rBV2	304	203	0.01%	0.002%
73	11.558	3256	3271	3295	rBV	625023	1002681	59.44%	8.026%
74	11.783	3338	3341	3346	rVB4	432	303	0.02%	0.002%
75	11.812	3346	3350	3355	rVB4	414	395	0.02%	0.003%
76	11.841	3355	3359	3360	rBV2	415	266	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035450.D
 Acq On : 27 Apr 2024 01:12
 Operator : SY/MD
 Sample : P2279-10 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	11.870	3364	3368	3371	rBV2	350	259	0.02%	0.002%
78	12.001	3405	3409	3411	rBV3	316	251	0.01%	0.002%
79	12.169	3458	3461	3464	rBV2	241	240	0.01%	0.002%
80	12.220	3474	3477	3480	rVB2	412	289	0.02%	0.002%
81	12.246	3480	3485	3486	rBV2	351	227	0.01%	0.002%
82	12.641	3605	3608	3612	rVB2	512	334	0.02%	0.003%
83	12.747	3639	3641	3646	rVB	308	270	0.02%	0.002%
84	12.841	3666	3670	3672	rBV2	329	304	0.02%	0.002%
85	13.075	3738	3743	3744	rBV3	397	322	0.02%	0.003%
86	13.111	3750	3754	3758	rBV2	210	203	0.01%	0.002%
87	13.220	3784	3788	3792	rBV2	512	363	0.02%	0.003%
88	13.259	3798	3800	3804	rVB2	401	225	0.01%	0.002%
89	13.378	3834	3837	3840	rBV	289	238	0.01%	0.002%
90	13.461	3861	3863	3866	rBV3	338	218	0.01%	0.002%
91	13.548	3888	3890	3895	rVB3	388	236	0.01%	0.002%
92	13.596	3902	3905	3909	rBV3	360	321	0.02%	0.003%
93	13.699	3934	3937	3940	rVB3	486	299	0.02%	0.002%
94	14.156	4074	4079	4081	rBV3	393	429	0.03%	0.003%
95	14.246	4104	4107	4110	rBV3	396	344	0.02%	0.003%
96	14.423	4160	4162	4164	rBV2	407	224	0.01%	0.002%
97	14.712	4250	4252	4254	rBV3	408	228	0.01%	0.002%
98	14.857	4292	4297	4301	rVB4	816	762	0.05%	0.006%
99	15.542	4508	4510	4513	rBV2	727	550	0.03%	0.004%
100	15.821	4595	4597	4598	rBV2	1013	495	0.03%	0.004%




Sum of corrected areas: 12493040

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035450.D
Acq On : 27 Apr 2024 01:12
Operator : SY/MD
Sample : P2279-10 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CORR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

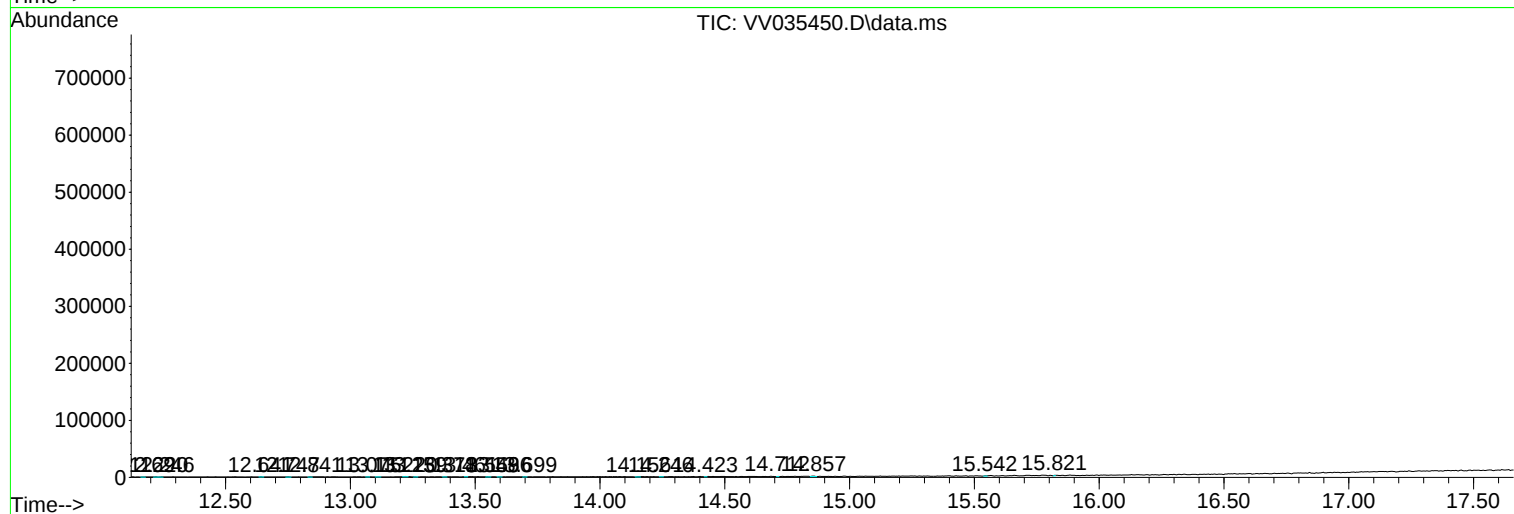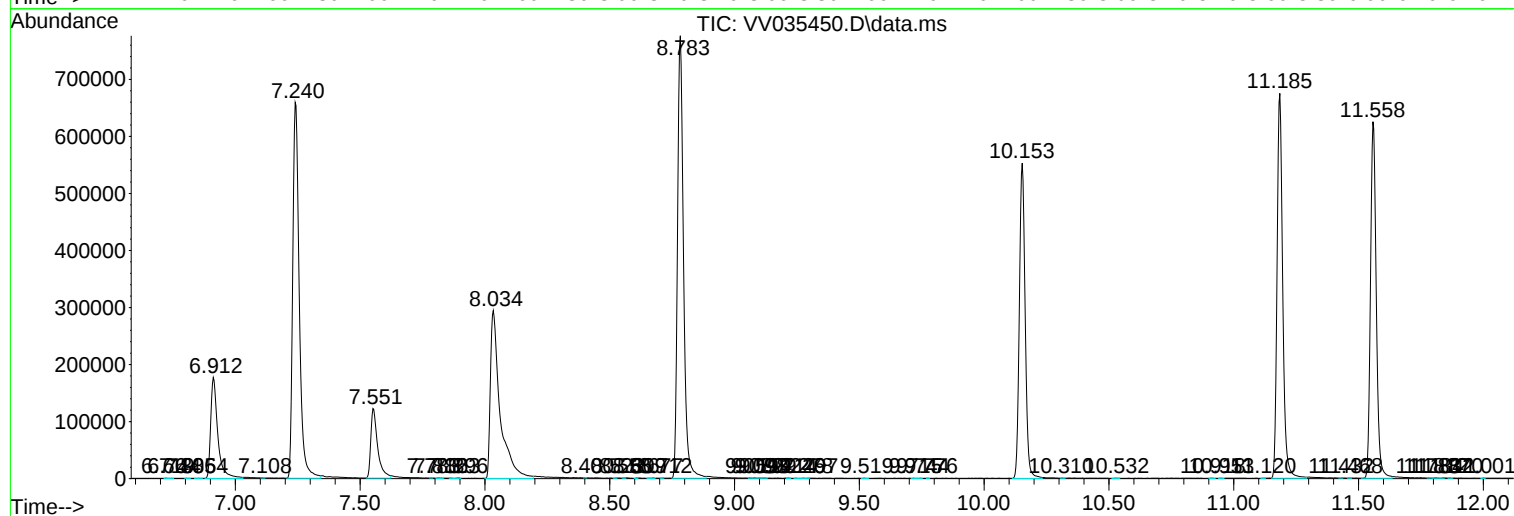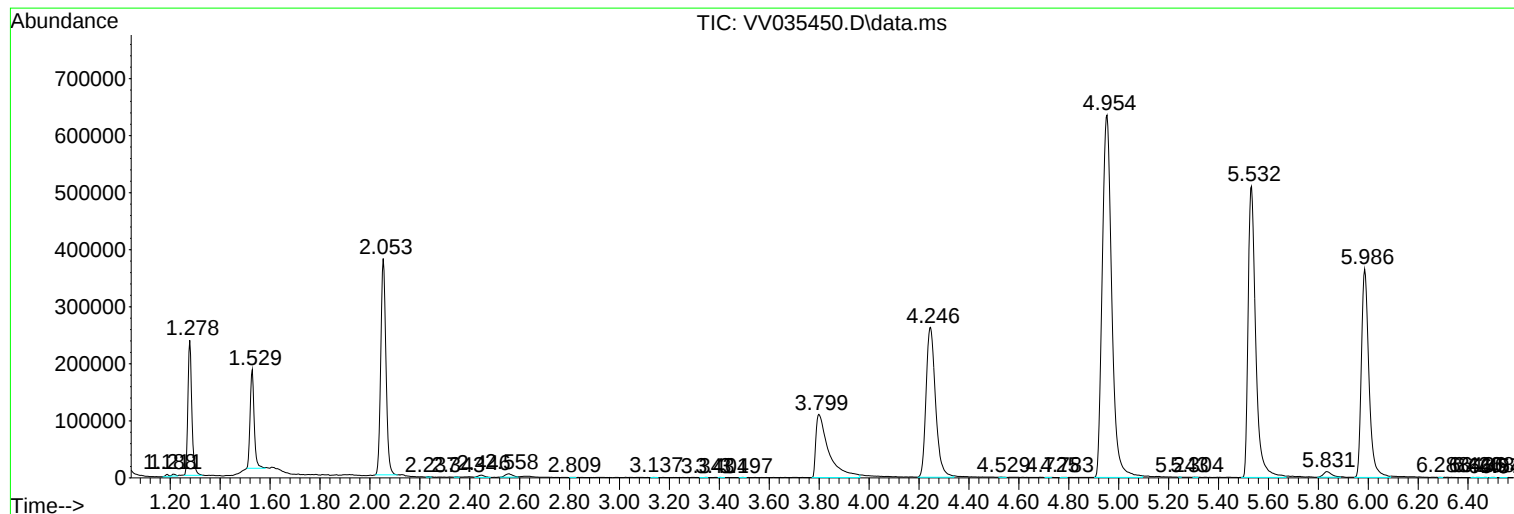

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035450.D
Acq On : 27 Apr 2024 01:12
Operator : SY/MD
Sample : P2279-10 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035450.D
Acq On : 27 Apr 2024 01:12
Operator : SY/MD
Sample : P2279-10 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------