

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035451.D
 Acq On : 27 Apr 2024 01:36
 Operator : SY/MD
 Sample : P2279-11 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035451.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	232542	255587	15.28%	1.992%
2	1.529	146	152	163	rBV	185258	201839	12.07%	1.573%
3	2.053	306	315	334	rVB	377188	544302	32.54%	4.242%
4	2.558	462	472	482	rBV2	8962	18879	1.13%	0.147%
5	2.780	538	541	544	rBV2	439	308	0.02%	0.002%
6	2.886	570	574	576	rBV2	231	168	0.01%	0.001%
7	3.159	657	659	660	rBV	151	45	0.00%	0.000%
8	3.175	660	664	667	rVV2	213	156	0.01%	0.001%
9	3.336	712	714	717	rBV	146	79	0.00%	0.001%
10	3.388	727	730	733	rBV2	269	202	0.01%	0.002%
11	3.503	764	766	767	rBV2	181	84	0.01%	0.001%
12	3.542	776	778	783	rVB2	258	120	0.01%	0.001%
13	3.581	788	790	795	rBV3	160	123	0.01%	0.001%
14	3.606	795	798	799	rBV	149	82	0.00%	0.001%
15	3.654	810	813	816	rVB	183	94	0.01%	0.001%
16	3.709	826	830	832	rBV2	178	131	0.01%	0.001%
17	3.799	849	858	912	rBV	110800	397563	23.77%	3.098%
18	4.246	982	997	1040	rVB2	259426	675693	40.40%	5.266%
19	4.667	1125	1128	1131	rBV3	314	235	0.01%	0.002%
20	4.854	1183	1186	1187	rBV	221	138	0.01%	0.001%
21	4.953	1201	1217	1231	rBV2	632656	1672520	100.00%	13.034%
22	5.368	1344	1346	1348	rBV	255	87	0.01%	0.001%
23	5.436	1365	1367	1368	rBV	253	80	0.00%	0.001%
24	5.532	1386	1397	1428	rBV	506923	1063375	63.58%	8.287%
25	5.986	1525	1538	1576	rBV	360991	763907	45.67%	5.953%
26	6.243	1614	1618	1622	rBV4	488	452	0.03%	0.004%
27	6.349	1648	1651	1654	rVB2	495	348	0.02%	0.003%
28	6.371	1655	1658	1659	rBV	171	93	0.01%	0.001%
29	6.400	1665	1667	1670	rBV2	193	91	0.01%	0.001%
30	6.420	1671	1673	1675	rVB2	178	56	0.00%	0.000%
31	6.452	1681	1683	1684	rBV2	353	113	0.01%	0.001%
32	6.471	1687	1689	1694	rVV2	387	335	0.02%	0.003%
33	6.506	1698	1700	1703	rVV	266	156	0.01%	0.001%
34	6.526	1704	1706	1708	rVB	265	95	0.01%	0.001%
35	6.577	1717	1722	1724	rBV3	458	359	0.02%	0.003%
36	6.590	1724	1726	1728	rBV2	199	100	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042624\
 Data File : VW035451.D
 Acq On : 27 Apr 2024 01:36
 Operator : SY/MD
 Sample : P2279-11 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.645	1740	1743	1745	rBV	194	97	0.01%	0.001%
38	6.825	1796	1799	1802	rVB	327	207	0.01%	0.002%
39	6.850	1803	1807	1808	rBV2	165	122	0.01%	0.001%
40	6.912	1815	1826	1861	rBV	171770	339864	20.32%	2.649%
41	7.243	1918	1929	1958	rBV	648166	1165831	69.71%	9.086%
42	7.555	2016	2026	2057	rBV	117855	230551	13.78%	1.797%
43	7.841	2113	2115	2118	rBV3	438	300	0.02%	0.002%
44	7.944	2144	2147	2149	rVB2	371	167	0.01%	0.001%
45	8.034	2165	2175	2231	rBV2	296135	784666	46.92%	6.115%
46	8.551	2334	2336	2338	rBV2	387	212	0.01%	0.002%
47	8.564	2338	2340	2342	rVB2	533	200	0.01%	0.002%
48	8.738	2390	2394	2397	rBV	386	365	0.02%	0.003%
49	8.783	2397	2408	2440	rBV2	785875	1513487	90.49%	11.795%
50	9.220	2542	2544	2547	rBV	304	183	0.01%	0.001%
51	9.256	2552	2555	2556	rBV2	208	106	0.01%	0.001%
52	9.307	2569	2571	2572	rBV2	246	90	0.01%	0.001%
53	9.416	2601	2605	2607	rBV2	236	190	0.01%	0.001%
54	9.429	2607	2609	2612	rVB2	235	89	0.01%	0.001%
55	9.481	2622	2625	2627	rBV2	201	142	0.01%	0.001%
56	9.522	2635	2638	2640	rBV	196	117	0.01%	0.001%
57	9.532	2640	2641	2644	rVV	193	74	0.00%	0.001%
58	9.622	2667	2669	2671	rVB2	199	63	0.00%	0.000%
59	9.767	2711	2714	2716	rBV2	329	207	0.01%	0.002%
60	9.992	2780	2784	2786	rBV	224	166	0.01%	0.001%
61	10.153	2822	2834	2862	rBV	545021	880737	52.66%	6.864%
62	10.538	2952	2954	2957	rBV	346	174	0.01%	0.001%
63	10.719	3007	3010	3012	rBV	233	140	0.01%	0.001%
64	10.747	3017	3019	3023	rVB2	232	142	0.01%	0.001%
65	10.828	3042	3044	3047	rBV2	221	110	0.01%	0.001%
66	10.927	3072	3075	3077	rBV2	203	151	0.01%	0.001%
67	10.940	3077	3079	3083	rVB2	268	128	0.01%	0.001%
68	11.127	3128	3137	3144	rBV5	10571	17476	1.04%	0.136%
69	11.185	3145	3155	3191	rVB	669675	1140973	68.22%	8.892%
70	11.503	3252	3254	3257	rBV2	413	268	0.02%	0.002%
71	11.561	3260	3272	3300	rBV2	638037	1148300	68.66%	8.949%
72	11.937	3386	3389	3390	rBV	348	198	0.01%	0.002%
73	12.040	3419	3421	3424	rBV2	409	154	0.01%	0.001%
74	12.104	3439	3441	3443	rBV	363	235	0.01%	0.002%
75	12.596	3592	3594	3596	rBV2	391	176	0.01%	0.001%
76	13.207	3778	3784	3798	rVB6	3921	6480	0.39%	0.050%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035451.D
Acq On : 27 Apr 2024 01:36
Operator : SY/MD
Sample : P2279-11 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Title : VOC Analysis

77	13.651	3919	3922	3925	rBV	369	372	0.02%	0.003%
----	--------	------	------	------	-----	-----	-----	-------	--------




Sum of corrected areas: 12831705

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035451.D
Acq On : 27 Apr 2024 01:36
Operator : SY/MD
Sample : P2279-11 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

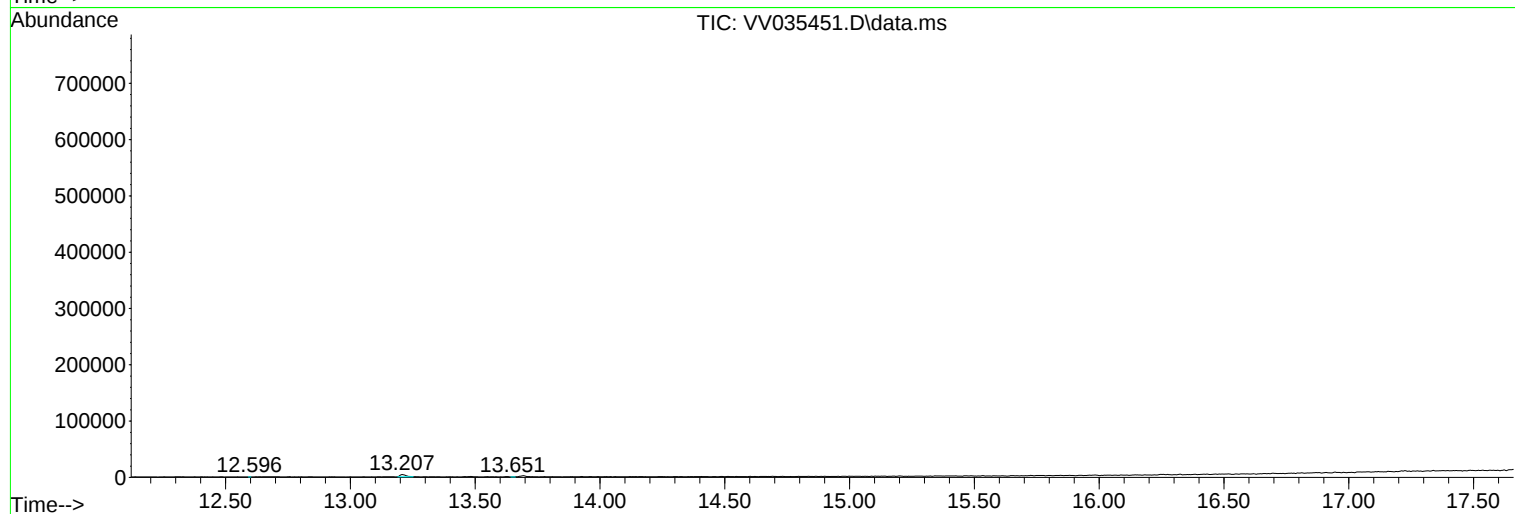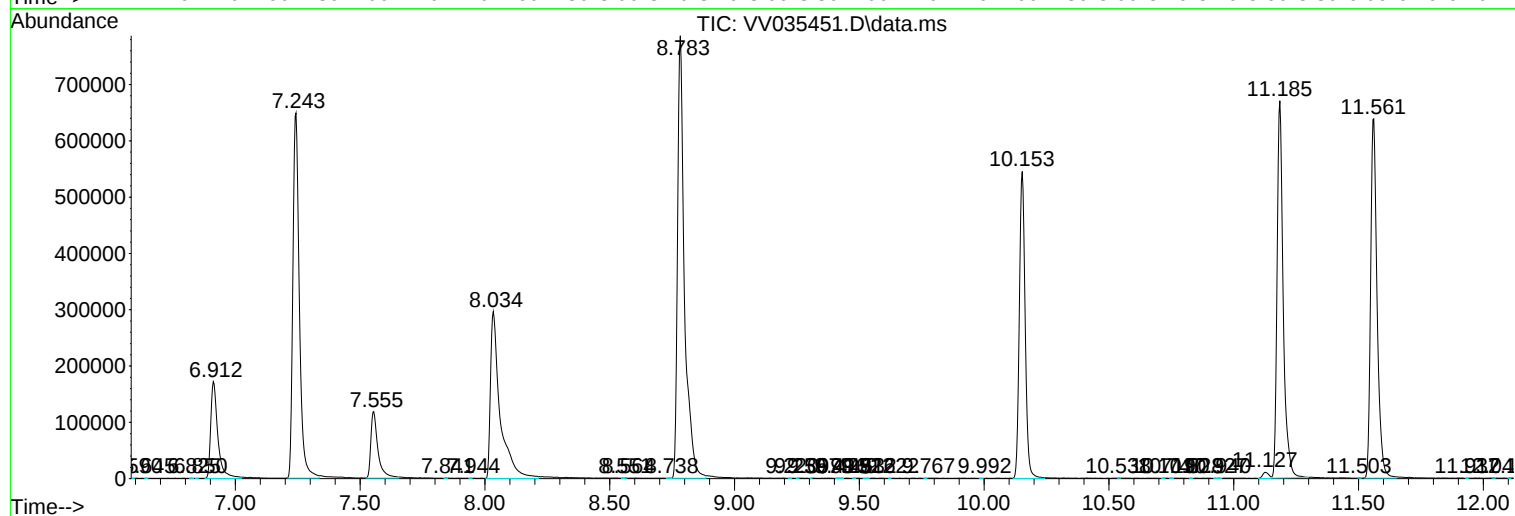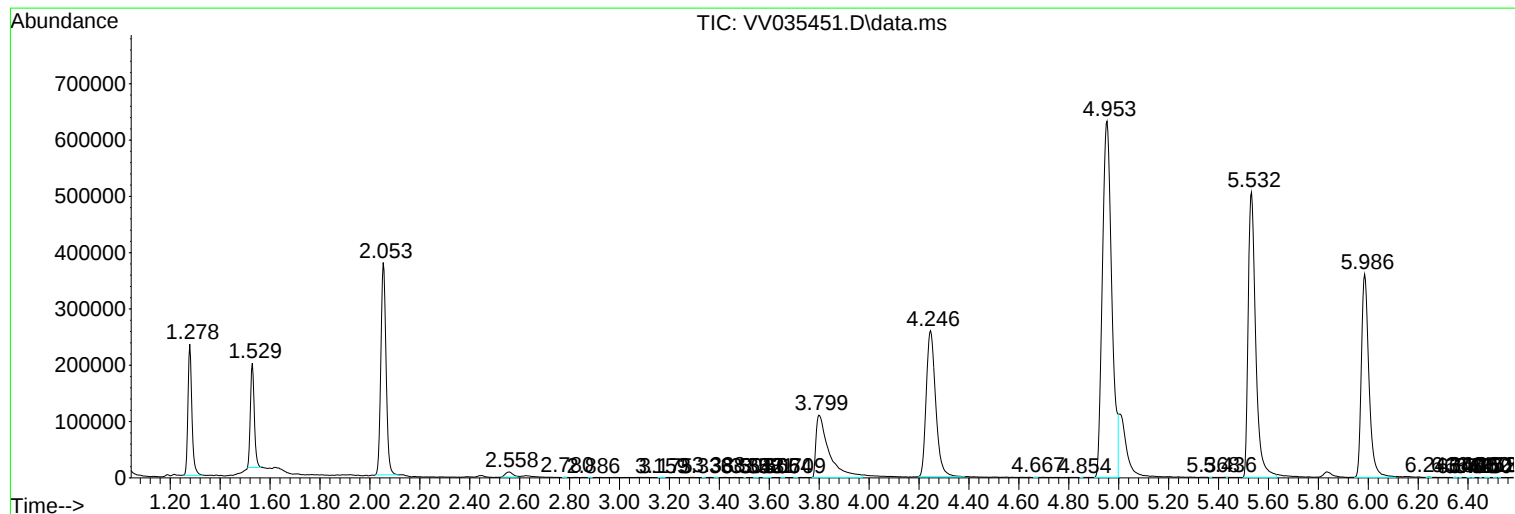

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035451.D
Acq On : 27 Apr 2024 01:36
Operator : SY/MD
Sample : P2279-11 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035451.D
Acq On : 27 Apr 2024 01:36
Operator : SY/MD
Sample : P2279-11 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------