

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035452.D
 Acq On : 27 Apr 2024 02:00
 Operator : SY/MD
 Sample : P2279-12 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M

Title : VOC Analysis

Signal : TIC: VV035452.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	226691	246893	13.02%	1.794%
2	1.529	146	152	164	rVB	171056	191155	10.08%	1.389%
3	2.053	306	315	332	rVB	362228	523535	27.61%	3.804%
4	2.555	462	471	485	rBV	10550	21804	1.15%	0.158%
5	2.741	526	529	531	rBV2	338	217	0.01%	0.002%
6	2.786	541	543	545	rVB	274	88	0.00%	0.001%
7	2.812	548	551	556	rBV2	334	290	0.02%	0.002%
8	2.841	556	560	566	rVB2	490	584	0.03%	0.004%
9	2.864	566	567	572	rBV	219	137	0.01%	0.001%
10	2.966	594	599	602	rBV3	274	318	0.02%	0.002%
11	3.024	614	617	622	rBV2	211	206	0.01%	0.001%
12	3.050	622	625	629	rVV3	229	184	0.01%	0.001%
13	3.127	646	649	652	rVB2	430	274	0.01%	0.002%
14	3.150	653	656	663	rVB3	284	267	0.01%	0.002%
15	3.208	671	674	678	rVB2	152	104	0.01%	0.001%
16	3.237	678	683	685	rBV2	180	147	0.01%	0.001%
17	3.285	694	698	702	rVV2	330	268	0.01%	0.002%
18	3.355	717	720	724	rBV	299	253	0.01%	0.002%
19	3.426	738	742	747	rVB2	311	311	0.02%	0.002%
20	3.465	751	754	756	rBV	264	141	0.01%	0.001%
21	3.584	789	791	793	rBV	273	146	0.01%	0.001%
22	3.629	801	805	812	rVB2	294	310	0.02%	0.002%
23	3.658	812	814	821	rBV2	204	203	0.01%	0.001%
24	3.719	830	833	834	rBV	224	98	0.01%	0.001%
25	3.799	849	858	920	rBV	109857	399555	21.08%	2.903%
26	4.246	982	997	1032	rBV	255873	672155	35.45%	4.884%
27	4.584	1100	1102	1105	rBV3	563	215	0.01%	0.002%
28	4.690	1131	1135	1138	rBV	372	332	0.02%	0.002%
29	4.870	1185	1191	1194	rVB3	343	294	0.02%	0.002%
30	4.892	1194	1198	1200	rBV	252	197	0.01%	0.001%
31	4.953	1201	1217	1228	rBV2	624672	1598135	84.30%	11.613%
32	5.445	1367	1370	1375	rBV3	354	367	0.02%	0.003%
33	5.532	1386	1397	1430	rBV	491997	1036329	54.66%	7.530%
34	5.838	1482	1492	1510	rVB4	8581	19916	1.05%	0.145%
35	5.986	1525	1538	1576	rBV	355657	748101	39.46%	5.436%
36	6.288	1630	1632	1636	rBV2	624	379	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035452.D
 Acq On : 27 Apr 2024 02:00
 Operator : SY/MD
 Sample : P2279-12 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.310	1636	1639	1641	rVB2	329	152	0.01%	0.001%
38	6.346	1648	1650	1652	rVB3	466	140	0.01%	0.001%
39	6.420	1671	1673	1676	rVB	259	123	0.01%	0.001%
40	6.468	1685	1688	1691	rVB	180	106	0.01%	0.001%
41	6.490	1691	1695	1697	rBV2	364	211	0.01%	0.002%
42	6.510	1697	1701	1704	rVV	239	163	0.01%	0.001%
43	6.548	1710	1713	1718	rBV	223	147	0.01%	0.001%
44	6.648	1741	1744	1748	rVV2	153	107	0.01%	0.001%
45	6.680	1748	1754	1757	rVV2	393	302	0.02%	0.002%
46	6.699	1758	1760	1765	rVB	217	128	0.01%	0.001%
47	6.751	1773	1776	1777	rBV	238	113	0.01%	0.001%
48	6.828	1797	1800	1802	rBV2	132	89	0.00%	0.001%
49	6.912	1815	1826	1859	rBV	164874	329395	17.37%	2.393%
50	7.162	1900	1904	1906	rBV2	374	267	0.01%	0.002%
51	7.243	1917	1929	1970	rBV	631535	1147351	60.52%	8.337%
52	7.551	2016	2025	2062	rBV	115958	223470	11.79%	1.624%
53	7.789	2097	2099	2101	rBV	386	179	0.01%	0.001%
54	7.905	2131	2135	2136	rBV2	308	179	0.01%	0.001%
55	7.934	2142	2144	2147	rVB	252	115	0.01%	0.001%
56	8.034	2165	2175	2226	rBV3	286565	761094	40.15%	5.530%
57	8.558	2335	2338	2341	rBV3	534	398	0.02%	0.003%
58	8.654	2366	2368	2370	rBV2	260	152	0.01%	0.001%
59	8.783	2397	2408	2415	rBV	794284	1376434	72.60%	10.002%
60	9.175	2527	2530	2532	rBV2	428	255	0.01%	0.002%
61	9.230	2545	2547	2549	rVB	252	101	0.01%	0.001%
62	9.304	2568	2570	2571	rBV	301	137	0.01%	0.001%
63	9.368	2587	2590	2591	rBV	239	94	0.00%	0.001%
64	9.407	2598	2602	2609	rBV2	397	386	0.02%	0.003%
65	9.468	2619	2621	2624	rVV	201	103	0.01%	0.001%
66	9.539	2641	2643	2646	rVB	335	142	0.01%	0.001%
67	9.564	2649	2651	2654	rBV2	159	89	0.00%	0.001%
68	9.580	2654	2656	2657	rBV2	265	102	0.01%	0.001%
69	9.638	2670	2674	2676	rBV2	343	243	0.01%	0.002%
70	9.709	2693	2696	2703	rVB	255	259	0.01%	0.002%
71	9.860	2740	2743	2745	rVV	195	124	0.01%	0.001%
72	9.915	2757	2760	2763	rBV	300	232	0.01%	0.002%
73	10.014	2788	2791	2793	rBV	227	147	0.01%	0.001%
74	10.088	2810	2814	2820	rVB2	300	279	0.01%	0.002%
75	10.153	2821	2834	2865	rBV	533044	866191	45.69%	6.294%
76	10.400	2909	2911	2916	rVV2	471	300	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035452.D
 Acq On : 27 Apr 2024 02:00
 Operator : SY/MD
 Sample : P2279-12 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	10.423	2916	2918	2920	rVB3	344	130	0.01%	0.001%
78	10.461	2928	2930	2933	rBV2	273	170	0.01%	0.001%
79	10.535	2952	2953	2956	rBV	164	102	0.01%	0.001%
80	10.677	2994	2997	2999	rBV	153	95	0.01%	0.001%
81	10.773	3025	3027	3032	rBV2	146	126	0.01%	0.001%
82	10.995	3091	3096	3099	rBV	227	256	0.01%	0.002%
83	11.037	3106	3109	3112	rBV	285	160	0.01%	0.001%
84	11.072	3117	3120	3126	rVB3	164	172	0.01%	0.001%
85	11.120	3126	3135	3145	rBV	61795	99632	5.26%	0.724%
86	11.185	3145	3155	3190	rVB2	717422	1543188	81.40%	11.213%
87	11.564	3259	3273	3300	rBV2	800840	1895839	100.00%	13.776%
88	11.863	3364	3366	3368	rBV	359	152	0.01%	0.001%
89	11.905	3377	3379	3383	rBV3	321	182	0.01%	0.001%
90	11.953	3392	3394	3396	rVB	356	99	0.01%	0.001%
91	11.976	3399	3401	3402	rBV	300	152	0.01%	0.001%
92	12.056	3423	3426	3429	rBV2	324	270	0.01%	0.002%
93	12.095	3435	3438	3442	rBV	366	293	0.02%	0.002%
94	12.313	3502	3506	3509	rBV	377	374	0.02%	0.003%
95	12.349	3513	3517	3520	rBV	317	299	0.02%	0.002%
96	12.458	3548	3551	3553	rBV2	521	302	0.02%	0.002%
97	12.757	3642	3644	3649	rVB2	556	370	0.02%	0.003%
98	12.979	3709	3713	3720	rBV4	525	612	0.03%	0.004%
99	13.204	3774	3783	3801	rBV3	18715	31657	1.67%	0.230%
100	13.686	3925	3933	3949	rVB4	7909	13641	0.72%	0.099%




Sum of corrected areas: 13762180

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035452.D
Acq On : 27 Apr 2024 02:00
Operator : SY/MD
Sample : P2279-12 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CORR5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

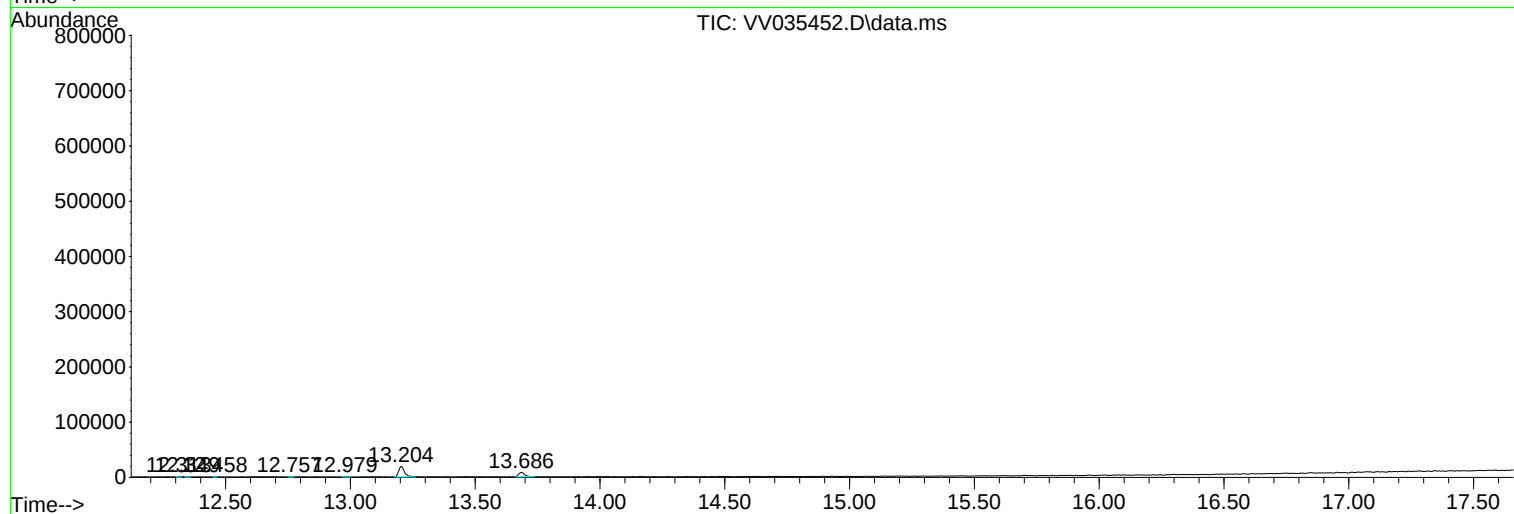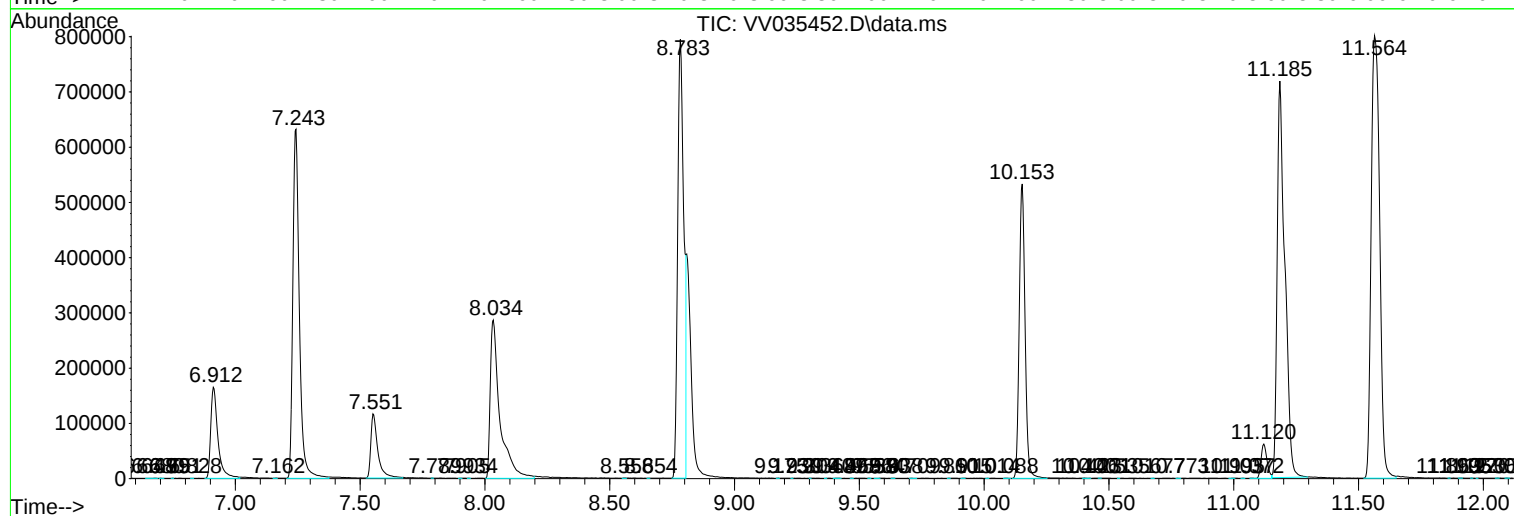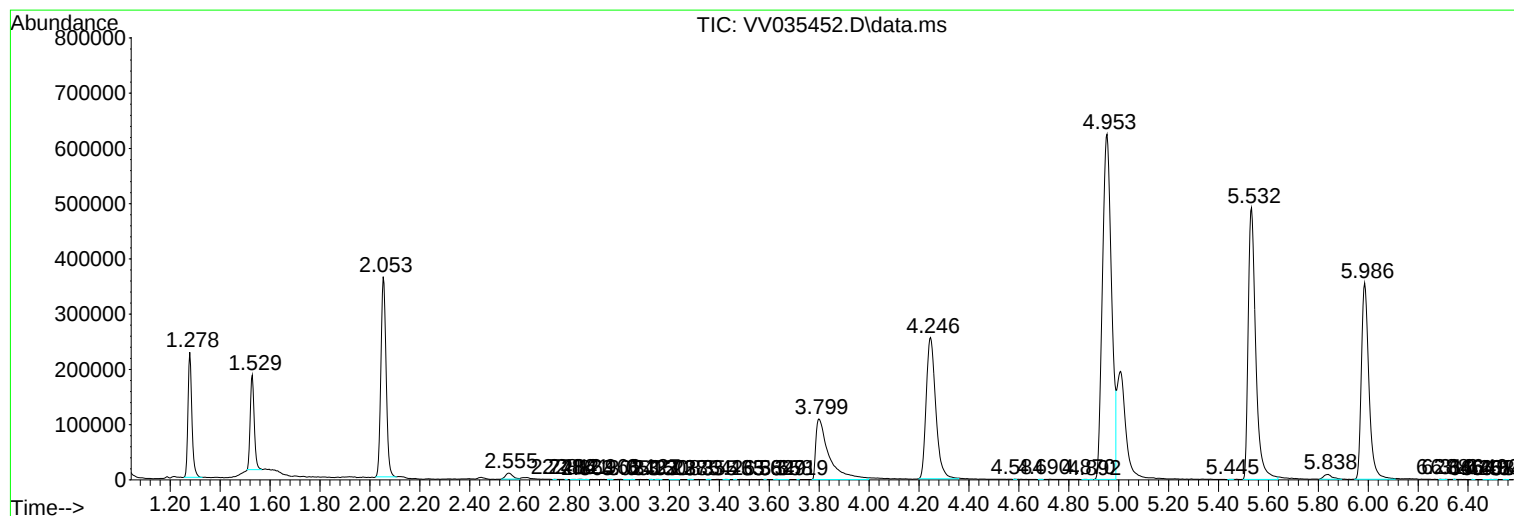

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035452.D
Acq On : 27 Apr 2024 02:00
Operator : SY/MD
Sample : P2279-12 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035452.D
Acq On : 27 Apr 2024 02:00
Operator : SY/MD
Sample : P2279-12 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
