

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035453.D
 Acq On : 27 Apr 2024 02:24
 Operator : SY/MD
 Sample : P2279-13 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M

Title : VOC Analysis

Signal : TIC: VV035453.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	41	46	50	rBV	3346	3303	0.19%	0.025%
2	1.278	67	74	87	rBV	244501	267746	15.22%	2.011%
3	1.529	145	152	164	rBV	195317	222498	12.64%	1.671%
4	2.053	305	315	332	rVB	395234	575535	32.71%	4.323%
5	2.281	383	386	387	rBV3	376	196	0.01%	0.001%
6	2.449	431	438	447	rVB5	3256	5077	0.29%	0.038%
7	2.558	459	472	484	rBV	11830	25796	1.47%	0.194%
8	2.892	573	576	583	rBV2	332	244	0.01%	0.002%
9	2.957	592	596	599	rBV2	274	211	0.01%	0.002%
10	3.050	618	625	629	rVV3	254	276	0.02%	0.002%
11	3.413	735	738	741	rBV2	418	269	0.02%	0.002%
12	3.526	771	773	778	rVV2	221	211	0.01%	0.002%
13	3.561	780	784	787	rVB2	308	260	0.01%	0.002%
14	3.674	815	819	823	rVB3	236	193	0.01%	0.001%
15	3.728	833	836	839	rBV	214	193	0.01%	0.001%
16	3.799	849	858	903	rBV2	116858	406511	23.10%	3.053%
17	4.246	980	997	1026	rBV	274974	712813	40.51%	5.354%
18	4.387	1039	1041	1048	rVB7	850	837	0.05%	0.006%
19	4.532	1084	1086	1089	rBV3	401	241	0.01%	0.002%
20	4.622	1111	1114	1117	rBV4	276	209	0.01%	0.002%
21	4.686	1132	1134	1137	rVB2	282	182	0.01%	0.001%
22	4.805	1164	1171	1173	rBV2	171	179	0.01%	0.001%
23	4.847	1182	1184	1189	rVB3	265	181	0.01%	0.001%
24	4.953	1201	1217	1256	rBV2	667226	1759717	100.00%	13.217%
25	5.246	1305	1308	1311	rVB3	447	230	0.01%	0.002%
26	5.346	1332	1339	1341	rBV3	520	482	0.03%	0.004%
27	5.358	1341	1343	1350	rVB3	299	323	0.02%	0.002%
28	5.532	1386	1397	1428	rBV	527726	1106640	62.89%	8.312%
29	5.834	1480	1491	1515	rVB2	10197	25778	1.46%	0.194%
30	5.985	1519	1538	1573	rBV	380405	800675	45.50%	6.014%
31	6.288	1628	1632	1634	rBV	537	364	0.02%	0.003%
32	6.317	1638	1641	1643	rVV2	356	283	0.02%	0.002%
33	6.342	1647	1649	1653	rVV2	412	309	0.02%	0.002%
34	6.390	1661	1664	1669	rVV3	456	292	0.02%	0.002%
35	6.426	1672	1675	1681	rBV3	359	379	0.02%	0.003%
36	6.683	1752	1755	1759	rVB	245	179	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035453.D
 Acq On : 27 Apr 2024 02:24
 Operator : SY/MD
 Sample : P2279-13 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.712	1759	1764	1767	rBV	203	217	0.01%	0.002%
38	6.911	1815	1826	1854	rBV	181241	354601	20.15%	2.663%
39	7.165	1902	1905	1907	rBV2	378	212	0.01%	0.002%
40	7.243	1917	1929	1960	rBV	708181	1271065	72.23%	9.547%
41	7.551	2016	2025	2058	rBV	127041	243242	13.82%	1.827%
42	7.886	2126	2129	2133	rBV3	225	230	0.01%	0.002%
43	7.937	2142	2145	2148	rBV4	347	252	0.01%	0.002%
44	8.034	2165	2175	2219	rBV3	311984	811053	46.09%	6.092%
45	8.435	2298	2300	2302	rVB	535	200	0.01%	0.002%
46	8.474	2308	2312	2315	rVB3	453	338	0.02%	0.003%
47	8.522	2323	2327	2333	rBV4	437	505	0.03%	0.004%
48	8.638	2359	2363	2365	rBV2	445	330	0.02%	0.002%
49	8.783	2397	2408	2440	rBV	814899	1362045	77.40%	10.230%
50	9.143	2515	2520	2523	rVV4	429	332	0.02%	0.002%
51	9.217	2541	2543	2547	rVB2	620	352	0.02%	0.003%
52	9.239	2547	2550	2553	rBV	473	268	0.02%	0.002%
53	9.265	2553	2558	2559	rBV3	277	231	0.01%	0.002%
54	9.342	2580	2582	2585	rVV2	294	193	0.01%	0.001%
55	9.358	2585	2587	2592	rVV2	351	259	0.01%	0.002%
56	9.435	2603	2611	2615	rBV3	299	353	0.02%	0.003%
57	9.574	2648	2654	2657	rBV2	354	277	0.02%	0.002%
58	9.609	2662	2665	2668	rVB2	383	244	0.01%	0.002%
59	9.828	2730	2733	2736	rBV	364	236	0.01%	0.002%
60	9.850	2737	2740	2744	rVV3	244	216	0.01%	0.002%
61	9.966	2773	2776	2782	rVB3	325	249	0.01%	0.002%
62	10.152	2820	2834	2858	rBV	570725	917654	52.15%	6.892%
63	10.368	2898	2901	2905	rBV2	534	374	0.02%	0.003%
64	10.641	2978	2986	2988	rBV	300	378	0.02%	0.003%
65	10.767	3022	3025	3030	rVV2	233	192	0.01%	0.001%
66	11.024	3101	3105	3109	rBV	222	191	0.01%	0.001%
67	11.127	3129	3137	3145	rBV2	10363	15854	0.90%	0.119%
68	11.185	3145	3155	3184	rVB	703975	1156677	65.73%	8.687%
69	11.496	3249	3252	3253	rBV	374	192	0.01%	0.001%
70	11.561	3257	3272	3297	rBV	688932	1199738	68.18%	9.011%
71	11.840	3356	3359	3361	rBV	429	297	0.02%	0.002%
72	11.876	3368	3370	3372	rBV	283	185	0.01%	0.001%
73	11.898	3375	3377	3384	rBV2	344	339	0.02%	0.003%
74	11.959	3394	3396	3401	rBV2	383	332	0.02%	0.002%
75	12.168	3459	3461	3465	rVV3	335	230	0.01%	0.002%
76	12.191	3465	3468	3475	rVB3	455	450	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035453.D
 Acq On : 27 Apr 2024 02:24
 Operator : SY/MD
 Sample : P2279-13 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	12.249	3483	3486	3493	rVB4	388	309	0.02%	0.002%
78	12.287	3494	3498	3500	rBV2	337	233	0.01%	0.002%
79	12.448	3544	3548	3550	rVV3	391	262	0.01%	0.002%
80	12.477	3556	3557	3562	rVB	343	192	0.01%	0.001%
81	12.503	3562	3565	3570	rBV	228	188	0.01%	0.001%
82	12.541	3570	3577	3579	rBV3	469	439	0.02%	0.003%
83	12.873	3678	3680	3686	rVB3	330	263	0.01%	0.002%
84	12.914	3688	3693	3701	rVB3	396	400	0.02%	0.003%
85	12.956	3702	3706	3711	rVB2	425	392	0.02%	0.003%
86	13.046	3732	3734	3736	rBV2	431	254	0.01%	0.002%
87	13.117	3753	3756	3759	rVB2	290	211	0.01%	0.002%
88	13.204	3774	3783	3797	rBV3	18057	31146	1.77%	0.234%
89	13.638	3916	3918	3921	rVB2	534	286	0.02%	0.002%
90	13.683	3923	3932	3945	rVV4	10274	16567	0.94%	0.124%
91	13.766	3955	3958	3966	rVB3	511	414	0.02%	0.003%
92	13.837	3977	3980	3984	rBV3	492	322	0.02%	0.002%
93	13.918	4002	4005	4008	rBV	322	261	0.01%	0.002%
94	14.014	4033	4035	4037	rBV2	442	178	0.01%	0.001%
95	14.307	4124	4126	4130	rVB	654	375	0.02%	0.003%
96	14.371	4143	4146	4147	rBV	368	195	0.01%	0.001%
97	14.499	4181	4186	4188	rBV2	490	496	0.03%	0.004%
98	14.789	4274	4276	4279	rBV3	458	317	0.02%	0.002%
99	14.966	4328	4331	4332	rBV	528	298	0.02%	0.002%
100	15.143	4382	4386	4391	rBV5	780	1049	0.06%	0.008%




Sum of corrected areas: 13314442

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035453.D
Acq On : 27 Apr 2024 02:24
Operator : SY/MD
Sample : P2279-13 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CORR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

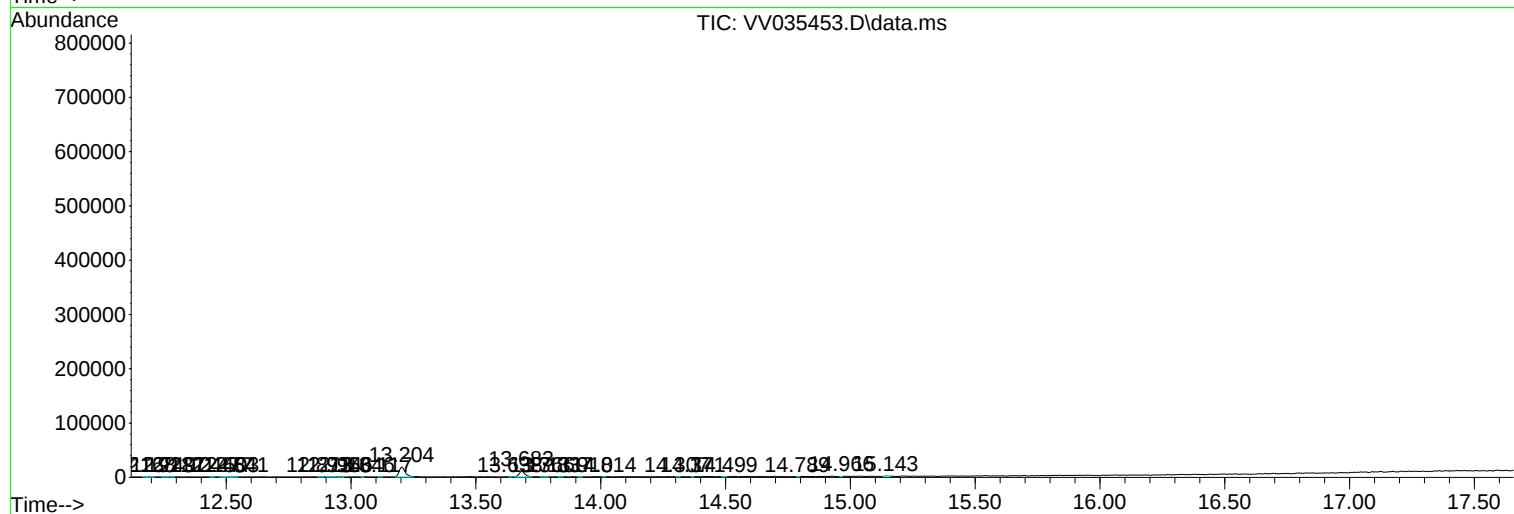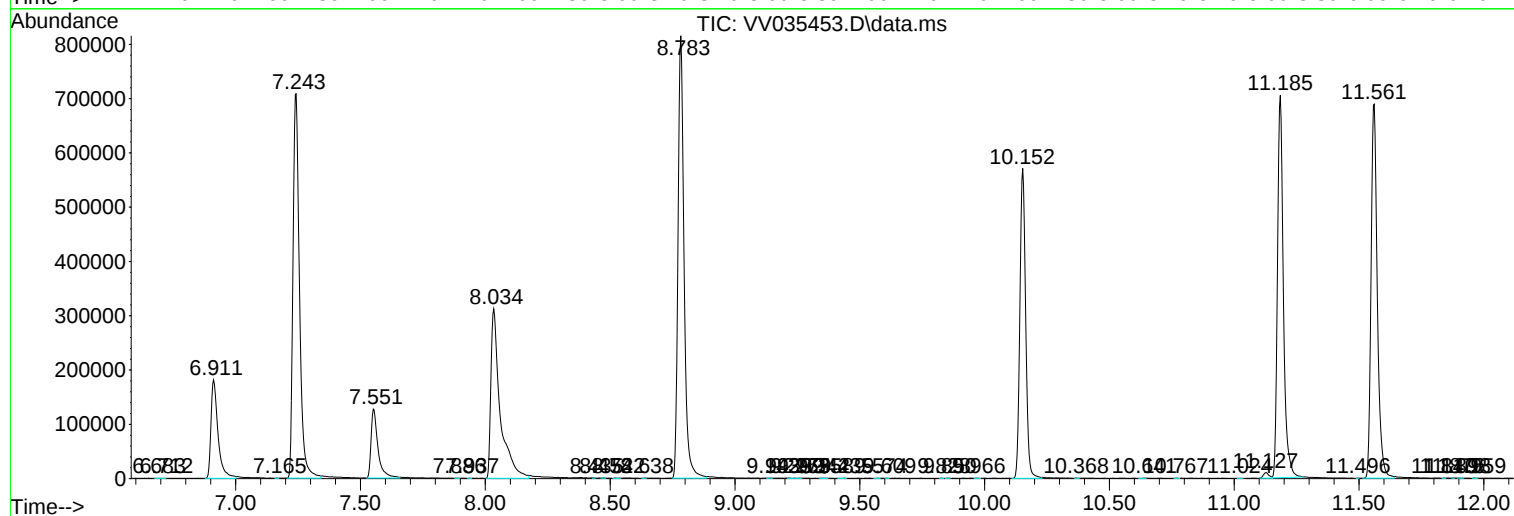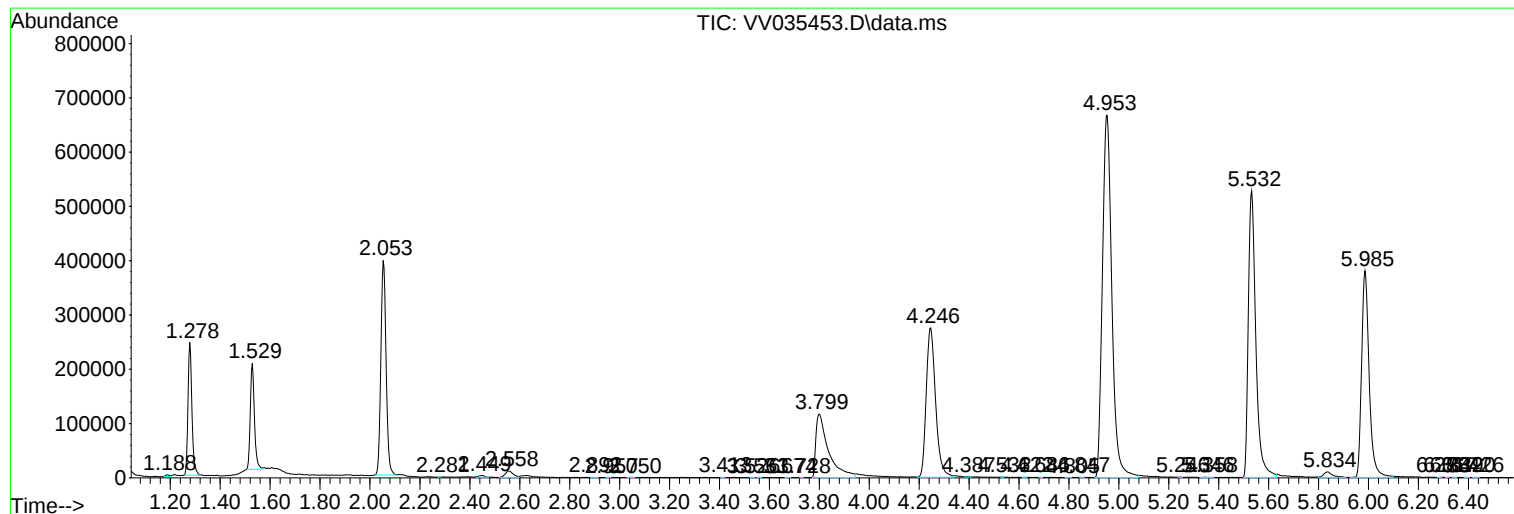

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035453.D
Acq On : 27 Apr 2024 02:24
Operator : SY/MD
Sample : P2279-13 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035453.D
Acq On : 27 Apr 2024 02:24
Operator : SY/MD
Sample : P2279-13 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------