

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035454.D
 Acq On : 27 Apr 2024 02:47
 Operator : SY/MD
 Sample : P2279-14 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035454.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	222309	242070	15.24%	2.065%
2	1.529	146	152	168	rVB	170271	189954	11.96%	1.620%
3	2.053	306	315	333	rVB	348469	506717	31.89%	4.323%
4	2.555	458	471	483	rBV2	15480	35220	2.22%	0.300%
5	2.780	538	541	544	rBV2	220	150	0.01%	0.001%
6	2.793	544	545	546	rBV2	151	47	0.00%	0.000%
7	2.944	588	592	594	rBV	198	162	0.01%	0.001%
8	2.963	596	598	601	rBV	160	117	0.01%	0.001%
9	3.034	619	620	622	rBV	232	56	0.00%	0.000%
10	3.050	622	625	627	rBV	158	90	0.01%	0.001%
11	3.063	627	629	630	rBV	216	73	0.00%	0.001%
12	3.108	640	643	647	rVB2	398	331	0.02%	0.003%
13	3.127	647	649	653	rBV2	226	181	0.01%	0.002%
14	3.178	661	665	668	rBV	361	285	0.02%	0.002%
15	3.220	677	678	679	rBV	140	36	0.00%	0.000%
16	3.285	695	698	705	rVB2	184	125	0.01%	0.001%
17	3.317	705	708	712	rBV2	190	161	0.01%	0.001%
18	3.371	721	725	729	rBV2	215	248	0.02%	0.002%
19	3.426	739	742	743	rBV2	166	84	0.01%	0.001%
20	3.522	768	772	776	rBV	226	153	0.01%	0.001%
21	3.542	776	778	779	rBV	79	39	0.00%	0.000%
22	3.616	799	801	804	rBV2	121	72	0.00%	0.001%
23	3.651	810	812	814	rBV	225	125	0.01%	0.001%
24	3.683	820	822	824	rBV2	245	140	0.01%	0.001%
25	3.722	831	834	835	rBV2	165	95	0.01%	0.001%
26	3.802	848	859	901	rBV2	110002	393486	24.76%	3.357%
27	4.246	982	997	1038	rBV	254258	651067	40.98%	5.554%
28	4.725	1142	1146	1151	rBV2	327	287	0.02%	0.002%
29	4.818	1171	1175	1178	rBV	288	287	0.02%	0.002%
30	4.953	1201	1217	1250	rBV2	600531	1588892	100.00%	13.555%
31	5.442	1365	1369	1370	rVB2	333	189	0.01%	0.002%
32	5.471	1375	1378	1380	rBV2	270	228	0.01%	0.002%
33	5.532	1386	1397	1435	rBV	475406	1008647	63.48%	8.605%
34	5.915	1514	1516	1517	rBV	282	110	0.01%	0.001%
35	5.985	1526	1538	1573	rBV	349665	727310	45.77%	6.205%
36	6.317	1639	1641	1644	rBV2	477	267	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042624\
 Data File : VW035454.D
 Acq On : 27 Apr 2024 02:47
 Operator : SY/MD
 Sample : P2279-14 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

37	6.339	1644	1648	1651	rBV2	378	309	0.02%	0.003%
38	6.365	1654	1656	1657	rBV	197	74	0.00%	0.001%
39	6.400	1665	1667	1670	rBV	301	179	0.01%	0.002%
40	6.423	1670	1674	1675	rVV2	324	216	0.01%	0.002%
41	6.439	1676	1679	1683	rVB2	411	240	0.02%	0.002%
42	6.455	1683	1684	1685	rBV2	73	26	0.00%	0.000%
43	6.532	1705	1708	1710	rBV2	210	95	0.01%	0.001%
44	6.545	1710	1712	1713	rBV	164	77	0.00%	0.001%
45	6.564	1715	1718	1721	rVB2	352	205	0.01%	0.002%
46	6.635	1735	1740	1742	rBV	292	192	0.01%	0.002%
47	6.683	1752	1755	1757	rBV2	187	107	0.01%	0.001%
48	6.728	1764	1769	1773	rBV	203	229	0.01%	0.002%
49	6.751	1773	1776	1777	rBV	142	74	0.00%	0.001%
50	6.799	1786	1791	1795	rBV	166	165	0.01%	0.001%
51	6.911	1816	1826	1858	rBV	162701	324904	20.45%	2.772%
52	7.243	1917	1929	1967	rBV	610318	1104568	69.52%	9.423%
53	7.554	2016	2026	2059	rBV	114761	220785	13.90%	1.883%
54	7.876	2122	2126	2128	rBV2	370	284	0.02%	0.002%
55	7.908	2133	2136	2138	rVB	226	118	0.01%	0.001%
56	7.921	2138	2140	2141	rBV	93	44	0.00%	0.000%
57	7.985	2155	2160	2163	rBV	209	187	0.01%	0.002%
58	8.034	2163	2175	2219	rBV3	275979	747590	47.05%	6.378%
59	8.519	2324	2326	2328	rBV	422	223	0.01%	0.002%
60	8.551	2333	2336	2337	rBV2	601	315	0.02%	0.003%
61	8.599	2349	2351	2353	rBV2	327	133	0.01%	0.001%
62	8.638	2361	2363	2365	rBV2	274	125	0.01%	0.001%
63	8.689	2377	2379	2380	rBV	249	62	0.00%	0.001%
64	8.783	2397	2408	2431	rBV	725765	1204398	75.80%	10.274%
65	9.114	2509	2511	2512	rBV	369	189	0.01%	0.002%
66	9.140	2516	2519	2522	rBV3	390	331	0.02%	0.003%
67	9.226	2544	2546	2550	rBV2	202	143	0.01%	0.001%
68	9.246	2550	2552	2555	rVB	576	317	0.02%	0.003%
69	9.368	2588	2590	2592	rBV2	200	104	0.01%	0.001%
70	9.381	2592	2594	2596	rBV	151	68	0.00%	0.001%
71	9.423	2604	2607	2611	rBV2	392	369	0.02%	0.003%
72	9.461	2616	2619	2623	rBV2	139	124	0.01%	0.001%
73	9.548	2644	2646	2649	rBV	103	63	0.00%	0.001%
74	9.567	2650	2652	2654	rBV2	217	95	0.01%	0.001%
75	9.583	2654	2657	2658	rBV	209	95	0.01%	0.001%
76	9.635	2669	2673	2675	rBV	277	218	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
 Data File : VV035454.D
 Acq On : 27 Apr 2024 02:47
 Operator : SY/MD
 Sample : P2279-14 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 CORR7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
 Title : VOC Analysis

77	9.686	2687	2689	2690	rBV	156	68	0.00%	0.001%
78	9.847	2738	2739	2740	rBV	205	55	0.00%	0.000%
79	9.937	2765	2767	2768	rBV	250	126	0.01%	0.001%
80	10.062	2802	2806	2807	rBV2	133	88	0.01%	0.001%
81	10.152	2821	2834	2864	rBV	534234	852898	53.68%	7.276%
82	10.468	2930	2932	2934	rBV	171	53	0.00%	0.000%
83	10.484	2934	2937	2938	rBV2	331	127	0.01%	0.001%
84	10.763	3020	3024	3029	rBV4	305	308	0.02%	0.003%
85	10.792	3031	3033	3037	rVB2	293	159	0.01%	0.001%
86	10.950	3079	3082	3086	rBV2	327	204	0.01%	0.002%
87	11.185	3144	3155	3181	rBV	607204	976393	61.45%	8.329%
88	11.484	3244	3248	3252	rVB3	474	379	0.02%	0.003%
89	11.561	3260	3272	3302	rBV	580175	933546	58.75%	7.964%
90	11.821	3347	3353	3359	rBV4	564	801	0.05%	0.007%
91	11.963	3395	3397	3399	rBV2	373	191	0.01%	0.002%
92	12.204	3470	3472	3474	rBV	325	164	0.01%	0.001%
93	12.828	3663	3666	3667	rBV	292	150	0.01%	0.001%
94	12.947	3701	3703	3705	rBV	355	171	0.01%	0.001%
95	13.213	3783	3786	3789	rBV3	1020	807	0.05%	0.007%




Sum of corrected areas: 11722229

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035454.D
Acq On : 27 Apr 2024 02:47
Operator : SY/MD
Sample : P2279-14 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
CORR7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

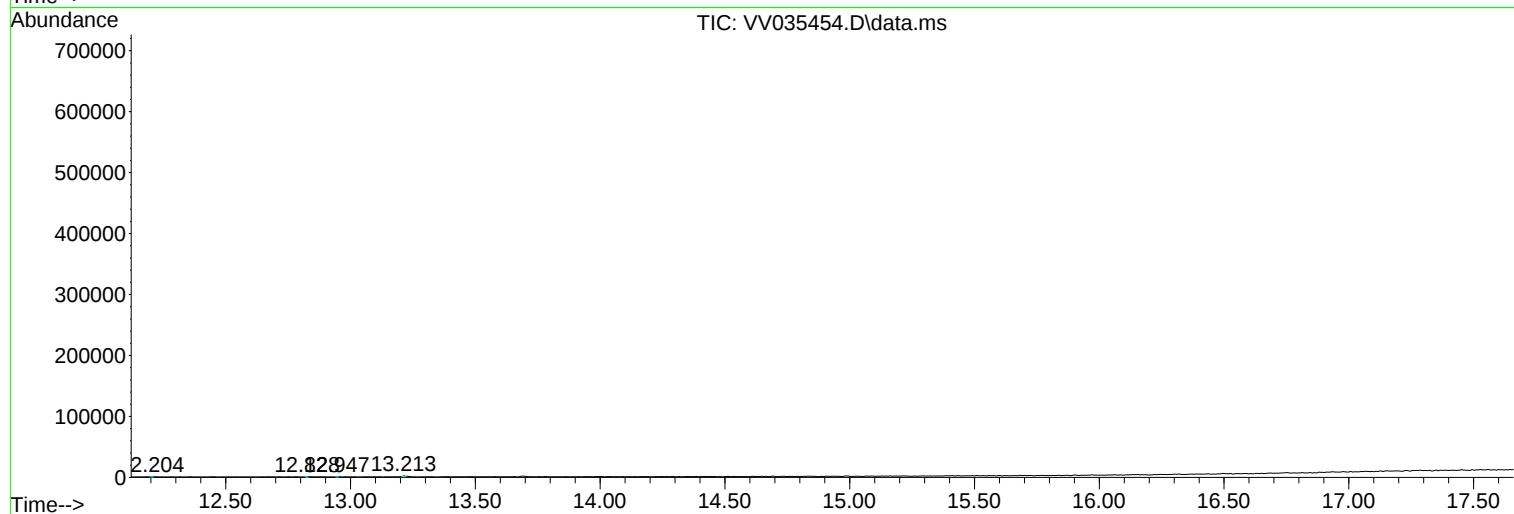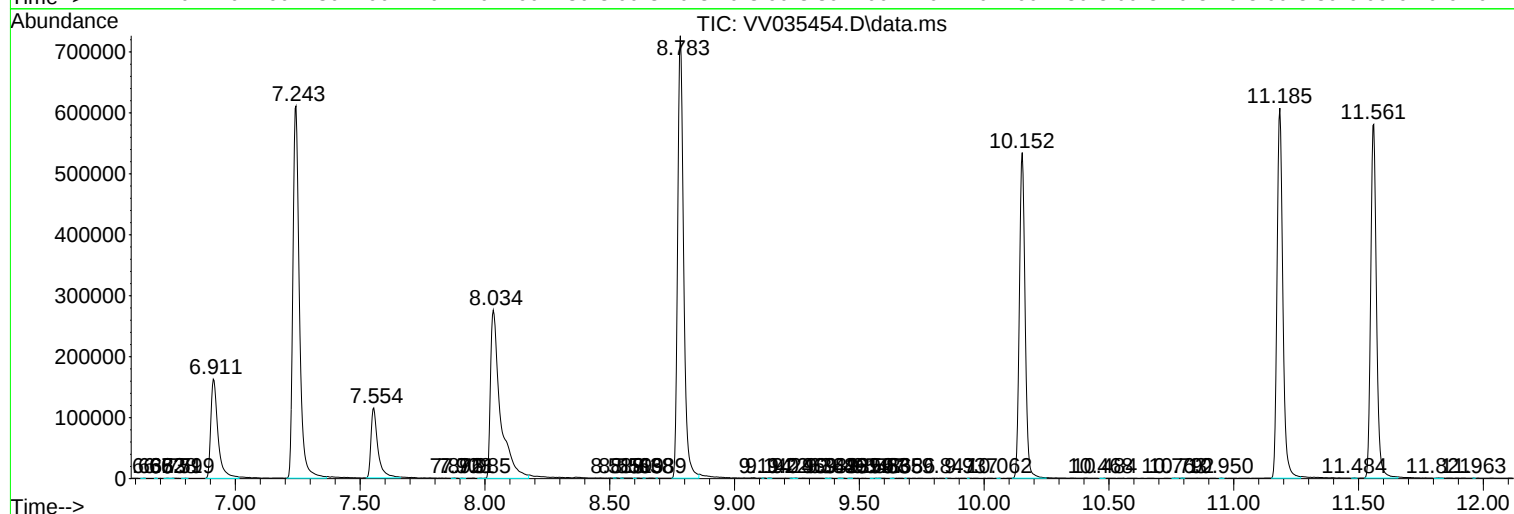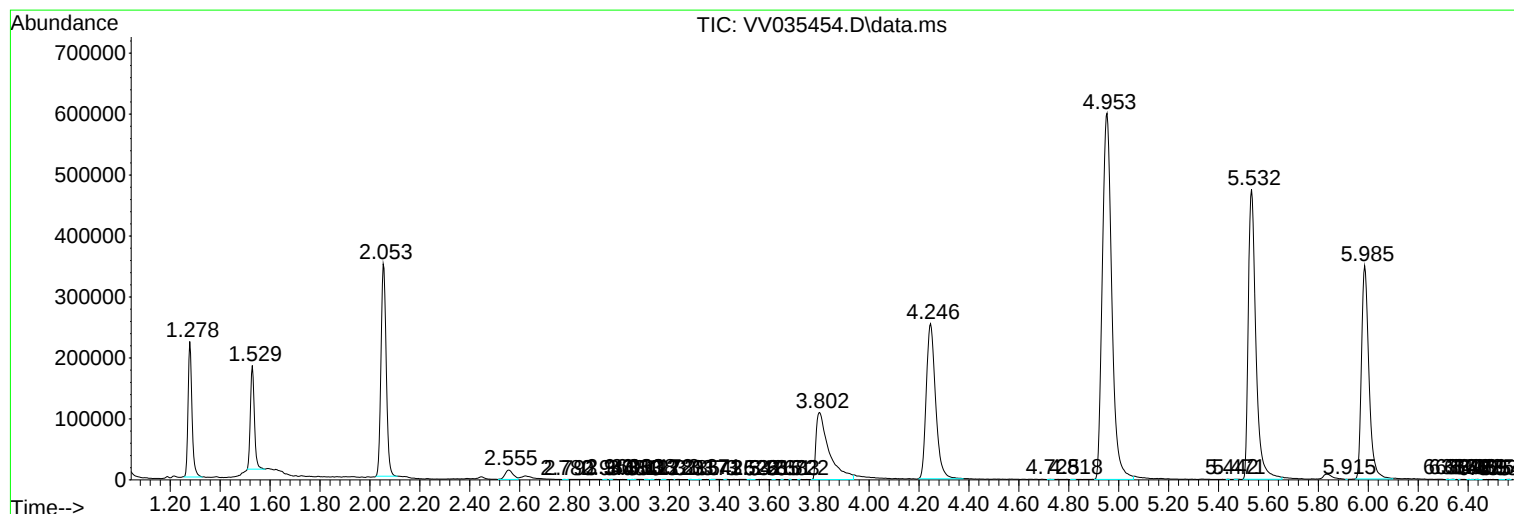

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035454.D
Acq On : 27 Apr 2024 02:47
Operator : SY/MD
Sample : P2279-14 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035454.D
Acq On : 27 Apr 2024 02:47
Operator : SY/MD
Sample : P2279-14 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0RR7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
