
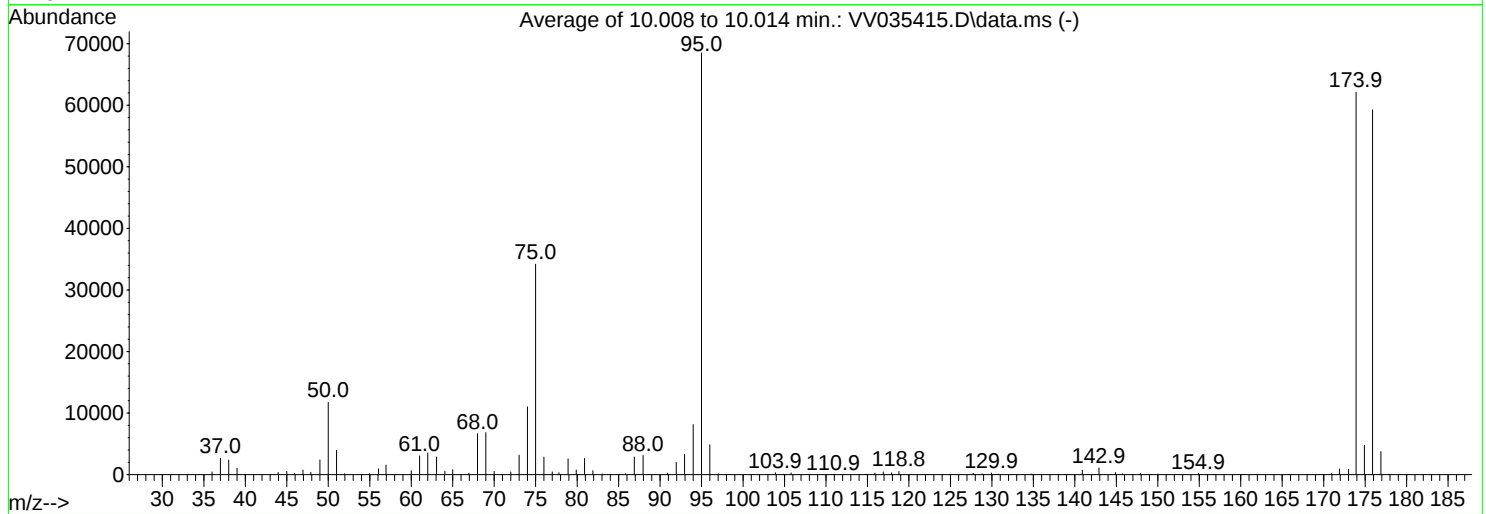


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042624\
Data File : VV035415.D
Acq On : 26 Apr 2024 09:01
Operator : SY/MD
Sample : BFB292
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB292

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042624WMA.M
Title : VOC Analysis
Last Update : Sat Apr 27 01:20:16 2024

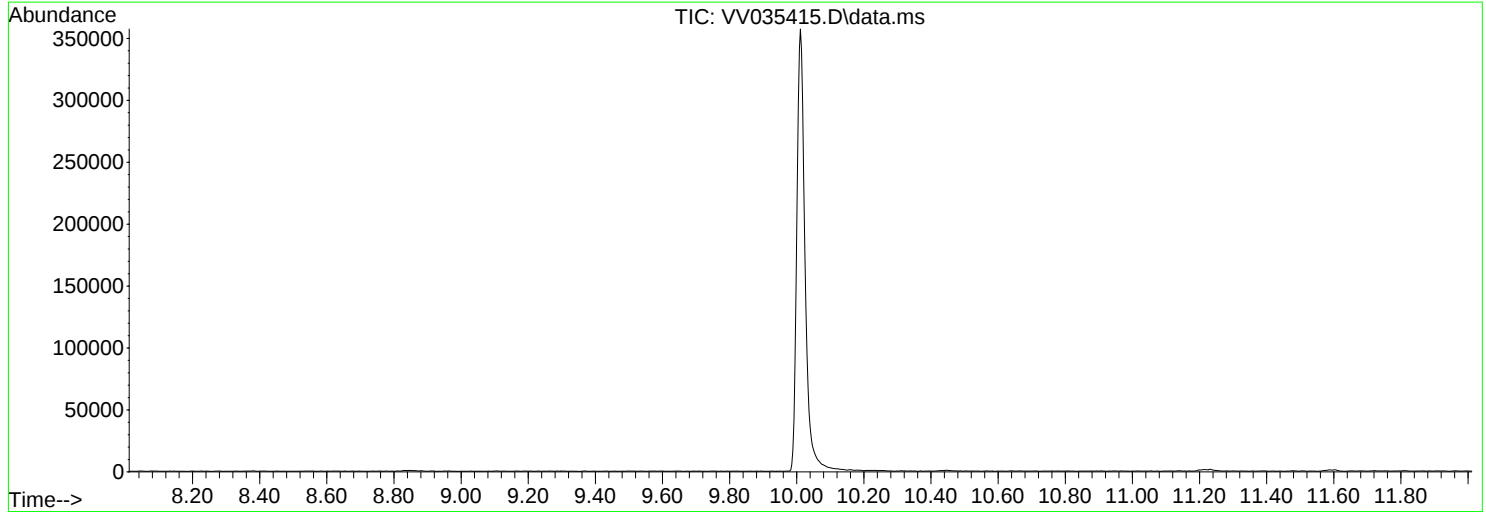

AutoFind: Scans 2789, 2790, 2791; Background Corrected with Scan 2779

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.2	11763	PASS
75	95	30	80	49.9	34187	PASS
95	95	100	100	100.0	68515	PASS
96	95	5	9	7.1	4864	PASS
173	174	0.00	2	1.4	853	PASS
174	95	50	120	90.7	62128	PASS
175	174	5	9	7.7	4767	PASS
176	174	95	105	95.4	59256	PASS
177	176	5	10	6.3	3757	PASS

m/z	Abundance
39.90	257.0
43.90	418.0

Instrument :
MSVOA_V
ClientSampleId :
BFB292

m/z	Abundance
36.00	462.0
37.00	2705.0
38.00	2517.0
39.00	1099.0
39.90	241.0
44.00	702.0
45.00	579.0
46.00	235.0
47.00	806.0
47.90	363.0
49.00	2408.0
50.00	12092.0
51.00	4041.0
52.00	142.0
53.00	102.0
54.90	141.0
56.10	980.0
57.00	1629.0
60.00	612.0
61.00	3040.0
62.00	3443.0
63.10	2805.0
64.10	621.0
65.00	821.0
66.90	238.0
68.00	6636.0
69.00	7039.0
70.00	512.0
72.00	397.0
73.00	3170.0
74.00	10706.0
75.00	34304.0
76.00	3049.0
77.10	412.0
77.80	272.0
78.90	2525.0
79.90	757.0
80.90	2687.0
81.90	610.0
85.90	174.0
86.90	2878.0
87.90	3106.0
90.80	238.0
91.90	1921.0
92.90	3379.0
94.00	8150.0
95.00	68040.0
96.00	4974.0
97.00	155.0
103.90	290.0
104.90	111.0
105.80	303.0
114.80	132.0
115.90	288.0
116.90	449.0
117.90	286.0
118.80	515.0
127.80	218.0
128.70	148.0
129.90	291.0
130.70	104.0
134.80	113.0
140.90	734.0
142.90	1119.0
144.90	450.0
145.70	108.0
148.00	158.0
154.90	154.0
156.70	116.0
171.00	164.0
171.90	897.0
173.00	796.0
173.90	59520.0
174.90	4671.0
175.90	57528.0
176.90	3563.0

Instrument :
MSVOA_V
ClientSampleId :
BFB292

m/z	Abundance
36.00	478.0
37.00	2730.0
38.00	2403.0
39.00	1023.0
39.90	275.0
44.00	825.0
45.00	547.0
45.90	273.0
46.90	760.0
47.90	369.0
49.00	2438.0
50.00	12166.0
51.00	4086.0
51.90	148.0
55.00	150.0
56.00	974.0
57.00	1582.0
60.00	668.0
61.00	3120.0
62.00	3609.0
63.10	2946.0
64.00	595.0
65.00	816.0
66.90	250.0
68.00	6802.0
69.00	7057.0
70.00	551.0
72.00	475.0
73.00	3310.0
74.00	11335.0
75.00	35336.0
76.00	2927.0
77.00	471.0
77.80	327.0
78.90	2690.0
79.90	756.0
80.90	2685.0
81.90	683.0
83.10	125.0
85.80	173.0
86.90	3000.0
88.00	3187.0
90.90	258.0
91.90	2097.0
93.00	3427.0
94.00	8398.0
95.00	70592.0
96.00	4976.0
97.10	126.0
103.90	333.0
104.90	117.0
105.80	305.0
114.90	105.0
115.90	276.0
116.90	479.0
117.90	321.0
118.80	545.0
127.70	243.0
128.80	139.0
130.00	275.0
130.80	125.0
134.80	114.0
140.90	777.0
142.90	1099.0
144.90	382.0
145.80	130.0
148.00	169.0
150.00	119.0
154.90	185.0
156.90	117.0
171.00	159.0
171.90	936.0
173.00	903.0
173.90	64288.0
174.90	4947.0
175.90	61048.0
176.90	3848.0
177.80	129.0

Instrument :
MSVOA_V
ClientSampleId :
BFB292

m/z	Abundance
36.00	405.0
37.00	2566.0
38.00	2197.0
39.00	962.0
39.90	297.0
44.00	828.0
45.00	467.0
45.90	233.0
46.90	726.0
47.90	410.0
49.00	2367.0
50.00	11032.0
51.00	3736.0
51.90	172.0
55.00	177.0
56.00	949.0
56.90	1441.0
60.00	660.0
61.00	2997.0
62.00	3476.0
63.00	2870.0
64.00	544.0
65.00	753.0
67.00	224.0
68.00	6534.0
69.00	6406.0
70.00	528.0
72.00	467.0
73.00	3044.0
74.00	11007.0
75.00	32920.0
76.00	2583.0
76.90	479.0
77.80	332.0
78.90	2543.0
79.90	727.0
80.90	2507.0
81.90	690.0
83.00	152.0
85.80	152.0
86.90	2677.0
88.00	3049.0
91.00	323.0
92.00	2012.0
93.00	3038.0
94.00	7873.0
95.00	66912.0
96.00	4642.0
97.10	118.0
103.90	312.0
105.80	271.0
110.90	119.0
115.90	257.0
116.90	436.0
117.90	324.0
118.80	506.0
127.80	252.0
128.90	128.0
130.00	211.0
130.80	122.0
134.70	119.0
140.90	680.0
142.90	1032.0
144.90	278.0
145.80	162.0
147.80	206.0
150.00	104.0
154.90	195.0
156.90	116.0
170.90	174.0
171.90	977.0
173.00	861.0
173.90	62576.0
174.90	4683.0
175.90	59192.0
176.90	3860.0
177.90	137.0

Instrument :
MSVOA_V
ClientSampleId :
BFB292