

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV042719\
 Data File : VV010534.D
 Acq On : 27 Apr 2019 07:18
 Operator : SY/MD
 Sample : K2586-12
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0X45

Quant Time: Apr 29 02:29:58 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042719WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Apr 29 01:58:06 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	223808	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	214383	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	98899	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	53708	4.93	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	98.60%
7) Chloroethane-d5	1.57	69	37746	6.48	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	129.60%
11) 1,1-Dichloroethene-d2	2.12	63	74921	3.66	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.20%
20) 2-Butanone-d5	3.93	46	124958	44.51	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.02%
24) Chloroform-d	4.40	84	132638	4.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.80%
26) 1,2-Dichloroethane-d4	5.08	65	70496	5.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.80%
32) Benzene-d6	5.10	84	285022	5.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.80%
36) 1,2-Dichloropropane-d6	6.12	67	78597	5.21	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	104.20%
41) Toluene-d8	7.36	98	244692	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.80%
43) trans-1,3-Dichloropropene-	7.66	79	24791	4.30	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.00%
46) 2-Hexanone-d5	8.13	63	113818	46.77	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.54%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	57499	4.80	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	111065	5.83	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.60%


Target Compounds					Ovalue
13) Acetone	2.19	43	24000	17.159 ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV042719\
Data File : VV010534.D
Acq On : 27 Apr 2019 07:18
Operator : SY/MD
Sample : K2586-12
Misc : 25mL/MSVOA V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0X45

Quant Time: Apr 29 02:29:58 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Apr 29 01:58:06 2019
Response via : Initial Calibration

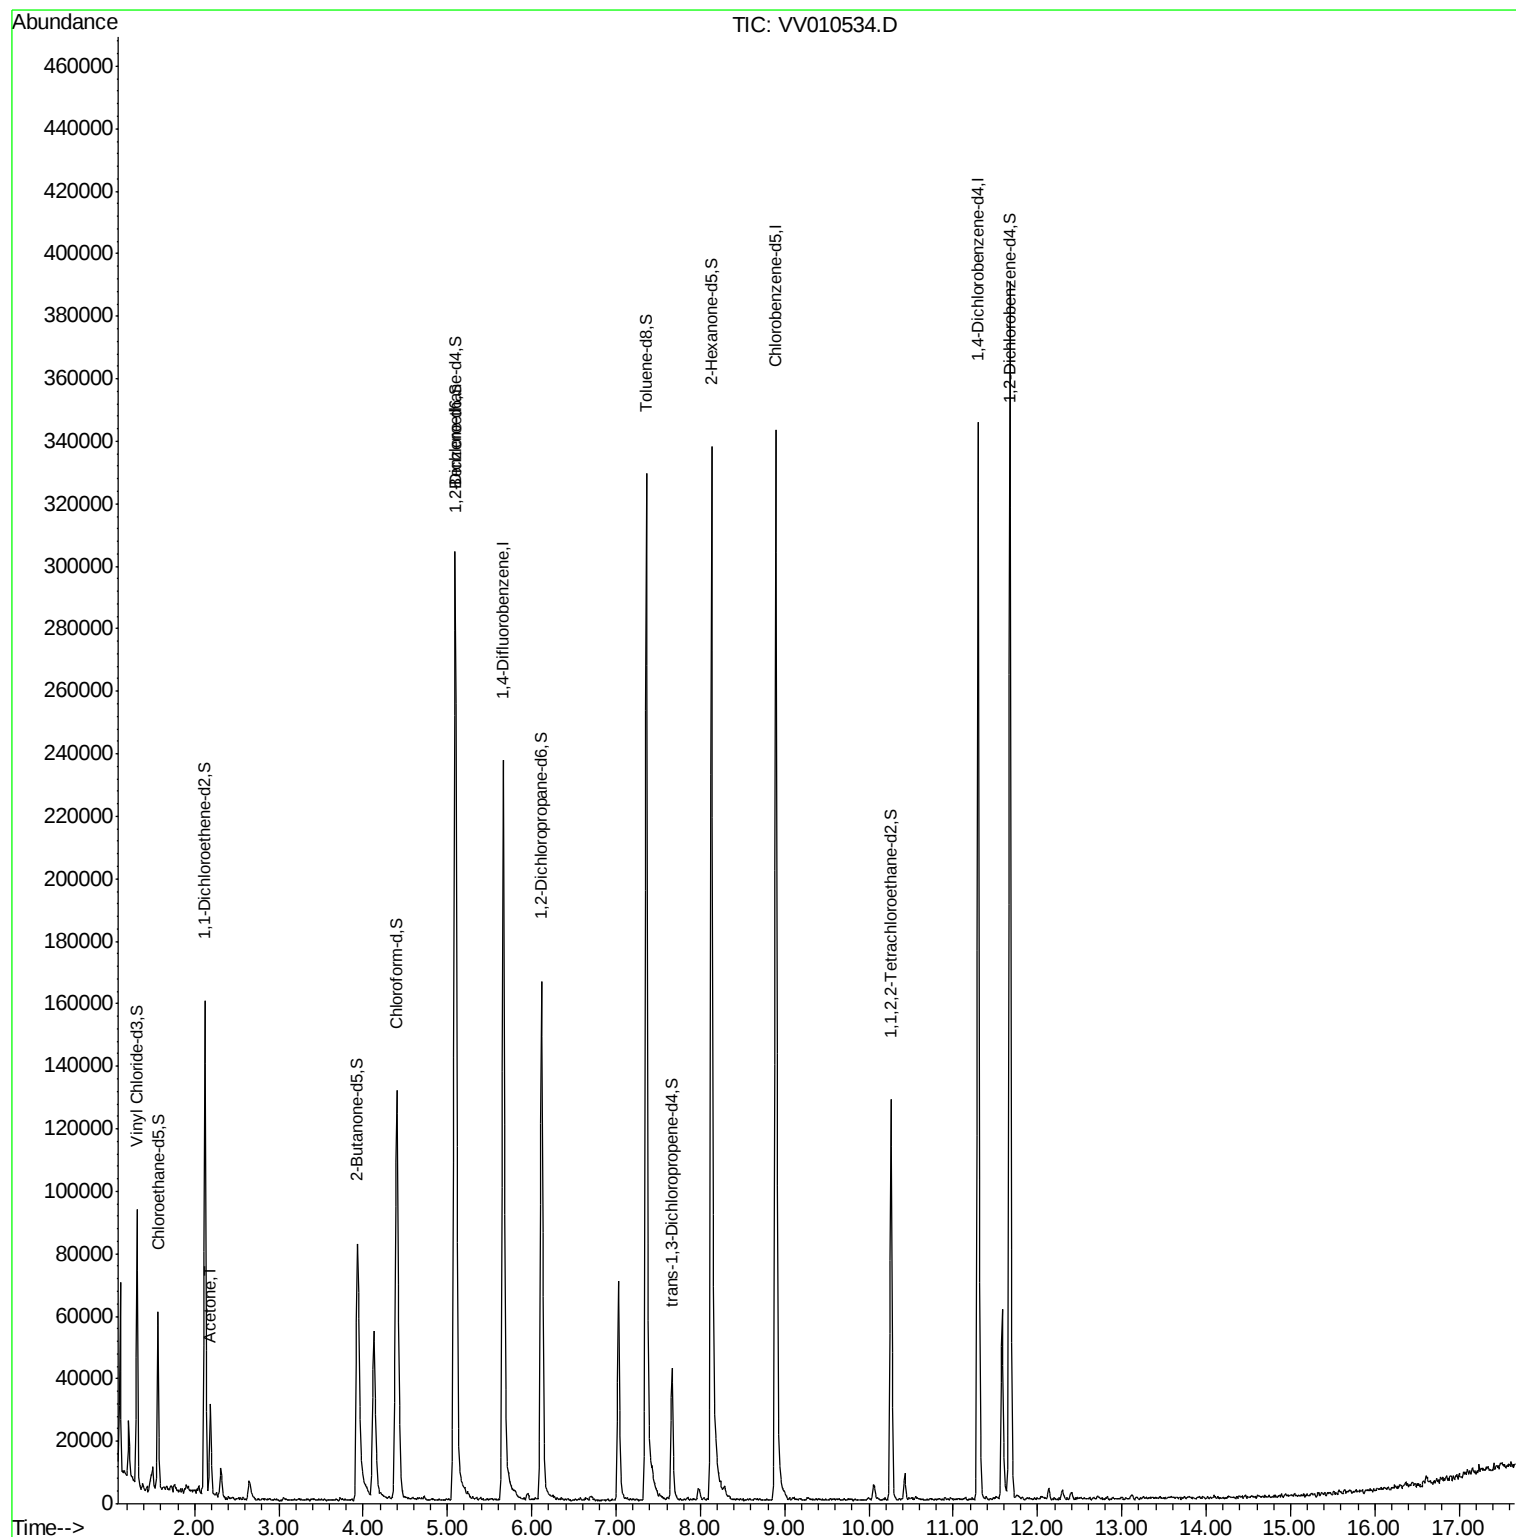

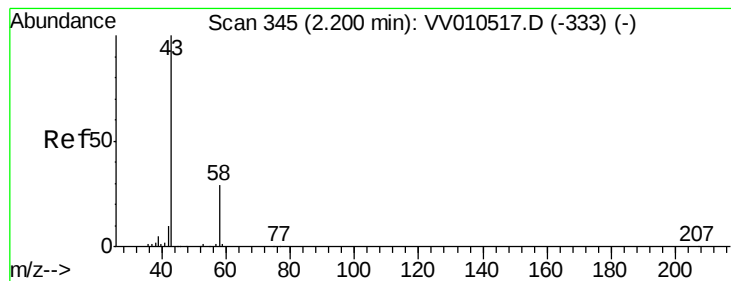

#13

Acetone

Concen: 17.159 ug/L

RT: 2.19 min Scan# 341

Delta R.T. -0.01 min

Lab File: VV010534.D

Acq: 27 Apr 2019 07:18

Instrument :

MSVOA_V

ClientSampleId :

C0X45

Tot Ion: 43 Resp: 24000

Ion Ratio Lower Upper

43 100

58 33.2 0.0 57.4

