


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042719\
Data File : VV010510.D
Acq On : 26 Apr 2019 17:50
Operator : SY/MD
Sample : BFB38
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB38

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042719WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Apr 29 01:58:06 2019

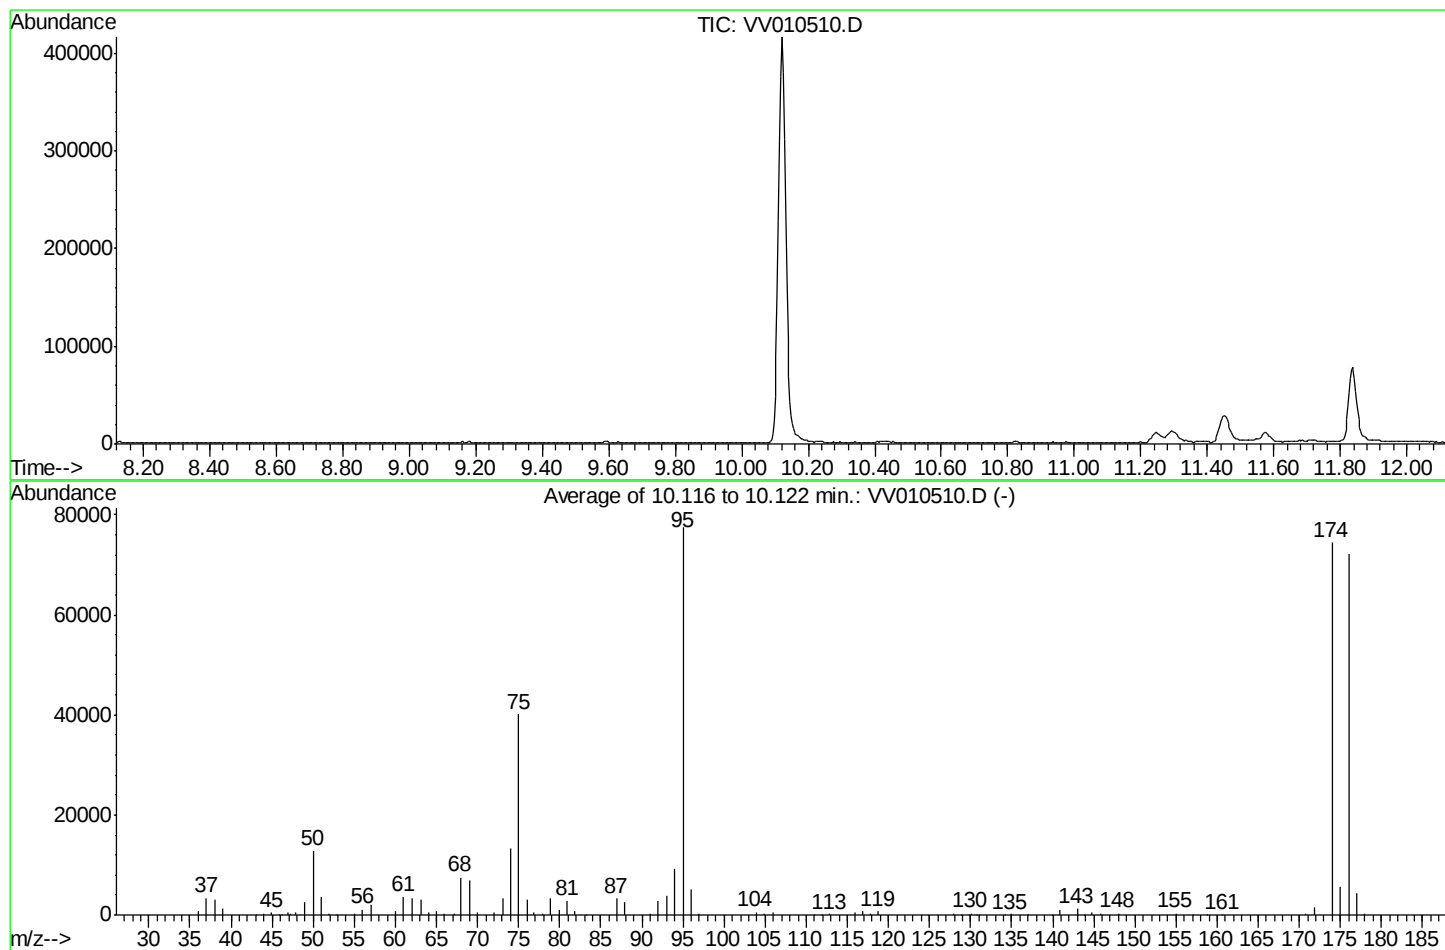

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	12802	PASS
75	95	30	80	51.8	40168	PASS
95	95	100	100	100.0	77504	PASS
96	95	5	9	6.6	5154	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	95.9	74349	PASS
175	174	5	9	7.5	5555	PASS
176	174	95	101	96.9	72066	PASS
177	176	5	9	6.1	4400	PASS

Scan 2795 (10.077 min): VV010510.D
BFB38

m/z	Abundance
40.00	1078.0
44.00	507.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38

m/z	Abundance
36.00	692.0
37.00	3513.0
38.00	2838.0
39.00	1237.0
39.80	1110.0
43.00	104.0
43.90	788.0
44.90	444.0
46.90	688.0
47.80	339.0
49.00	2675.0
50.00	12294.0
51.00	3624.0
52.00	188.0
55.00	226.0
55.90	1115.0
57.00	2079.0
59.90	771.0
61.00	3431.0
62.00	3414.0
63.10	3034.0
64.10	547.0
64.90	730.0
65.90	133.0
67.10	220.0
67.90	7181.0
69.00	6404.0
70.00	563.0
72.00	513.0
73.00	3202.0
74.00	12461.0
75.00	38040.0
76.10	2910.0
76.90	461.0
78.90	3214.0
79.90	795.0
80.90	2699.0
81.90	797.0
83.20	102.0
86.90	3144.0
87.90	2440.0
90.90	367.0
92.00	2502.0
93.00	3644.0
94.00	8642.0
95.00	72944.0
96.00	5071.0
96.90	169.0
103.90	524.0
104.90	131.0
105.90	571.0
111.80	139.0
112.90	127.0
116.00	426.0
116.80	784.0
117.80	234.0
118.80	745.0
127.90	218.0
130.00	255.0
131.10	180.0
134.90	122.0
137.10	102.0
140.90	926.0
143.00	1049.0
143.80	155.0
144.70	338.0
145.80	150.0
148.00	293.0
155.00	230.0
158.80	115.0
170.80	146.0
171.90	1292.0
174.00	69128.0
175.00	5241.0
176.00	64224.0
177.00	4255.0
177.90	215.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38

m/z	Abundance
36.10	827.0
37.00	3460.0
38.00	3071.0
39.00	1253.0
39.90	1011.0
43.00	108.0
44.00	751.0
44.90	451.0
45.90	120.0
46.90	548.0
47.30	417.0
47.90	438.0
49.00	2786.0
50.00	13062.0
51.00	3676.0
51.90	193.0
54.90	276.0
56.00	1070.0
57.00	2053.0
59.90	893.0
61.00	3693.0
62.10	3473.0
63.10	3114.0
64.10	636.0
65.00	837.0
65.90	157.0
67.20	258.0
68.00	7685.0
69.00	7105.0
70.00	597.0
72.00	483.0
73.10	3406.0
74.00	13884.0
75.00	41416.0
76.10	3052.0
76.90	521.0
77.80	338.0
78.90	3489.0
79.90	944.0
80.90	2915.0
81.80	848.0
83.30	118.0
87.00	3299.0
88.00	2771.0
90.90	392.0
91.90	2947.0
93.00	3899.0
94.00	9399.0
95.00	79888.0
96.10	5389.0
97.00	145.0
103.90	585.0
104.90	165.0
105.90	570.0
112.80	160.0
116.00	511.0
116.80	694.0
117.70	272.0
118.80	800.0
128.00	284.0
128.90	111.0
130.10	279.0
131.10	169.0
134.90	142.0
137.00	121.0
140.90	1081.0
143.00	1188.0
143.70	136.0
144.70	440.0
145.80	195.0
148.00	317.0
155.00	290.0
158.80	102.0
170.80	146.0
171.90	1538.0
174.00	76600.0
175.00	5875.0
176.00	74448.0
177.00	4376.0
177.90	202.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38

m/z	Abundance
36.10	838.0
37.00	3264.0
38.00	3015.0
39.00	1170.0
39.90	942.0
44.00	721.0
45.00	462.0
46.20	123.0
46.80	534.0
47.90	497.0
49.00	2605.0
50.00	13050.0
51.00	3498.0
51.90	236.0
52.90	129.0
54.90	281.0
56.10	940.0
57.00	2036.0
60.00	906.0
61.00	3723.0
62.10	3369.0
63.00	2921.0
64.10	570.0
65.00	898.0
65.90	124.0
67.10	252.0
68.00	7451.0
69.00	7288.0
69.90	616.0
72.10	445.0
73.10	3506.0
74.00	13828.0
75.00	41048.0
76.10	3001.0
76.80	549.0
77.90	525.0
78.90	3348.0
79.90	1035.0
80.90	3104.0
81.80	751.0
87.00	3319.0
88.00	2816.0
91.00	415.0
91.90	2717.0
93.00	3757.0
94.00	9620.0
95.00	79680.0
96.10	5003.0
97.10	134.0
103.90	507.0
104.90	140.0
105.90	473.0
111.00	116.0
112.90	137.0
115.90	455.0
116.90	677.0
117.70	300.0
118.80	699.0
128.00	294.0
128.90	116.0
129.80	268.0
130.10	286.0
130.80	140.0
134.20	106.0
134.90	156.0
136.90	148.0
139.90	105.0
140.90	1169.0
143.00	1324.0
144.70	423.0
145.80	184.0
148.00	246.0
154.90	343.0
157.10	105.0
160.70	107.0
170.80	128.0
171.90	1611.0
174.00	77320.0
175.00	5550.0
176.00	77528.0
177.00	4571.0
177.90	171.0

Instrument :
MSVOA_V
ClientSampleId :
BFB38