


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV042720\
 Data File : VV015716.D
 Acq On : 27 Apr 2020 09:26
 Operator : SY/MD
 Sample : BFB44
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB44

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR042220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Apr 28 02:16:08 2020

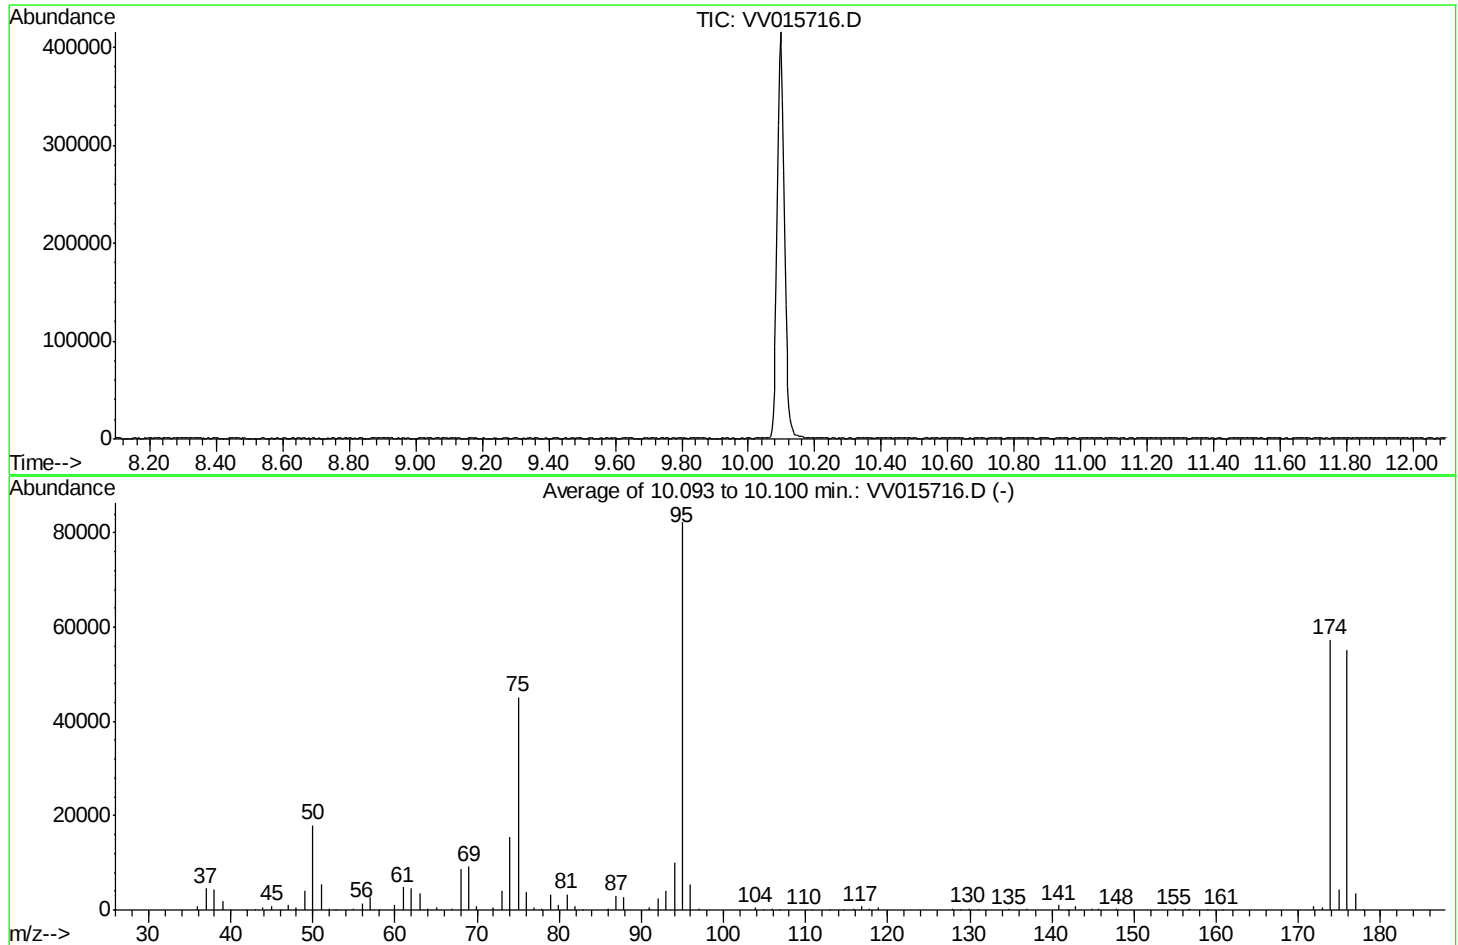

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2787

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	18005	PASS
75	95	30	80	54.9	45178	PASS
95	95	100	100	100.0	82242	PASS
96	95	5	9	6.6	5411	PASS
173	174	0.00	2	0.8	467	PASS
174	95	50	120	69.7	57314	PASS
175	174	5	9	7.4	4222	PASS
176	174	95	101	96.4	55250	PASS
177	176	5	9	6.6	3673	PASS

m/z	Abundance
36.00	844.0
37.00	4431.0
38.00	4321.0
39.00	1861.0
39.90	445.0
41.80	103.0
44.00	1039.0
45.00	939.0
46.10	126.0
47.00	1030.0
48.00	574.0
49.00	3976.0
50.00	17656.0
51.00	5364.0
52.00	273.0
52.80	139.0
55.00	315.0
56.00	1444.0
57.00	2520.0
60.00	1018.0
61.00	4646.0
62.00	4742.0
63.00	3398.0
64.00	372.0
65.00	618.0
67.00	254.0
68.00	8455.0
69.00	9078.0
69.90	787.0
71.90	542.0
73.00	3939.0
74.00	14931.0
75.00	43800.0
76.00	3984.0
77.00	520.0
77.90	348.0
78.90	3003.0
79.90	1019.0
80.90	3334.0
81.90	724.0
82.80	144.0
85.90	154.0
86.90	3050.0
87.90	2747.0
90.90	437.0
92.00	2439.0
93.00	3902.0
94.00	9807.0
95.00	79280.0
96.00	5337.0
97.00	175.0
103.90	462.0
104.80	123.0
105.90	366.0
106.90	144.0
109.90	122.0
110.80	104.0
112.90	128.0
114.70	121.0
115.90	348.0
116.80	666.0
117.80	393.0
118.90	547.0
127.90	382.0
128.90	137.0
129.90	345.0
131.00	102.0
134.80	188.0
136.90	205.0
140.90	989.0
141.80	112.0
142.90	947.0
144.90	228.0
145.70	151.0
147.80	177.0
155.00	200.0
156.70	118.0
158.90	103.0
160.70	101.0
171.90	698.0
173.90	53968.0
175.00	4045.0
175.90	52040.0
177.00	3609.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

m/z	Abundance
36.00	843.0
37.00	4628.0
38.00	4544.0
39.00	1930.0
39.90	447.0
41.90	113.0
43.90	999.0
45.00	943.0
46.10	151.0
47.00	1071.0
48.00	589.0
49.00	4185.0
50.00	18624.0
51.00	5613.0
52.00	284.0
52.80	130.0
55.00	323.0
56.00	1526.0
57.00	2797.0
58.00	102.0
60.00	976.0
61.00	4982.0
62.00	4841.0
63.00	3655.0
64.00	385.0
65.00	641.0
67.00	287.0
68.00	9162.0
69.00	9472.0
69.90	749.0
71.80	543.0
73.00	4182.0
74.00	16040.0
75.00	46960.0
76.00	4114.0
76.90	549.0
77.90	302.0
78.90	3272.0
79.90	1083.0
80.90	3499.0
81.90	745.0
82.90	158.0
86.00	173.0
87.00	3112.0
87.90	2797.0
90.90	442.0
92.00	2416.0
93.00	4193.0
94.00	10397.0
95.00	85504.0
96.00	5613.0
96.90	156.0
103.90	501.0
104.80	149.0
105.90	410.0
106.90	140.0
112.90	123.0
115.90	374.0
116.80	744.0
117.80	418.0
118.90	617.0
127.90	359.0
128.80	123.0
129.90	363.0
131.00	121.0
134.80	193.0
136.80	253.0
140.90	1004.0
141.90	111.0
142.90	971.0
144.90	247.0
145.70	190.0
147.90	229.0
154.90	229.0
156.70	155.0
160.80	116.0
171.90	716.0
173.00	729.0
173.90	59376.0
175.00	4410.0
175.90	57264.0
177.00	3790.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

m/z	Abundance
35.90	811.0
37.00	4448.0
38.00	4229.0
39.00	1878.0
39.90	426.0
41.90	111.0
43.00	111.0
43.90	917.0
45.00	800.0
46.10	150.0
47.00	1007.0
48.00	554.0
49.00	3824.0
50.00	17736.0
51.00	5343.0
52.00	294.0
52.80	110.0
55.00	298.0
56.00	1499.0
57.00	2736.0
58.00	121.0
60.00	916.0
61.00	4699.0
62.00	4469.0
63.00	3479.0
64.00	396.0
65.00	601.0
66.90	282.0
68.00	8792.0
69.00	8928.0
70.00	657.0
71.80	487.0
73.00	3894.0
74.00	15348.0
75.00	44776.0
76.00	3715.0
76.90	481.0
77.90	221.0
78.90	3200.0
79.90	1043.0
80.90	3352.0
81.90	718.0
82.80	135.0
86.00	154.0
87.00	2926.0
87.90	2576.0
90.90	388.0
92.00	2230.0
93.00	3922.0
94.00	9884.0
95.00	81944.0
96.00	5285.0
96.90	123.0
103.90	497.0
104.90	147.0
105.80	425.0
115.90	351.0
116.80	750.0
117.80	396.0
118.90	603.0
127.80	297.0
128.70	116.0
129.80	357.0
130.90	129.0
134.80	177.0
136.80	267.0
140.90	973.0
142.90	908.0
144.90	224.0
145.70	189.0
147.90	242.0
154.90	257.0
156.80	181.0
160.80	136.0
171.90	664.0
172.90	674.0
173.90	58600.0
175.00	4212.0
175.90	56448.0
177.00	3621.0
177.90	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44

Scan 2787 (10.051 min): VV015716.D
BFB44

m/z	Abundance
39.90	358.0
43.90	418.0

Instrument :
MSVOA_V
ClientSampleId :
BFB44