

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
 Data File : VV021164.D
 Acq On : 27 Apr 2021 10:35
 Operator : SY/MD
 Sample : VV0427MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Apr 28 03:28:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 28 03:28:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	669085	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	644894	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	306861	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	260036	47.30	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	94.60%		
7) Chloroethane-d5	1.571	69	196496	48.58	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	97.16%		
11) 1,1-Dichloroethene-d2	2.108	63	361901	35.69	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	71.38%		
21) 2-Butanone-d5	3.899	46	263974	98.32	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	98.32%		
24) Chloroform-d	4.352	84	467503	47.70	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.40%		
26) 1,2-Dichloroethane-d4	5.034	65	314017	50.40	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.80%		
32) Benzene-d6	5.050	84	855522	49.81	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.62%		
36) 1,2-Dichloropropane-d6	6.072	67	251636	49.08	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	98.16%		
41) Toluene-d8	7.317	98	799224	48.08	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.16%		
43) trans-1,3-Dichloroprop...	7.625	79	136102	48.58	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	97.16%		
47) 2-Hexanone-d5	8.091	63	195027	95.92	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	95.92%		
56) 1,1,2,2-Tetrachloroeth...	10.220	84	355716	46.00	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	92.00%		
66) 1,2-Dichlorobenzene-d4	11.632	152	328857	54.25	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	108.50%		
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.625	75	7134	0.96	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
Data File : VV021164.D
Acq On : 27 Apr 2021 10:35
Operator : SY/MD
Sample : VV0427MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Apr 28 03:28:47 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 28 03:28:03 2021
Response via : Initial Calibration

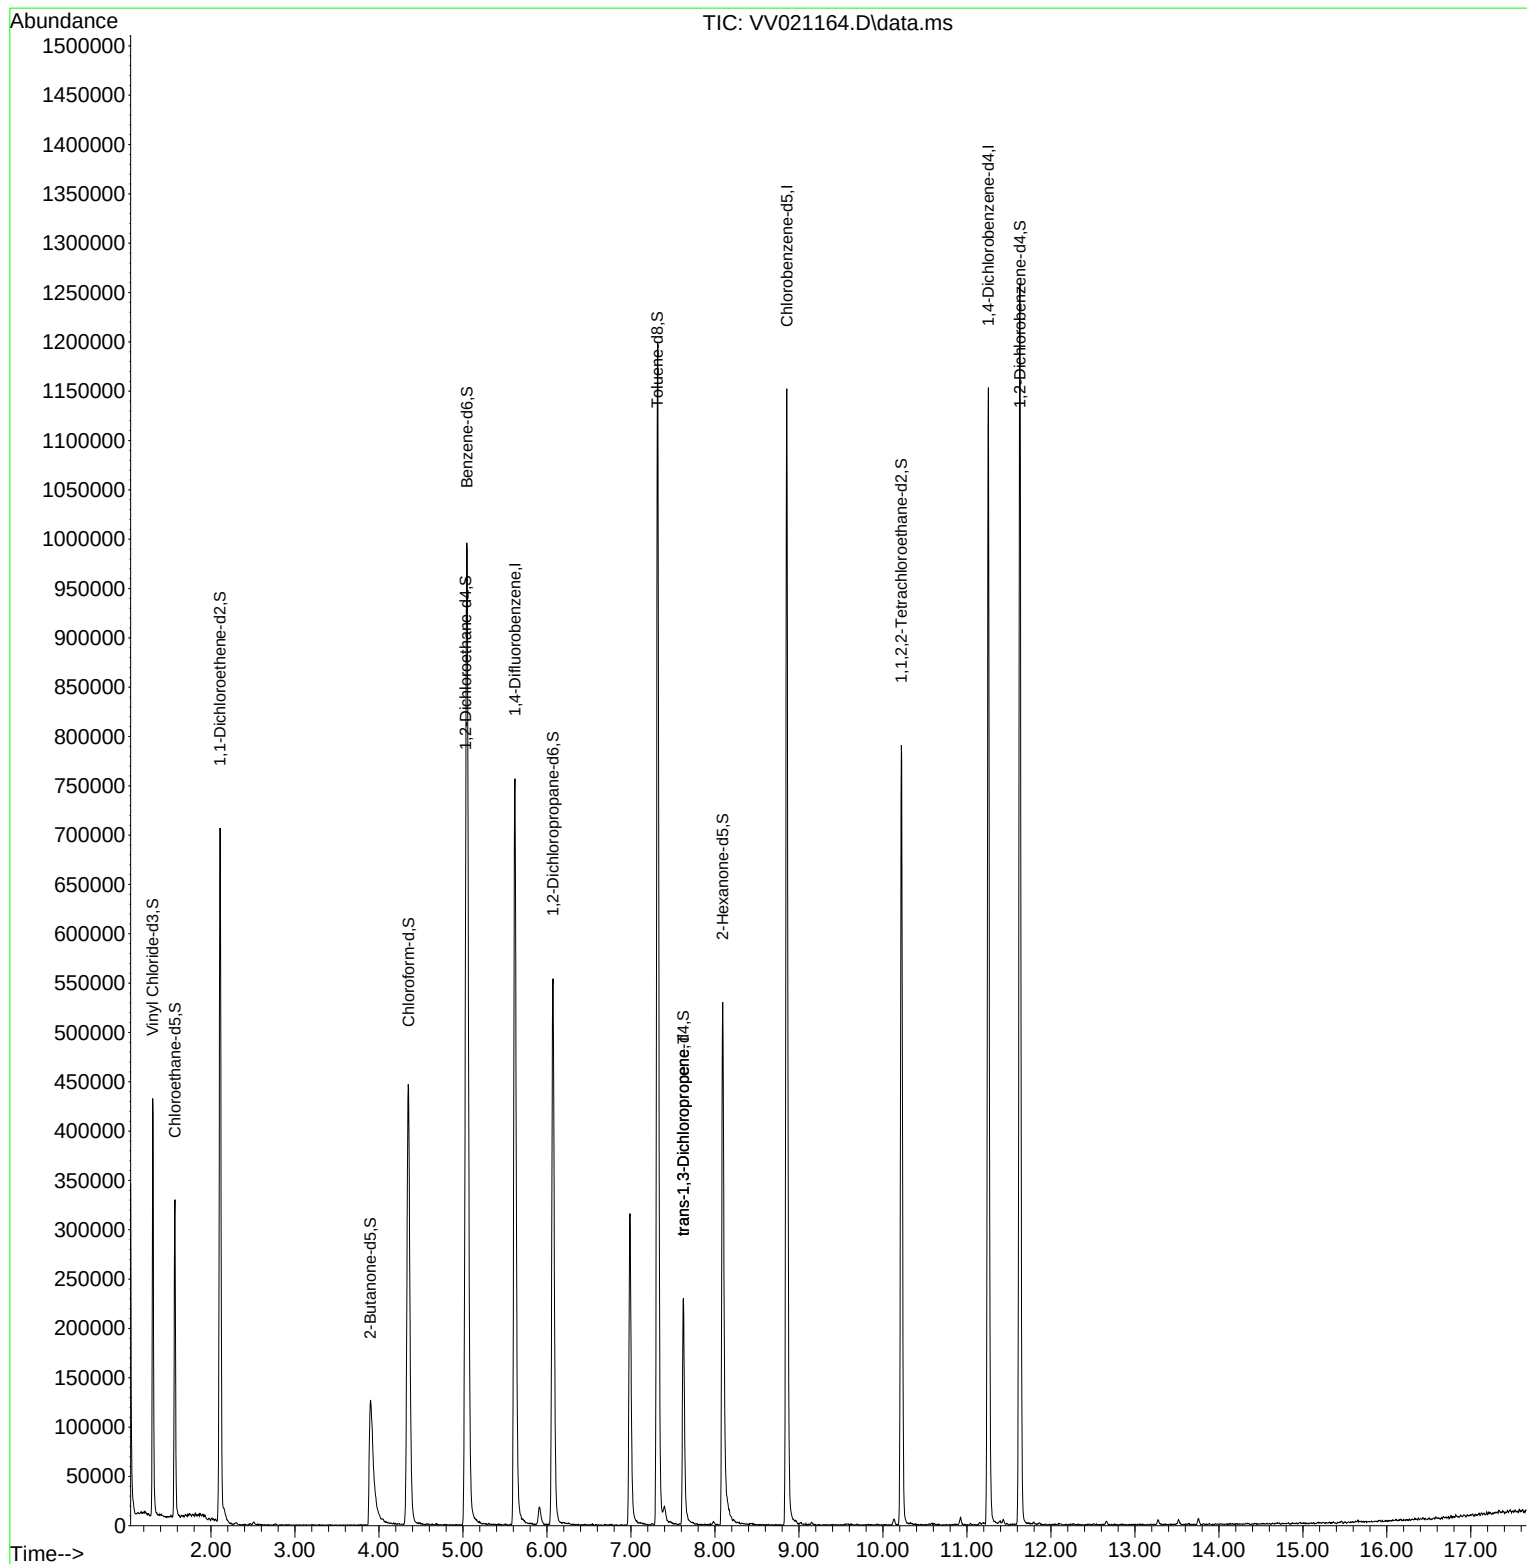

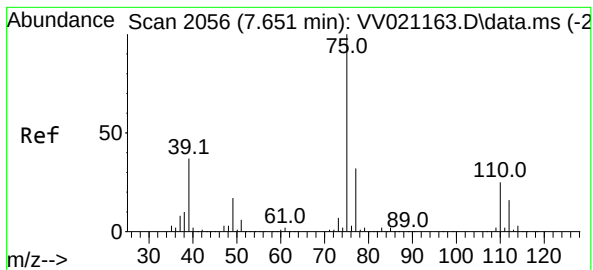

#44
 trans-1,3-Dichloropropene
 Concen: 0.96 ug/L
 RT: 7.625 min Scan# 2048
 Delta R.T. -0.026 min
 Lab File: VV021164.D
 Acq: 27 Apr 2021 10:35

Instrument :
 MSVOA_V
 ClientSampleId :

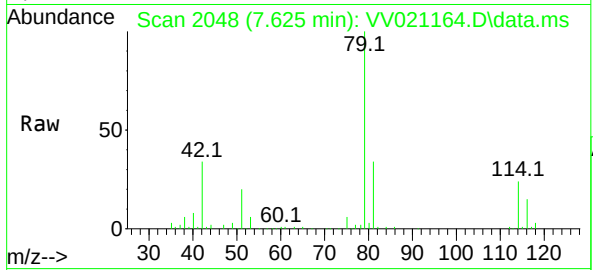

Tgt Ion: 75 Resp: 7134
 Ion Ratio Lower Upper
 75 100
 77 34.9 21.8 40.6

