

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
 Data File : VV021168.D
 Acq On : 27 Apr 2021 12:18
 Operator : SY/MD
 Sample : M2123-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Apr 28 03:29:27 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 28 03:28:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	654314	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	637634	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	299813	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	238334	44.33	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	88.66%
7) Chloroethane-d5	1.571	69	188207	47.58	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	95.16%
11) 1,1-Dichloroethene-d2	2.108	63	334370	33.72	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.44%
21) 2-Butanone-d5	3.899	46	247850	94.40	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	94.40%
24) Chloroform-d	4.352	84	439058	45.81	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.62%
26) 1,2-Dichloroethane-d4	5.034	65	303059	49.74	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.48%
32) Benzene-d6	5.053	84	804708	47.39	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.78%
36) 1,2-Dichloropropane-d6	6.072	67	243096	47.96	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.92%
41) Toluene-d8	7.320	98	769239	46.80	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.60%
43) trans-1,3-Dichloroprop...	7.625	79	127967	46.20	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.40%
47) 2-Hexanone-d5	8.091	63	193949	96.47	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	96.47%
56) 1,1,2,2-Tetrachloroeth...	10.223	84	347811	45.49	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.98%
66) 1,2-Dichlorobenzene-d4	11.632	152	316718	53.48	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.96%
Target Compounds						
44) trans-1,3-Dichloropropene	7.625	75	5719	0.78	ug/L	Qvalue # 83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
Data File : VV021168.D
Acq On : 27 Apr 2021 12:18
Operator : SY/MD
Sample : M2123-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Apr 28 03:29:27 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 28 03:28:03 2021
Response via : Initial Calibration

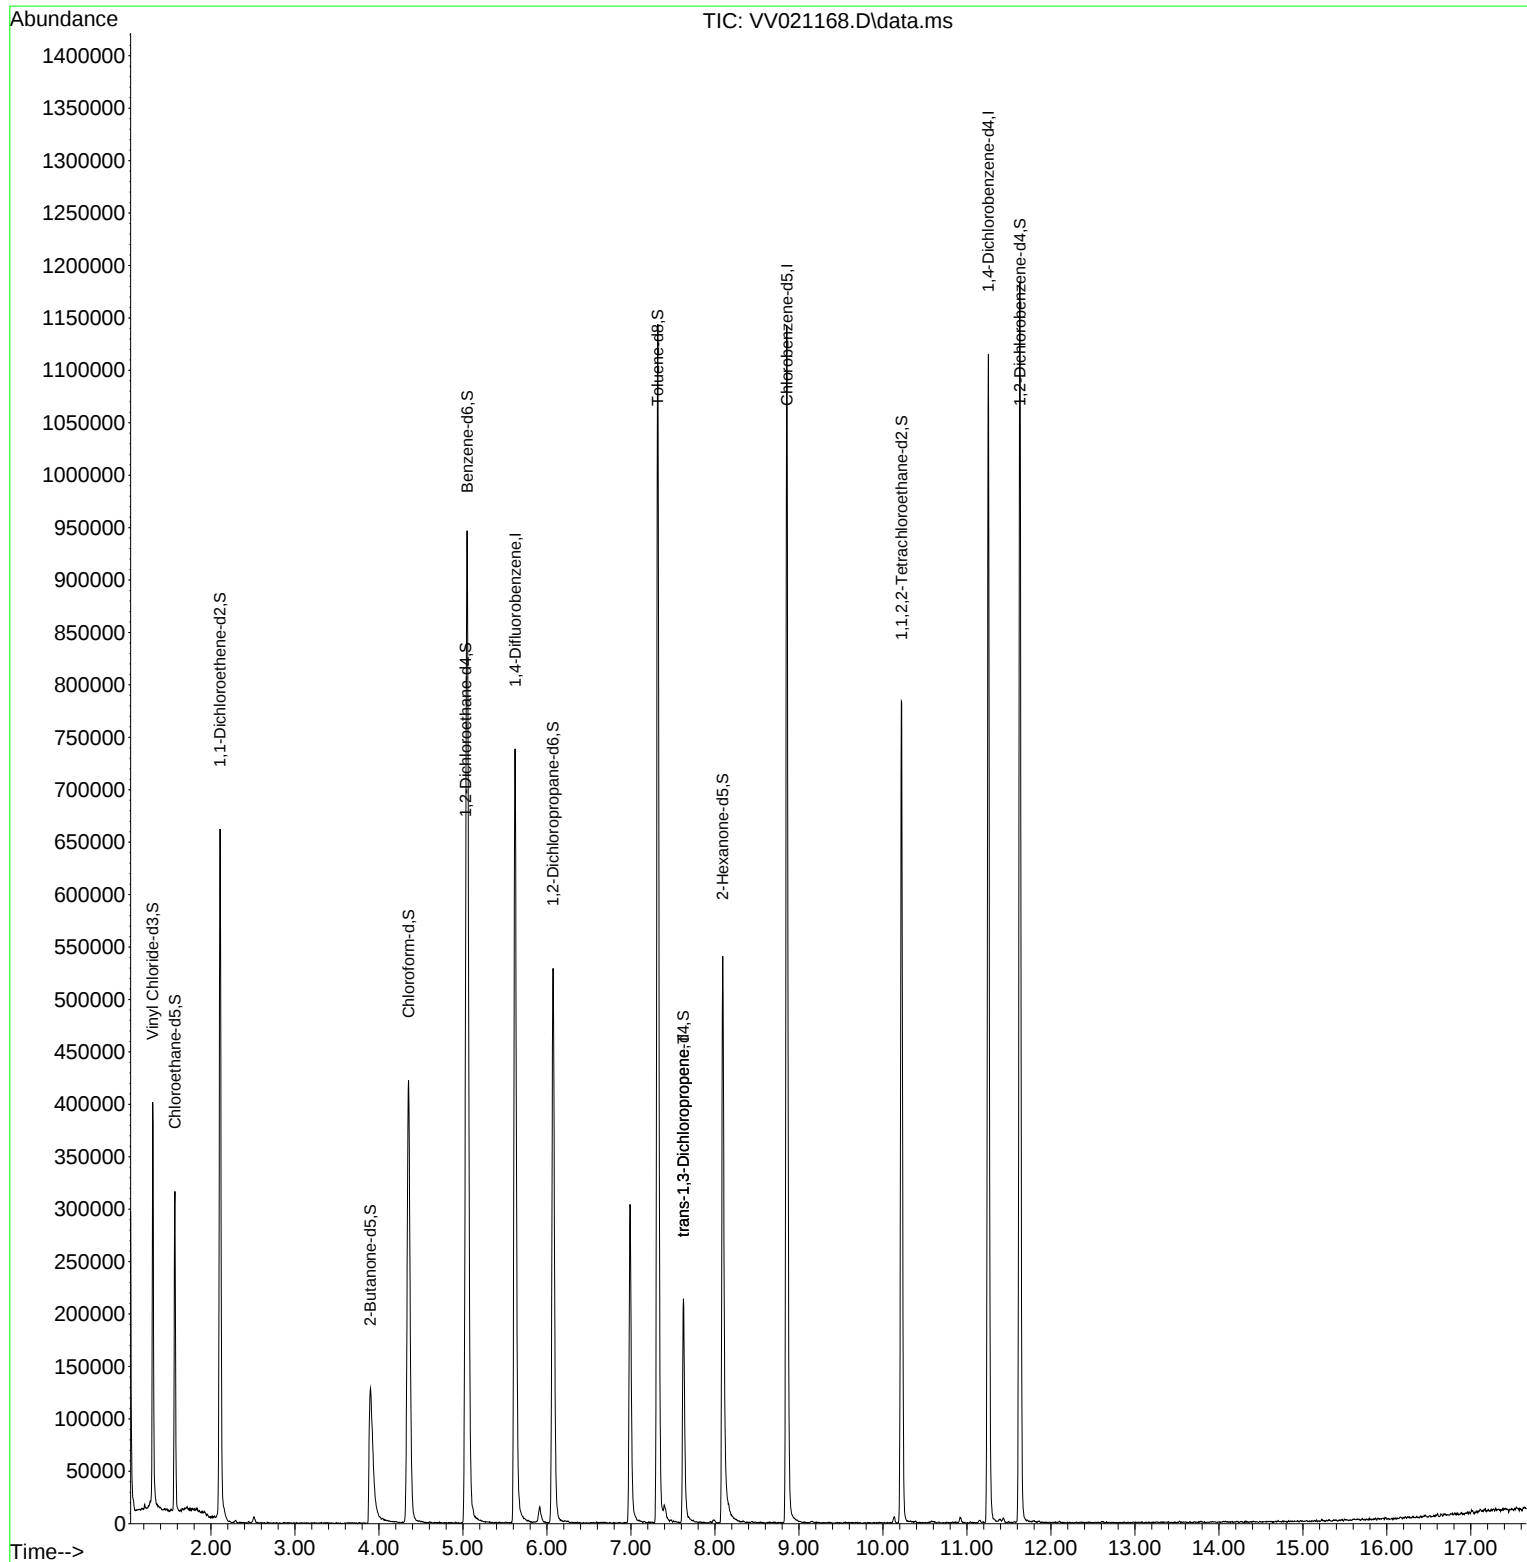

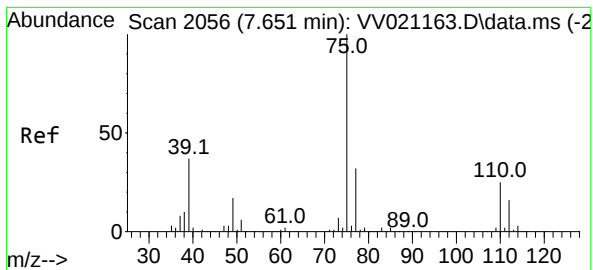

#44
 trans-1,3-Dichloropropene
 Concen: 0.78 ug/L
 RT: 7.625 min Scan# 2048
 Delta R.T. -0.026 min
 Lab File: VV021168.D
 Acq: 27 Apr 2021 12:18

Instrument :
 MSVOA_V
 ClientSampleId :

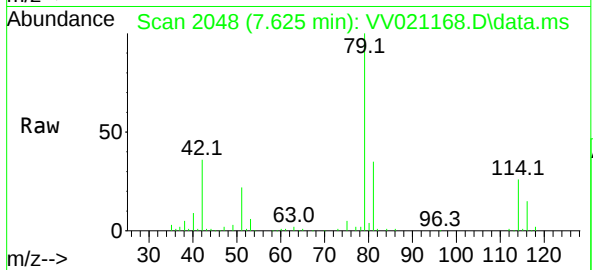

Tgt Ion: 75 Resp: 5719
 Ion Ratio Lower Upper
 75 100
 77 40.6 21.8 40.6#

