

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042721\
 Data File : VW021171.D
 Acq On : 27 Apr 2021 13:29
 Operator : SY/MD
 Sample : VIBLK172
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK172

Quant Time: Apr 28 03:29:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 28 03:28:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	610168	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	599014	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	268935	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	217676	43.42	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	86.84%	
7) Chloroethane-d5	1.571	69	170860	46.32	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	92.64%	
11) 1,1-Dichloroethene-d2	2.108	63	314627	34.02	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	68.04%	
21) 2-Butanone-d5	3.895	46	248192	101.37	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	101.37%	
24) Chloroform-d	4.352	84	418545	46.83	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	93.66%	
26) 1,2-Dichloroethane-d4	5.034	65	298060	52.46	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	104.92%	
32) Benzene-d6	5.053	84	773619	48.49	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.98%	
36) 1,2-Dichloropropane-d6	6.072	67	237934	49.97	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	99.94%	
41) Toluene-d8	7.320	98	724655	46.93	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	93.86%	
43) trans-1,3-Dichloroprop...	7.625	79	124062	47.67	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	95.34%	
47) 2-Hexanone-d5	8.091	63	192860	102.11	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	102.11%	
56) 1,1,2,2-Tetrachloroeth...	10.223	84	337741	47.02	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	94.04%	
66) 1,2-Dichlorobenzene-d4	11.631	152	290428	54.67	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	109.34%	
Target Compounds						
46) Tetrachloroethene	7.985	164	11129	2.69	ug/L	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
Data File : VV021171.D
Acq On : 27 Apr 2021 13:29
Operator : SY/MD
Sample : VIBLK172
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK172

Quant Time: Apr 28 03:29:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 28 03:28:03 2021
Response via : Initial Calibration

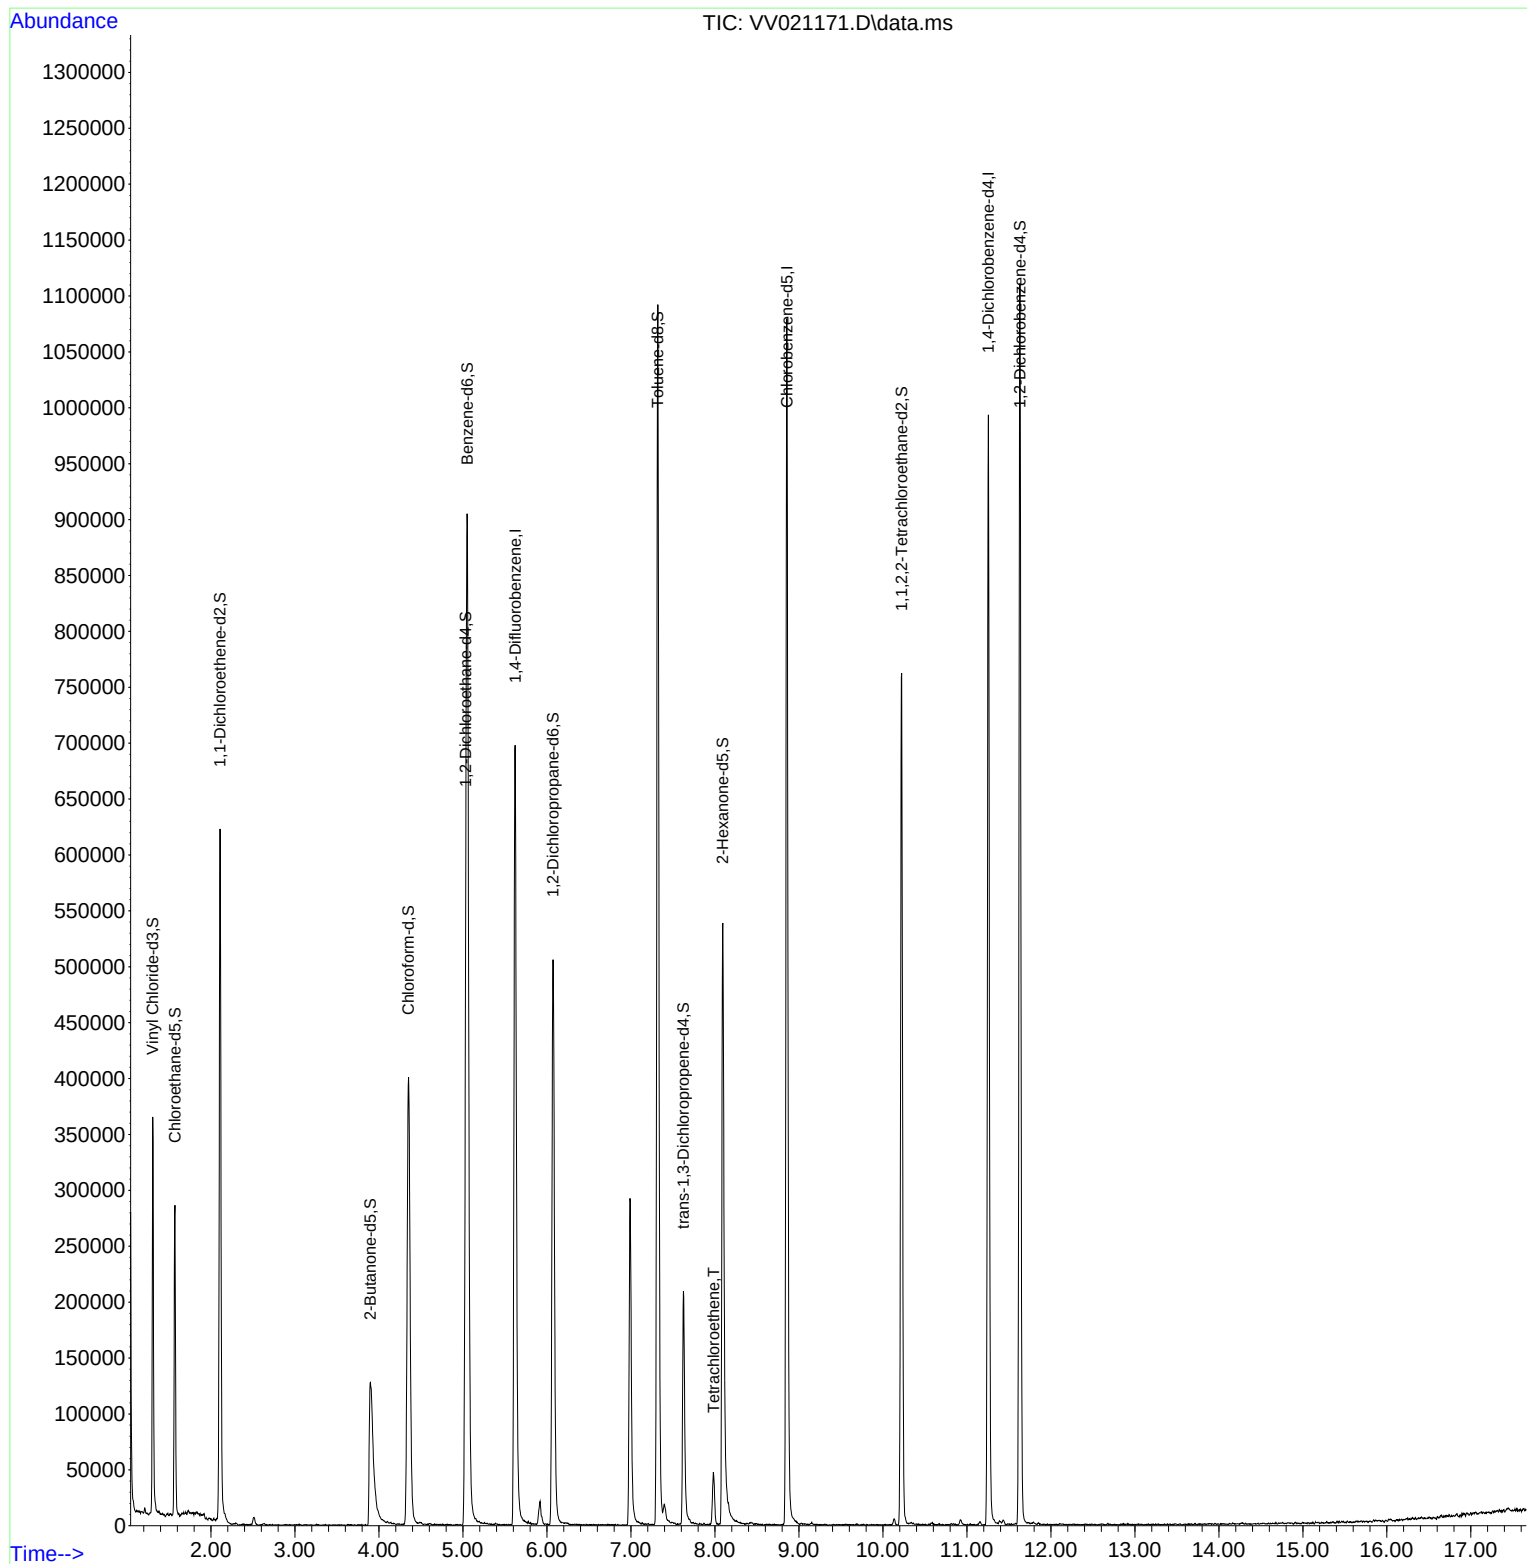

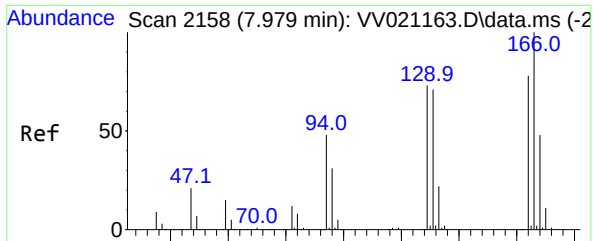

#46
Tetrachloroethene
Concen: 2.69 ug/L
RT: 7.985 min Scan# 2160
Delta R.T. 0.006 min
Lab File: VV021171.D
Acq: 27 Apr 2021 13:29

Instrument :
MSVOA_V
ClientSampleId :
VIBLK172

Tgt Ion:164 Resp: 11129

Ion	Ratio	Lower	Upper
164	100		
129	80.8	63.8	118.4
131	76.4	59.3	110.1
166	112.6	87.7	162.9

