

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042721\
 Data File : VW021180.D
 Acq On : 27 Apr 2021 17:51
 Operator : SY/MD
 Sample : M2165-01ME 10X
 Misc : 5.22g/5.0mL/100uL/5.3mL/MSVOA_V/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB3E4ME

Quant Time: Apr 28 03:31:39 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 28 03:28:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	514174	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	512712	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	245643	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	284967	67.45	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 134.90%			
7) Chloroethane-d5	1.571	69	222396	71.55	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 143.10%#			
11) 1,1-Dichloroethene-d2	2.108	63	425972	54.66	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 109.32%			
21) 2-Butanone-d5	3.905	46	331726	160.79	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 160.79%#			
24) Chloroform-d	4.352	84	556024	73.82	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 147.64%#			
26) 1,2-Dichloroethane-d4	5.034	65	387055	80.84	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 161.68%#			
32) Benzene-d6	5.053	84	1021614	74.82	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 149.64%#			
36) 1,2-Dichloropropane-d6	6.072	67	312551	76.68	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 153.36%#			
41) Toluene-d8	7.320	98	982679	74.36	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 148.72%#			
43) trans-1,3-Dichloroprop...	7.625	79	162626	73.01	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 146.02%#			
47) 2-Hexanone-d5	8.095	63	256647	158.76	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 158.76%#			
56) 1,1,2,2-Tetrachloroeth...	10.220	84	435447	70.83	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 141.66%#			
66) 1,2-Dichlorobenzene-d4	11.632	152	393561	81.11	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 162.22%#			
Target Compounds						Qvalue
46) Tetrachloroethene	7.979	164	97355	27.52	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
Data File : VV021180.D
Acq On : 27 Apr 2021 17:51
Operator : SY/MD
Sample : M2165-01ME 10X
Misc : 5.22g/5.0mL/100uL/5.3mL/MSVOA_V/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB3E4ME

Quant Time: Apr 28 03:31:39 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 28 03:28:03 2021
Response via : Initial Calibration

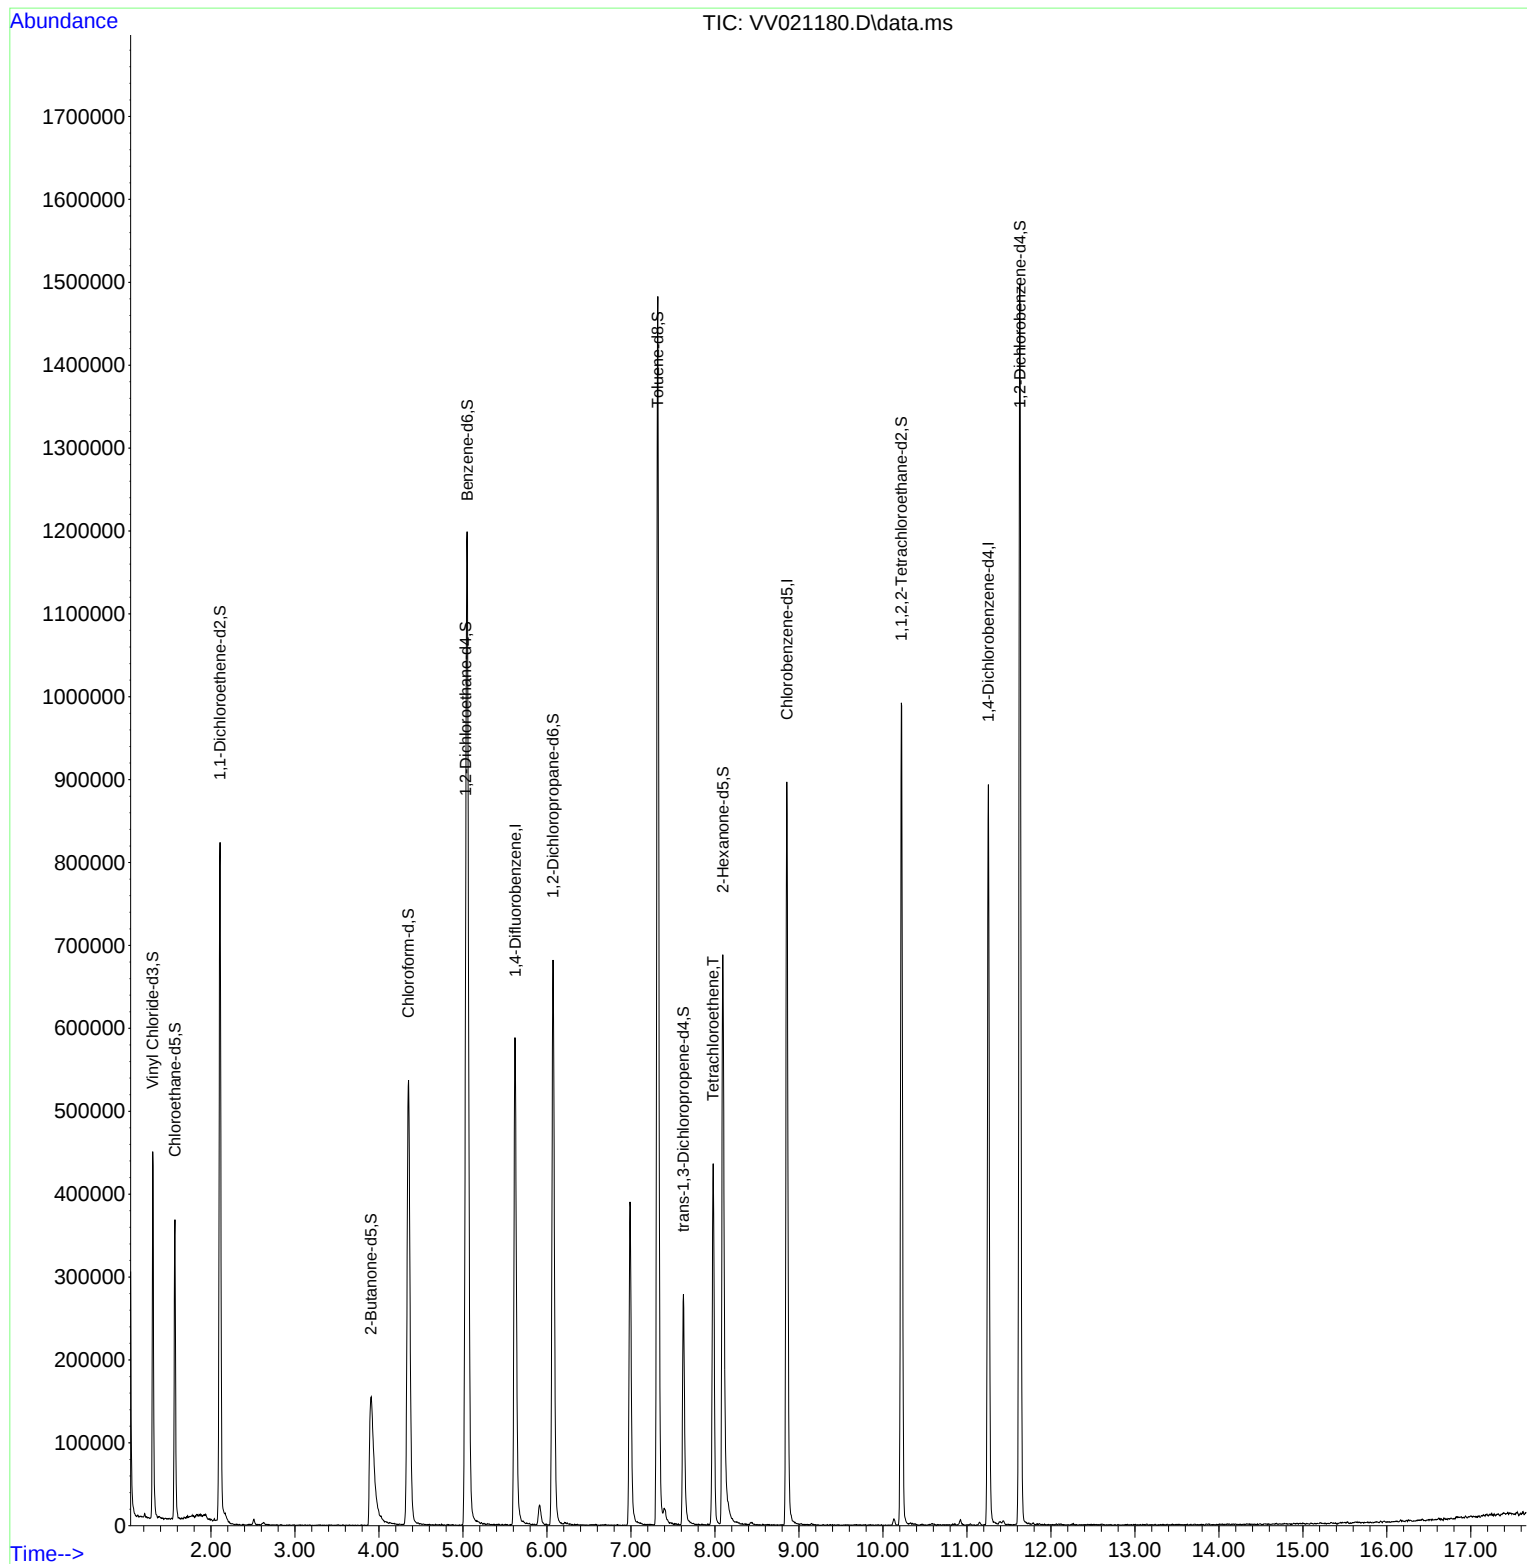

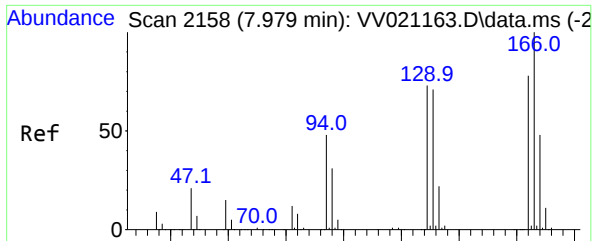

#46
 Tetrachloroethene
 Concen: 27.52 ug/L
 RT: 7.979 min Scan# 2158
 Delta R.T. 0.000 min
 Lab File: VV021180.D
 Acq: 27 Apr 2021 17:51

Instrument :
 MSVOA_V
 ClientSampleId :
 GB3E4ME

Tgt Ion:164 Resp: 97355

Ion	Ratio	Lower	Upper
164	100		
129	91.5	63.8	118.4
131	84.4	59.3	110.1
166	130.4	87.7	162.9

