

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042721\
 Data File : VW021185.D
 Acq On : 27 Apr 2021 19:48
 Operator : SY/MD
 Sample : M2165-04ME 40X
 Misc : 6.35g/5.0mL/100uL/5.8mL/MSVOA_V/MEOH
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB3E5ME

Quant Time: Apr 28 03:32:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 28 03:28:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	668735	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	659489	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	313093	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.311	65	207263	37.72	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	75.44%		
7) Chloroethane-d5	1.571	69	166050	41.08	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	82.16%		
11) 1,1-Dichloroethene-d2	2.111	63	309292	30.52	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	61.04%		
21) 2-Butanone-d5	3.902	46	243311	90.67	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	90.67%		
24) Chloroform-d	4.352	84	414130	42.27	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	84.54%		
26) 1,2-Dichloroethane-d4	5.037	65	287937	46.24	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.48%		
32) Benzene-d6	5.053	84	751407	42.78	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.56%		
36) 1,2-Dichloropropane-d6	6.072	67	224014	42.73	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	85.46%		
41) Toluene-d8	7.320	98	714769	42.05	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	84.10%		
43) trans-1,3-Dichloroprop...	7.625	79	119873	41.84	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.68%		
47) 2-Hexanone-d5	8.095	63	187801	90.32	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	90.32%		
56) 1,1,2,2-Tetrachloroeth...	10.220	84	325938	41.22	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	82.44%		
66) 1,2-Dichlorobenzene-d4	11.632	152	291440	47.12	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.24%		
Target Compounds						
					Qvalue	
46) Tetrachloroethene	7.979	164	361491	79.43	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
Data File : VV021185.D
Acq On : 27 Apr 2021 19:48
Operator : SY/MD
Sample : M2165-04ME 40X
Misc : 6.35g/5.0mL/100uL/5.8mL/MSVOA_V/MEOH
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB3E5ME

Quant Time: Apr 28 03:32:33 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 28 03:28:03 2021
Response via : Initial Calibration

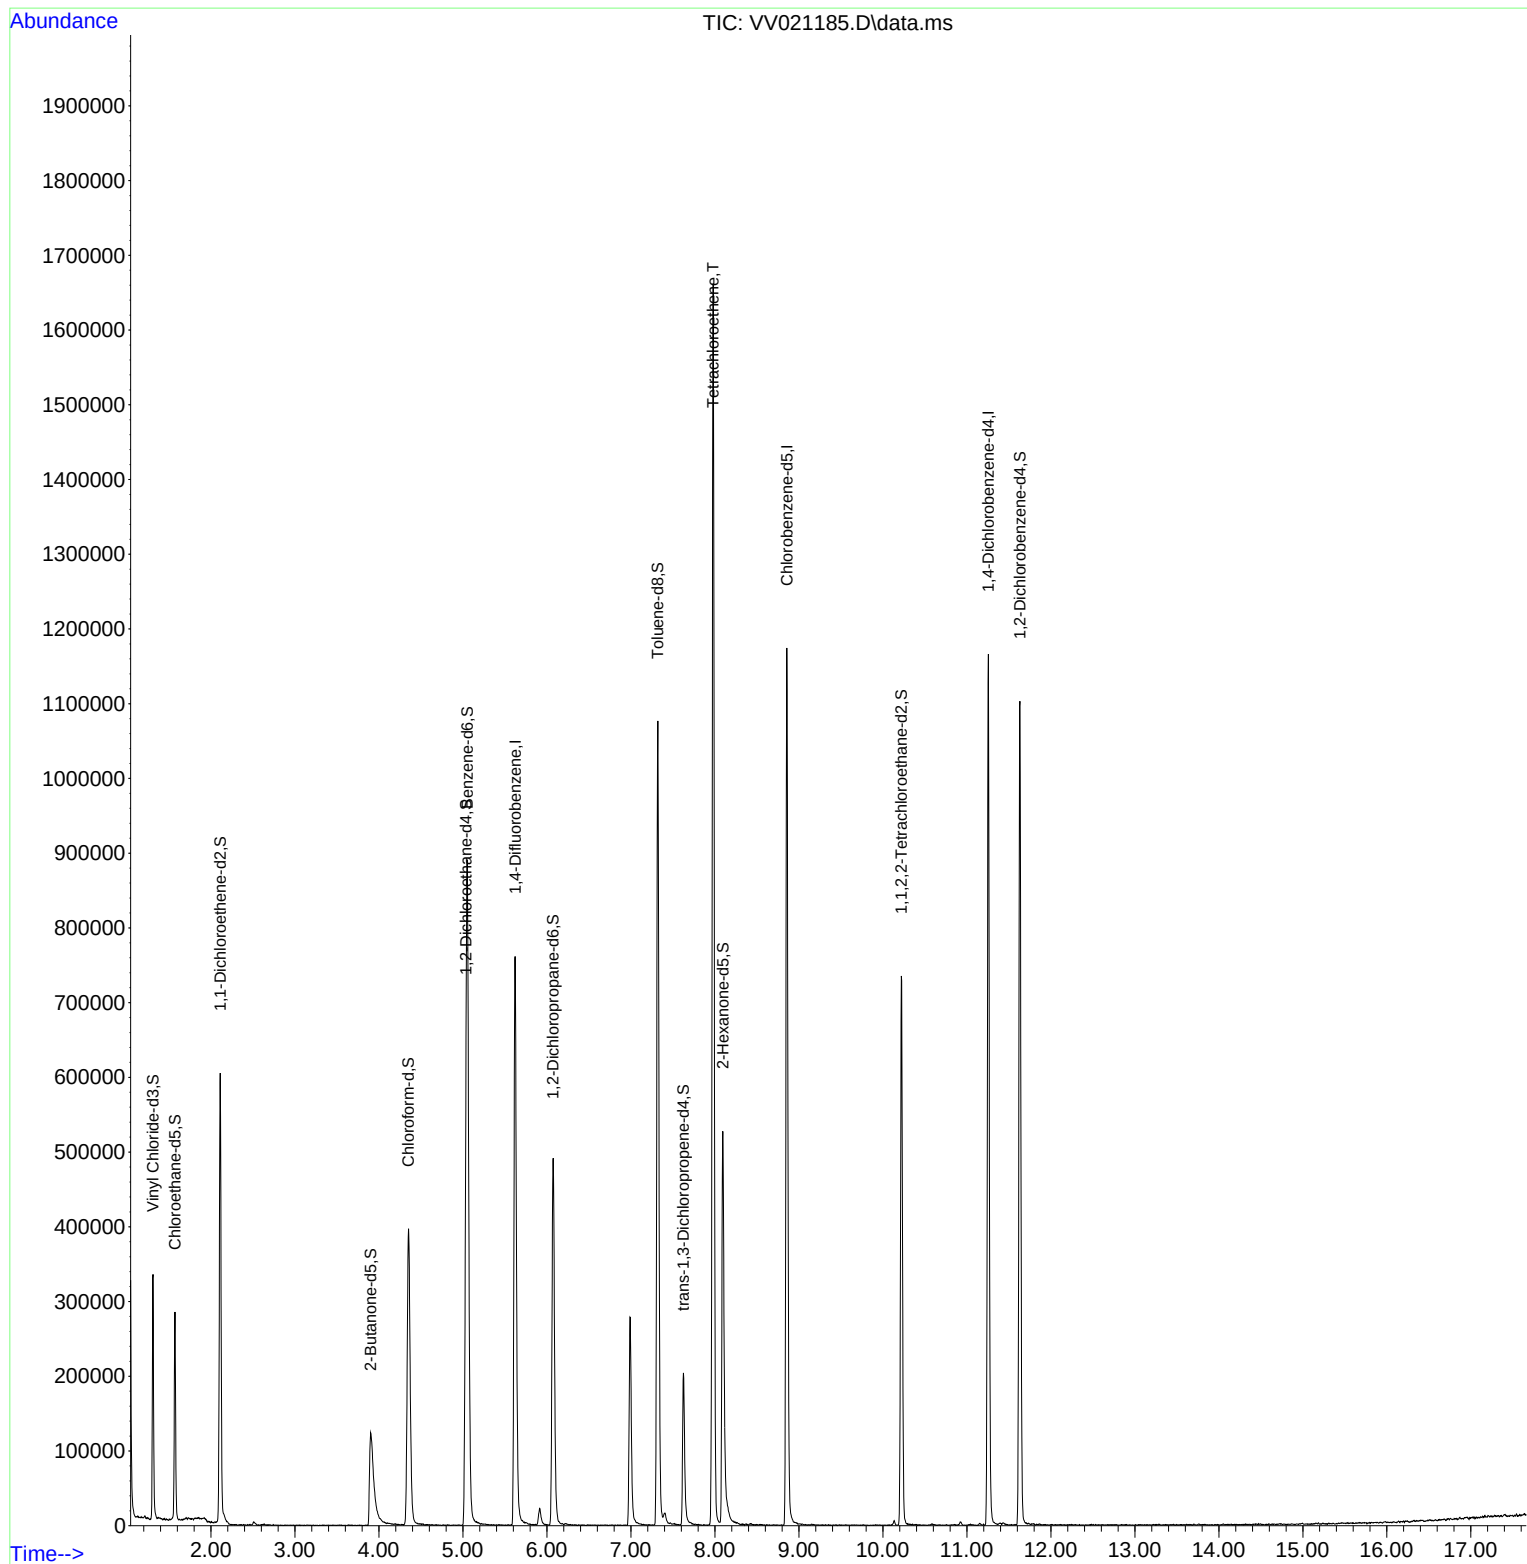

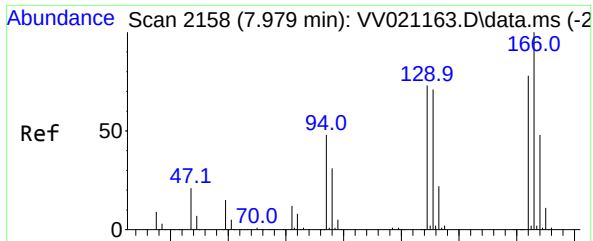

#46
 Tetrachloroethene
 Concen: 79.43 ug/L
 RT: 7.979 min Scan# 2158
 Delta R.T. 0.000 min
 Lab File: VV021185.D
 Acq: 27 Apr 2021 19:48

Instrument :
 MSVOA_V
 ClientSampleId :
 GB3E5ME

Tgt Ion:164 Resp: 361491

Ion	Ratio	Lower	Upper
164	100		
129	92.8	63.8	118.4
131	90.7	59.3	110.1
166	128.2	87.7	162.9

