

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042721\
 Data File : VW021187.D
 Acq On : 27 Apr 2021 20:35
 Operator : SY/MD
 Sample : M2165-05DL 400X
 Misc : 5.44g/5.0mL/100uL/5.10mL/MSVOA_V/MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB3E6DL

Quant Time: Apr 28 03:32:55 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 28 03:28:03 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	648377	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	628923	50.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.255	152	293988	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	205565	38.58	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 77.16%			
7) Chloroethane-d5	1.571	69	163109	41.62	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 83.24%			
11) 1,1-Dichloroethene-d2	2.108	63	305024	31.04	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 62.08%			
21) 2-Butanone-d5	3.908	46	234811	90.25	ug/L	0.01
Spiked Amount 100.000	Range 40 - 130		Recovery = 90.25%			
24) Chloroform-d	4.352	84	409557	43.12	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 86.24%			
26) 1,2-Dichloroethane-d4	5.037	65	283290	46.92	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 93.84%			
32) Benzene-d6	5.053	84	746163	44.55	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 89.10%			
36) 1,2-Dichloropropane-d6	6.072	67	224223	44.85	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 89.70%			
41) Toluene-d8	7.320	98	692786	42.74	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 85.48%			
43) trans-1,3-Dichloroprop...	7.625	79	114714	41.99	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 83.98%			
47) 2-Hexanone-d5	8.095	63	182406	91.99	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 91.99%			
56) 1,1,2,2-Tetrachloroeth...	10.220	84	319369	42.35	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 84.70%			
66) 1,2-Dichlorobenzene-d4	11.631	152	285485	49.16	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 98.32%			
Target Compounds						
46) Tetrachloroethene	7.979	164	135822	31.30	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
Data File : VV021187.D
Acq On : 27 Apr 2021 20:35
Operator : SY/MD
Sample : M2165-05DL 400X
Misc : 5.44g/5.0mL/100uL/5.10mL/MSVOA_V/MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB3E6DL

Quant Time: Apr 28 03:32:55 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 28 03:28:03 2021
Response via : Initial Calibration

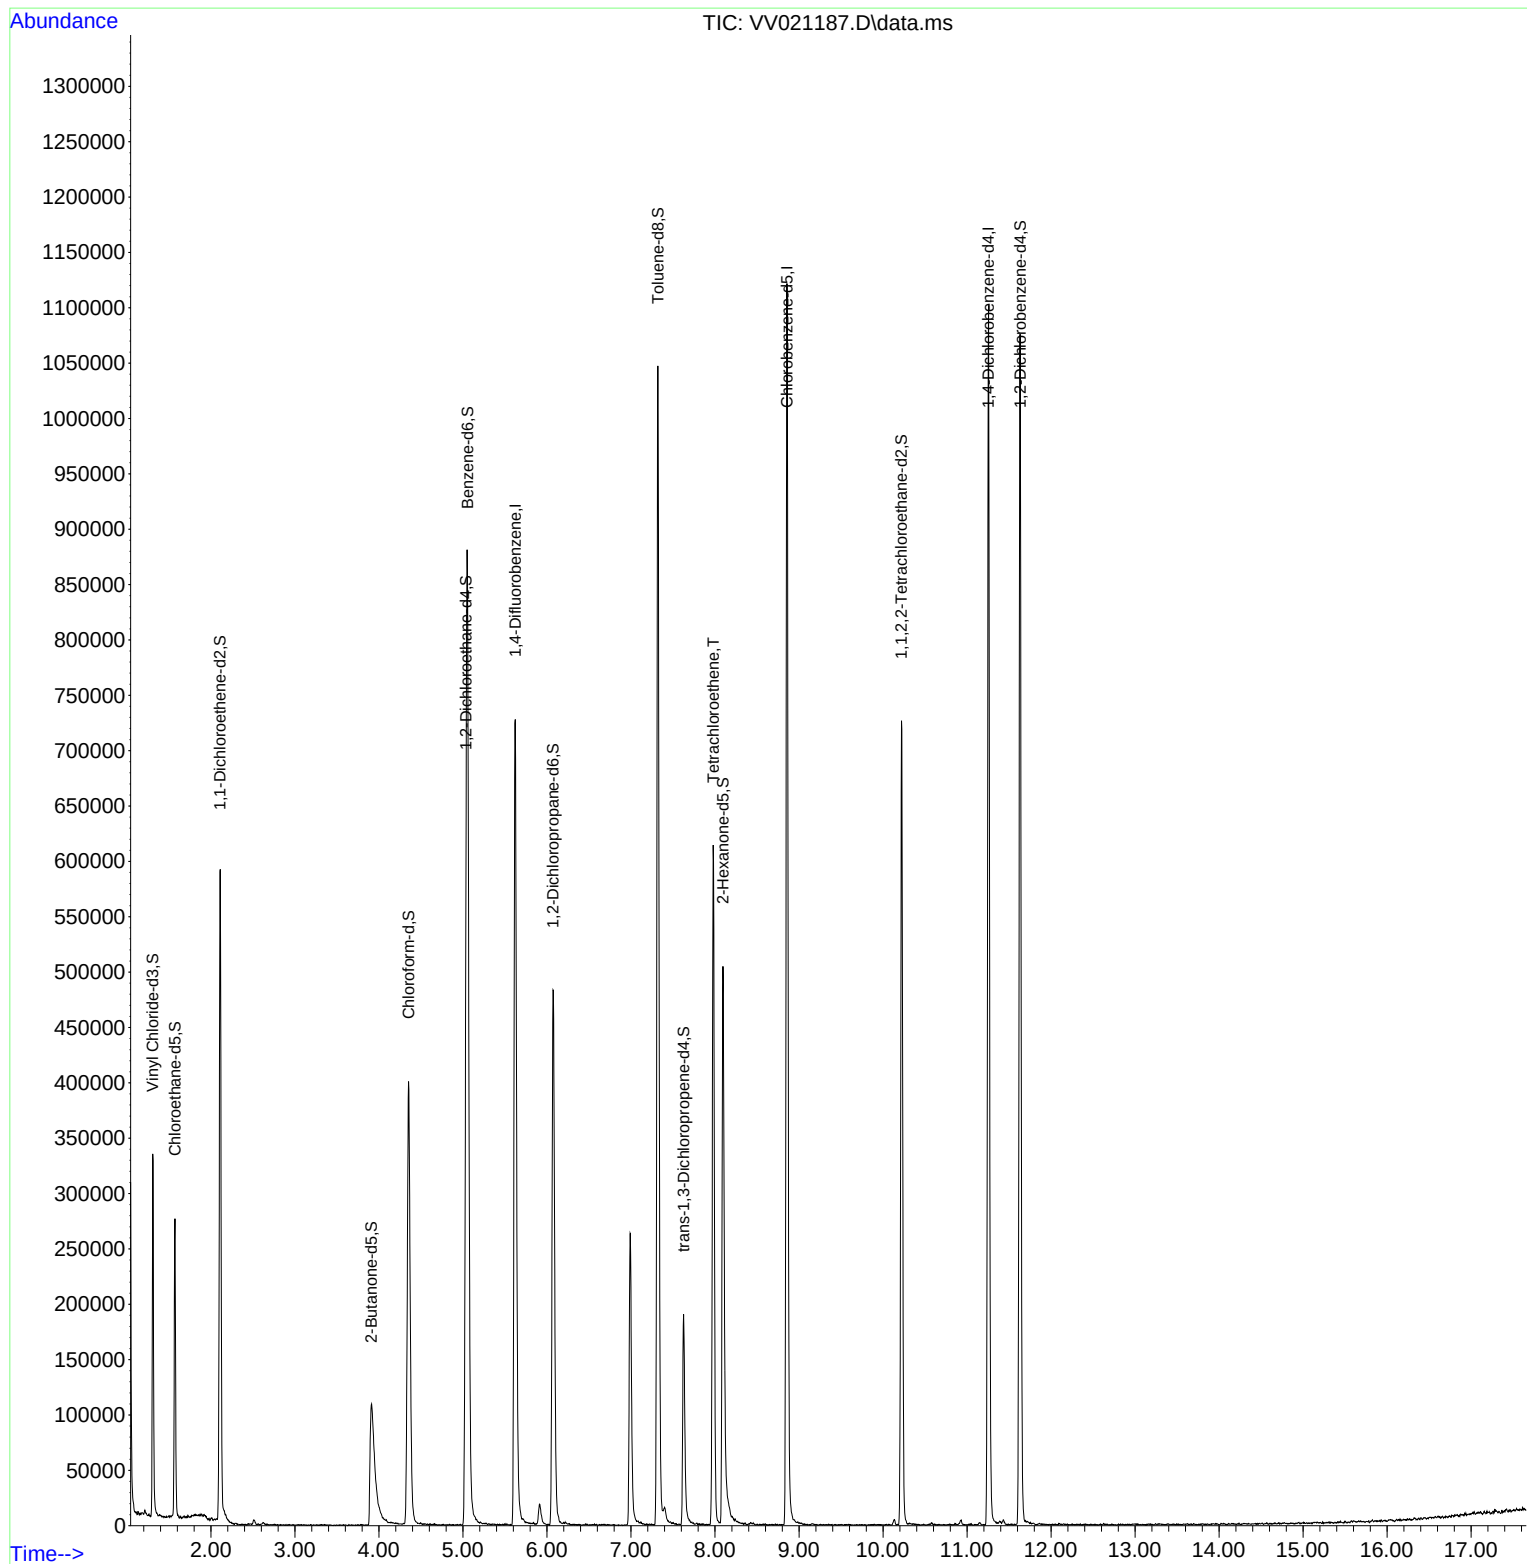

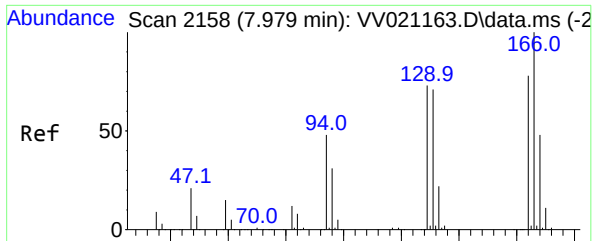

#46
 Tetrachloroethene
 Concen: 31.30 ug/L
 RT: 7.979 min Scan# 2158
 Delta R.T. -0.000 min
 Lab File: VV021187.D
 Acq: 27 Apr 2021 20:35

Instrument :
 MSVOA_V
 ClientSampleId :
 GB3E6DL

Tgt Ion:164 Resp: 135822

Ion	Ratio	Lower	Upper
164	100		
129	92.5	63.8	118.4
131	86.8	59.3	110.1
166	131.7	87.7	162.9

