

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
 Data File : VV021168.D
 Acq On : 27 Apr 2021 12:18
 Operator : SY/MD
 Sample : M2123-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

Signal : TIC: VV021168.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	78	83	97	rVB	383908	395104	16.32%	2.099%
2	1.571	158	165	180	rVB	304592	343096	14.17%	1.823%
3	2.108	323	332	365	rVB	660554	980739	40.51%	5.211%
4	2.326	398	400	402	rBV2	479	197	0.01%	0.001%
5	2.343	402	405	410	rVV2	833	632	0.03%	0.003%
6	2.449	434	438	446	rBV5	1378	1246	0.05%	0.007%
7	2.677	506	509	514	rVB4	1019	807	0.03%	0.004%
8	2.738	526	528	530	rBV	515	262	0.01%	0.001%
9	2.818	551	553	555	rVB2	529	227	0.01%	0.001%
10	2.851	558	563	564	rBV3	411	312	0.01%	0.002%
11	2.860	564	566	568	rBV2	553	317	0.01%	0.002%
12	3.018	613	615	617	rBB	511	165	0.01%	0.001%
13	3.053	622	626	629	rBV2	594	384	0.02%	0.002%
14	3.191	663	669	671	rBV2	775	716	0.03%	0.004%
15	3.349	714	718	719	rBV2	476	255	0.01%	0.001%
16	3.371	723	725	729	rBV2	640	470	0.02%	0.002%
17	3.494	757	763	767	rVB2	848	656	0.03%	0.003%
18	3.513	767	769	770	rBV2	531	223	0.01%	0.001%
19	3.561	782	784	785	rBV	254	131	0.01%	0.001%
20	3.609	797	799	801	rBV	317	173	0.01%	0.001%
21	3.687	821	823	826	rBV2	481	275	0.01%	0.001%
22	3.732	834	837	842	rVB2	887	663	0.03%	0.004%
23	3.757	842	845	847	rBV	874	657	0.03%	0.003%
24	3.796	853	857	859	rBV2	511	373	0.02%	0.002%
25	3.899	878	889	922	rBV	128835	426601	17.62%	2.267%
26	4.352	1015	1030	1062	rBV2	419991	1035618	42.78%	5.503%
27	4.722	1143	1145	1147	rBV	988	418	0.02%	0.002%
28	4.831	1177	1179	1182	rBV3	686	381	0.02%	0.002%
29	4.908	1200	1203	1204	rBV	1024	513	0.02%	0.003%
30	4.950	1214	1216	1218	rVB2	492	206	0.01%	0.001%
31	5.050	1230	1247	1276	rBV2	946122	2421001	100.00%	12.864%
32	5.577	1409	1411	1412	rBV2	833	354	0.01%	0.002%
33	5.622	1412	1425	1456	rVV2	737934	1497060	61.84%	7.955%
34	5.915	1508	1516	1531	rVB3	14492	28988	1.20%	0.154%
35	6.072	1552	1565	1588	rBV	527843	1074847	44.40%	5.711%
36	6.362	1652	1655	1659	rBV4	805	712	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
 Data File : VV021168.D
 Acq On : 27 Apr 2021 12:18
 Operator : SY/MD
 Sample : M2123-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	6.391	1662	1664	1666	rVV3	569	247	0.01%	0.001%
38	6.413	1669	1671	1674	rVB2	555	341	0.01%	0.002%
39	6.439	1674	1679	1683	rBV5	968	1006	0.04%	0.005%
40	6.590	1724	1726	1730	rBV2	1016	675	0.03%	0.004%
41	6.770	1780	1782	1785	rBV2	216	142	0.01%	0.001%
42	6.789	1786	1788	1791	rVV	551	244	0.01%	0.001%
43	6.821	1795	1798	1799	rBV	458	312	0.01%	0.002%
44	6.902	1820	1823	1825	rBV	452	262	0.01%	0.001%
45	6.915	1825	1827	1828	rBV	370	206	0.01%	0.001%
46	6.944	1834	1836	1838	rBV	657	363	0.01%	0.002%
47	6.989	1840	1850	1876	rVV	303501	544456	22.49%	2.893%
48	7.153	1897	1901	1902	rBV2	1341	1076	0.04%	0.006%
49	7.320	1940	1953	1973	rBV	1143510	1992416	82.30%	10.587%
50	7.587	2035	2036	2038	rBV	683	368	0.02%	0.002%
51	7.625	2038	2048	2067	rVV	213457	378022	15.61%	2.009%
52	7.860	2119	2121	2122	rBV2	981	361	0.01%	0.002%
53	7.979	2153	2158	2160	rBV3	2716	2312	0.10%	0.012%
54	8.046	2177	2179	2180	rBV	523	218	0.01%	0.001%
55	8.095	2183	2194	2214	rBV	539964	989602	40.88%	5.258%
56	8.542	2330	2333	2339	rBV4	1045	1102	0.05%	0.006%
57	8.715	2385	2387	2392	rVB3	1221	856	0.04%	0.005%
58	8.741	2392	2395	2397	rBV	661	445	0.02%	0.002%
59	8.857	2419	2431	2465	rBV	1141595	1844340	76.18%	9.800%
60	9.207	2539	2540	2543	rBV2	742	335	0.01%	0.002%
61	9.230	2545	2547	2548	rBV2	538	201	0.01%	0.001%
62	9.294	2565	2567	2570	rBV2	589	347	0.01%	0.002%
63	9.426	2606	2608	2609	rBV	351	125	0.01%	0.001%
64	9.490	2626	2628	2631	rBV2	501	330	0.01%	0.002%
65	9.596	2659	2661	2662	rBV2	571	323	0.01%	0.002%
66	9.622	2667	2669	2672	rBV3	592	471	0.02%	0.003%
67	9.776	2713	2717	2719	rBV	541	473	0.02%	0.003%
68	9.825	2728	2732	2736	rBV3	891	879	0.04%	0.005%
69	9.902	2754	2756	2760	rBV2	596	415	0.02%	0.002%
70	9.921	2760	2762	2764	rVB	599	236	0.01%	0.001%
71	10.017	2790	2792	2796	rVB2	634	254	0.01%	0.001%
72	10.050	2799	2802	2805	rBV	933	707	0.03%	0.004%
73	10.136	2821	2829	2836	rBV4	6051	8621	0.36%	0.046%
74	10.178	2839	2842	2843	rBV	423	260	0.01%	0.001%
75	10.220	2843	2855	2876	rBV	783609	1242308	51.31%	6.601%
76	10.709	3004	3007	3009	rBV2	411	260	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
 Data File : VV021168.D
 Acq On : 27 Apr 2021 12:18
 Operator : SY/MD
 Sample : M2123-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

77	10.828	3040	3044	3049	rBV5	1438	1545	0.06%	0.008%
78	11.005	3095	3099	3104	rBV3	723	716	0.03%	0.004%
79	11.043	3104	3111	3117	rBV5	1274	1678	0.07%	0.009%
80	11.088	3123	3125	3129	rVB2	669	527	0.02%	0.003%
81	11.152	3137	3145	3151	rBV7	2558	4397	0.18%	0.023%
82	11.255	3165	3177	3195	rBV	1114449	1722067	71.13%	9.150%
83	11.632	3282	3294	3316	rBV	1182549	1854597	76.60%	9.855%
84	12.085	3433	3435	3438	rBV3	831	604	0.02%	0.003%
85	12.143	3450	3453	3456	rVB3	986	598	0.02%	0.003%
86	12.831	3665	3667	3668	rBV3	524	180	0.01%	0.001%
87	12.876	3675	3681	3686	rBV4	967	1178	0.05%	0.006%
88	12.940	3699	3701	3705	rVB2	569	348	0.01%	0.002%
89	14.329	4131	4133	4135	rBV	1258	638	0.03%	0.003%




Sum of corrected areas: 18819769

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
Data File : VV021168.D
Acq On : 27 Apr 2021 12:18
Operator : SY/MD
Sample : M2123-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

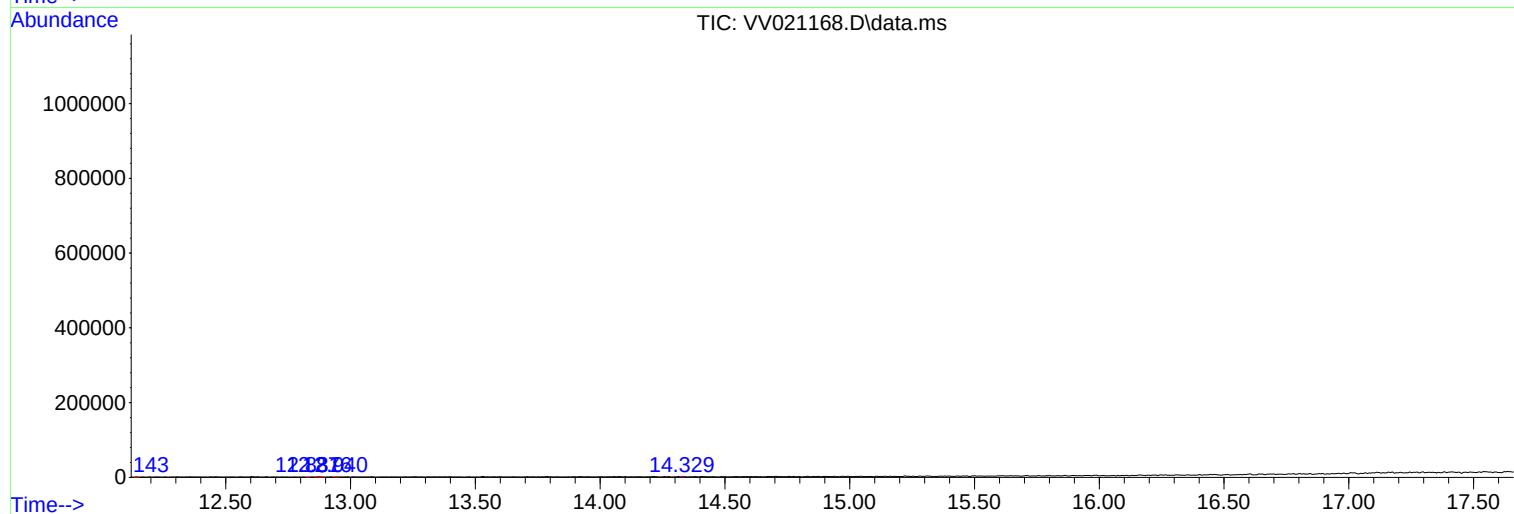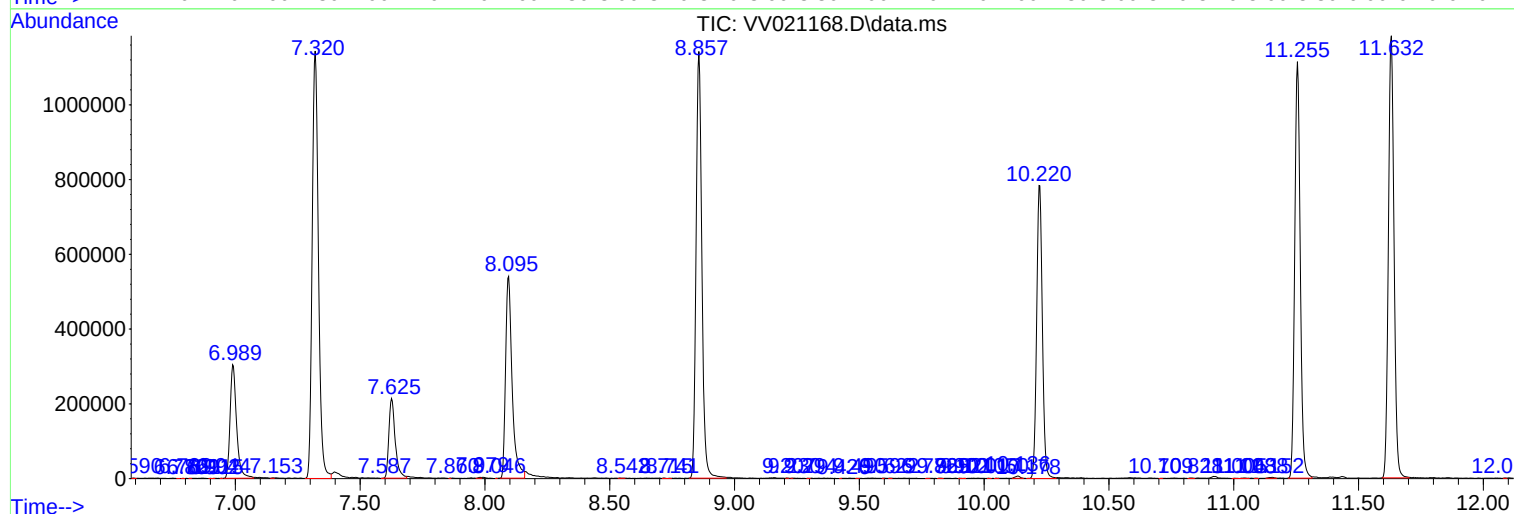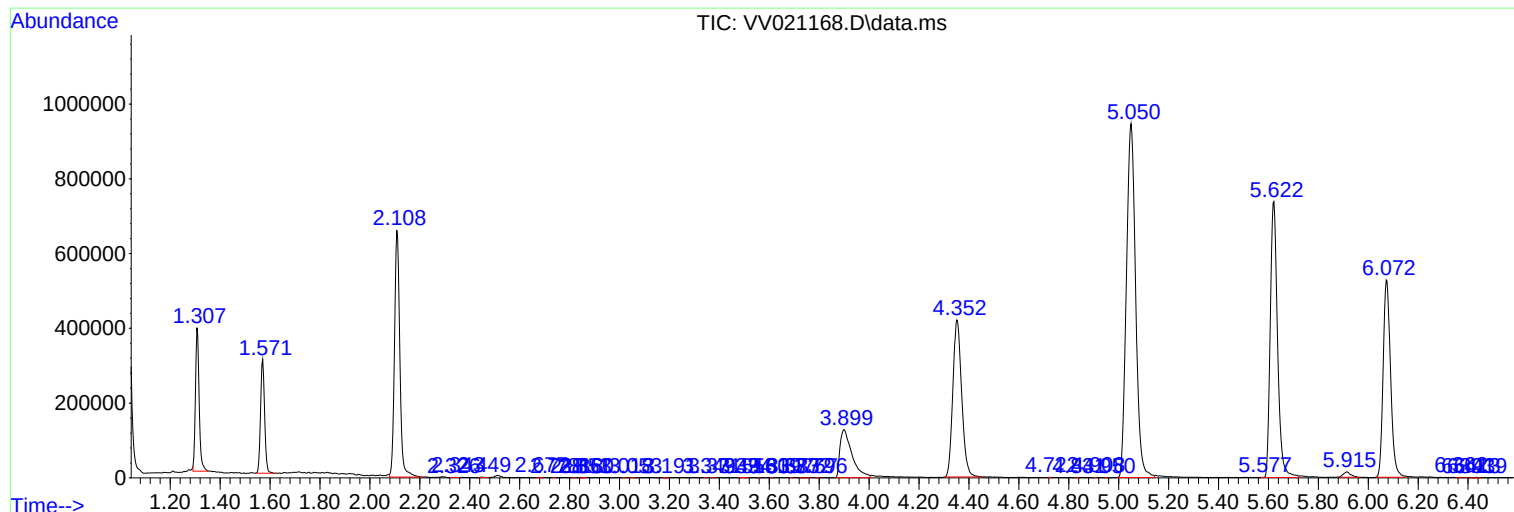

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
Data File : VV021168.D
Acq On : 27 Apr 2021 12:18
Operator : SY/MD
Sample : M2123-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
Data File : VV021168.D
Acq On : 27 Apr 2021 12:18
Operator : SY/MD
Sample : M2123-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
