

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
 Data File : VV021169.D
 Acq On : 27 Apr 2021 12:42
 Operator : SY/MD
 Sample : M2326-01 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

Signal : TIC: VV021169.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	100	rVB	395557	404611	0.98%	0.642%
2	1.571	158	165	176	rVB	296049	334575	0.81%	0.531%
3	2.108	323	332	361	rVB	654721	977067	2.36%	1.550%
4	2.346	403	406	409	rBV3	993	788	0.00%	0.001%
5	2.375	413	415	416	rBV3	625	240	0.00%	0.000%
6	2.513	450	458	470	rVB3	5236	9330	0.02%	0.015%
7	2.577	475	478	480	rVV3	606	302	0.00%	0.000%
8	2.603	483	486	490	rVB4	793	595	0.00%	0.001%
9	2.635	490	496	503	rBV4	1107	1694	0.00%	0.003%
10	2.690	512	513	515	rBV	521	140	0.00%	0.000%
11	2.703	515	517	520	rVB2	404	154	0.00%	0.000%
12	2.716	520	521	522	rBV2	256	61	0.00%	0.000%
13	2.741	526	529	530	rBV2	555	333	0.00%	0.001%
14	2.822	552	554	556	rVB	786	273	0.00%	0.000%
15	2.870	567	569	571	rVB	714	321	0.00%	0.001%
16	2.889	573	575	577	rBV	282	160	0.00%	0.000%
17	2.915	581	583	587	rVB2	468	354	0.00%	0.001%
18	2.934	587	589	593	rVB	738	416	0.00%	0.001%
19	2.953	593	595	596	rBV	342	162	0.00%	0.000%
20	2.966	596	599	602	rBV2	307	168	0.00%	0.000%
21	2.982	602	604	606	rBV2	349	174	0.00%	0.000%
22	3.034	614	620	624	rBV5	954	1245	0.00%	0.002%
23	3.150	654	656	659	rVB	677	408	0.00%	0.001%
24	3.169	661	662	666	rVB2	502	236	0.00%	0.000%
25	3.198	666	671	673	rBV2	642	536	0.00%	0.001%
26	3.224	676	679	680	rBV2	224	107	0.00%	0.000%
27	3.243	683	685	688	rBV	417	151	0.00%	0.000%
28	3.288	695	699	702	rBV3	947	891	0.00%	0.001%
29	3.400	732	734	737	rBV2	332	172	0.00%	0.000%
30	3.423	737	741	744	rVV2	667	474	0.00%	0.001%
31	3.494	761	763	766	rBV	334	113	0.00%	0.000%
32	3.577	786	789	791	rBV3	599	369	0.00%	0.001%
33	3.590	791	793	797	rVV3	423	281	0.00%	0.000%
34	3.674	818	819	822	rVB2	517	236	0.00%	0.000%
35	3.789	853	855	856	rBV2	301	87	0.00%	0.000%
36	3.912	878	893	920	rBV4	233753	738082	1.78%	1.171%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042721\
 Data File : VW021169.D
 Acq On : 27 Apr 2021 12:42
 Operator : SY/MD
 Sample : M2326-01 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	4.352	1015	1030	1063	rBV	421727	1036560	2.50%	1.644%
38	4.677	1127	1131	1136	rBV4	1130	1369	0.00%	0.002%
39	4.780	1161	1163	1166	rVB	370	204	0.00%	0.000%
40	4.802	1166	1170	1173	rBV3	680	473	0.00%	0.001%
41	4.831	1176	1179	1184	rBV3	732	655	0.00%	0.001%
42	4.899	1195	1200	1203	rBV3	633	649	0.00%	0.001%
43	4.924	1206	1208	1211	rVB2	733	353	0.00%	0.001%
44	4.963	1218	1220	1223	rBV	369	265	0.00%	0.000%
45	4.979	1223	1225	1227	rBV	379	191	0.00%	0.000%
46	5.050	1230	1247	1281	rVV3	942163	2421371	5.84%	3.841%
47	5.394	1352	1354	1357	rVB2	901	377	0.00%	0.001%
48	5.413	1357	1360	1363	rBV3	1071	741	0.00%	0.001%
49	5.452	1368	1372	1376	rBV3	1174	862	0.00%	0.001%
50	5.503	1384	1388	1391	rBV3	1137	977	0.00%	0.002%
51	5.619	1412	1424	1453	rBV2	751783	1527951	3.68%	2.424%
52	5.918	1502	1517	1550	rBV	1072128	2123348	5.12%	3.368%
53	6.072	1553	1565	1593	rVB	531872	1072938	2.59%	1.702%
54	6.294	1633	1634	1637	rBV2	950	332	0.00%	0.001%
55	6.371	1656	1658	1659	rBV	550	231	0.00%	0.000%
56	6.426	1672	1675	1679	rBV2	860	578	0.00%	0.001%
57	6.461	1683	1686	1688	rBV2	576	291	0.00%	0.000%
58	6.722	1765	1767	1768	rBV2	705	270	0.00%	0.000%
59	6.764	1777	1780	1784	rBV	560	484	0.00%	0.001%
60	6.789	1787	1788	1789	rBV	469	121	0.00%	0.000%
61	6.989	1840	1850	1873	rBV	298269	547175	1.32%	0.868%
62	7.320	1941	1953	1972	rBV	1166290	2005210	4.83%	3.181%
63	7.625	2038	2048	2073	rBV	217894	380113	0.92%	0.603%
64	7.860	2119	2121	2124	rBV	843	699	0.00%	0.001%
65	7.905	2133	2135	2137	rVB3	808	286	0.00%	0.000%
66	7.982	2142	2159	2184	rBV	25152373	41479296	100.00%	65.802%
67	8.091	2185	2193	2225	rVB	582951	1061114	2.56%	1.683%
68	8.667	2370	2372	2376	rVB5	784	507	0.00%	0.001%
69	8.857	2419	2431	2465	rBV	1180884	1903532	4.59%	3.020%
70	9.082	2498	2501	2504	rBV2	1528	1054	0.00%	0.002%
71	9.098	2504	2506	2509	rBV3	584	351	0.00%	0.001%
72	9.362	2586	2588	2589	rBV	698	303	0.00%	0.000%
73	9.493	2626	2629	2631	rVB2	588	252	0.00%	0.000%
74	9.509	2631	2634	2635	rBV	524	307	0.00%	0.000%
75	9.535	2639	2642	2644	rBV3	873	416	0.00%	0.001%
76	9.603	2661	2663	2665	rBV2	1057	543	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
 Data File : VV021169.D
 Acq On : 27 Apr 2021 12:42
 Operator : SY/MD
 Sample : M2326-01 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	9.667	2681	2683	2684	rBV	669	303	0.00%	0.000%
78	9.834	2731	2735	2738	rBV2	615	716	0.00%	0.001%
79	9.886	2749	2751	2755	rBV	538	394	0.00%	0.001%
80	9.940	2765	2768	2770	rVB3	942	512	0.00%	0.001%
81	9.972	2776	2778	2780	rBV2	425	242	0.00%	0.000%
82	10.130	2820	2827	2834	rBV6	4928	7137	0.02%	0.011%
83	10.220	2843	2855	2875	rBV	784967	1227965	2.96%	1.948%
84	10.513	2944	2946	2948	rBV	504	295	0.00%	0.000%
85	10.525	2948	2950	2953	rVV2	991	623	0.00%	0.001%
86	10.612	2975	2977	2982	rVB3	1020	610	0.00%	0.001%
87	10.651	2987	2989	2991	rBV	745	421	0.00%	0.001%
88	10.741	3014	3017	3018	rBV	719	453	0.00%	0.001%
89	10.779	3027	3029	3031	rBV3	799	418	0.00%	0.001%
90	10.927	3067	3075	3084	rBV3	4902	7562	0.02%	0.012%
91	10.972	3087	3089	3093	rBV2	343	322	0.00%	0.001%
92	11.046	3109	3112	3116	rBV4	1325	1250	0.00%	0.002%
93	11.091	3124	3126	3127	rBV2	482	155	0.00%	0.000%
94	11.255	3165	3177	3199	rBV	1193201	1829272	4.41%	2.902%
95	11.632	3281	3294	3317	rBV	1208159	1906917	4.60%	3.025%
96	12.693	3619	3624	3625	rBV2	500	383	0.00%	0.001%
97	12.844	3667	3671	3674	rBV5	624	514	0.00%	0.001%
98	13.866	3985	3989	3992	rBV	825	876	0.00%	0.001%
99	13.979	4021	4024	4027	rBV3	894	591	0.00%	0.001%
100	14.265	4110	4113	4115	rBV3	1192	742	0.00%	0.001%


Sum of corrected areas: 63036728

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
Data File : VV021169.D
Acq On : 27 Apr 2021 12:42
Operator : SY/MD
Sample : M2326-01 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

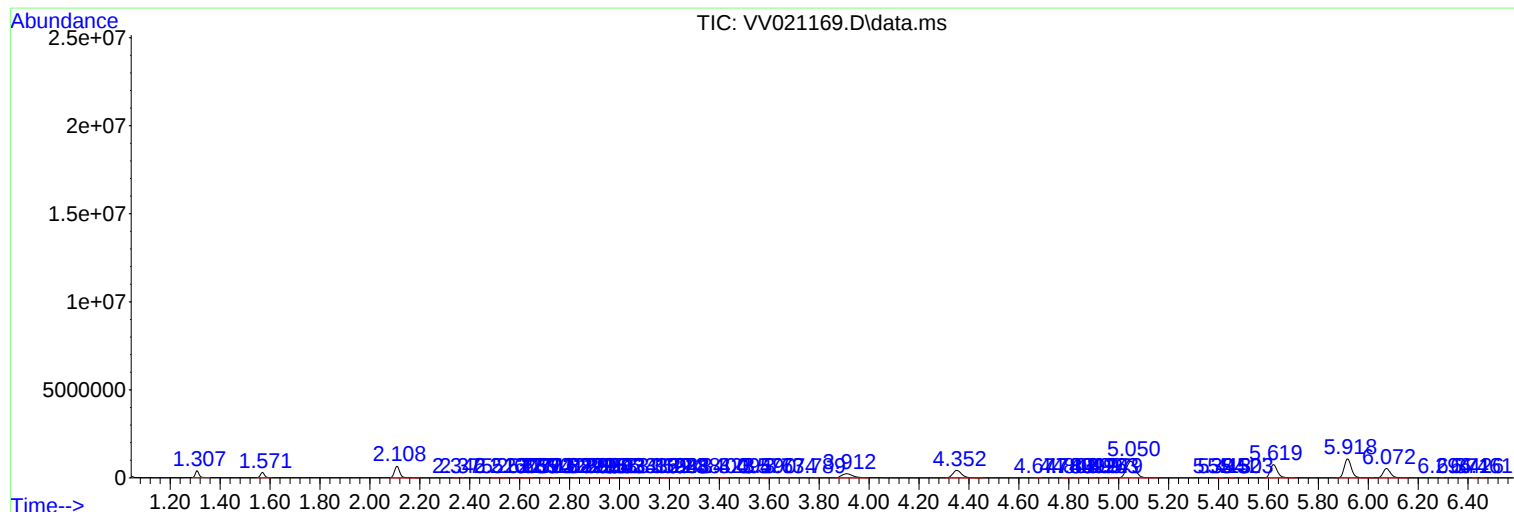

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
Data File : VV021169.D
Acq On : 27 Apr 2021 12:42
Operator : SY/MD
Sample : M2326-01 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
Data File : VV021169.D
Acq On : 27 Apr 2021 12:42
Operator : SY/MD
Sample : M2326-01 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
