

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
 Data File : VV021170.D
 Acq On : 27 Apr 2021 13:05
 Operator : SY/MD
 Sample : M2326-02 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

Signal : TIC: VV021170.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	96	rVB2	433077	453740	1.22%	0.756%
2	1.568	157	164	177	rVB	285845	323057	0.87%	0.538%
3	2.108	322	332	359	rVB	654561	963901	2.59%	1.606%
4	2.355	407	409	412	rBV2	711	347	0.00%	0.001%
5	2.510	452	457	467	rVB4	5801	9056	0.02%	0.015%
6	2.619	485	491	495	rBV3	1382	1925	0.01%	0.003%
7	2.664	503	505	506	rBV	677	164	0.00%	0.000%
8	2.760	531	535	547	rVB7	3652	6535	0.02%	0.011%
9	2.873	568	570	571	rBV7	554	300	0.00%	0.000%
10	2.941	586	591	594	rBV2	891	772	0.00%	0.001%
11	2.979	599	603	606	rBV3	505	442	0.00%	0.001%
12	3.101	638	641	644	rVB2	721	434	0.00%	0.001%
13	3.121	644	647	650	rBV2	897	553	0.00%	0.001%
14	3.137	650	652	655	rBV2	479	312	0.00%	0.001%
15	3.233	679	682	683	rBV2	455	239	0.00%	0.000%
16	3.252	686	688	690	rBV	602	325	0.00%	0.001%
17	3.387	727	730	732	rBV4	709	436	0.00%	0.001%
18	3.423	738	741	744	rBV2	425	376	0.00%	0.001%
19	3.436	744	745	748	rVB2	593	291	0.00%	0.000%
20	3.503	763	766	768	rBV2	432	283	0.00%	0.000%
21	3.516	768	770	773	rVV	373	200	0.00%	0.000%
22	3.532	773	775	779	rVB	642	326	0.00%	0.001%
23	3.564	781	785	788	rBV2	655	472	0.00%	0.001%
24	3.584	788	791	792	rBV	398	237	0.00%	0.000%
25	3.629	802	805	806	rBV2	482	214	0.00%	0.000%
26	3.661	813	815	818	rBV	442	329	0.00%	0.001%
27	3.677	818	820	825	rVB2	428	268	0.00%	0.000%
28	3.735	834	838	841	rBV2	338	313	0.00%	0.001%
29	3.767	845	848	853	rVB4	1104	841	0.00%	0.001%
30	3.793	853	856	857	rBV2	439	281	0.00%	0.000%
31	3.850	870	874	876	rVB2	589	349	0.00%	0.001%
32	3.912	877	893	928	rBV2	796901	2134504	5.73%	3.556%
33	4.352	1015	1030	1054	rBV	410732	1012619	2.72%	1.687%
34	4.799	1167	1169	1179	rVB8	979	1301	0.00%	0.002%
35	4.841	1179	1182	1189	rBV2	1028	763	0.00%	0.001%
36	4.876	1191	1193	1197	rBV3	903	612	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
 Data File : VV021170.D
 Acq On : 27 Apr 2021 13:05
 Operator : SY/MD
 Sample : M2326-02 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	5.050	1229	1247	1275	rBV2	923619	2370688	6.37%	3.950%
38	5.355	1339	1342	1346	rBV4	1582	1121	0.00%	0.002%
39	5.510	1387	1390	1391	rBV2	988	567	0.00%	0.001%
40	5.619	1412	1424	1454	rBV	729349	1497017	4.02%	2.494%
41	5.918	1503	1517	1544	rBV	1133830	2228090	5.98%	3.712%
42	6.072	1553	1565	1585	rBV	521079	1041760	2.80%	1.736%
43	6.339	1645	1648	1650	rBV3	635	447	0.00%	0.001%
44	6.436	1675	1678	1679	rBV2	529	264	0.00%	0.000%
45	6.481	1688	1692	1694	rBV3	683	489	0.00%	0.001%
46	6.548	1711	1713	1719	rVB5	696	595	0.00%	0.001%
47	6.577	1719	1722	1727	rVB3	790	489	0.00%	0.001%
48	6.600	1727	1729	1730	rBV	456	185	0.00%	0.000%
49	6.654	1742	1746	1749	rBV2	1221	839	0.00%	0.001%
50	6.690	1752	1757	1759	rBV3	832	746	0.00%	0.001%
51	6.725	1766	1768	1771	rVB	495	210	0.00%	0.000%
52	6.764	1777	1780	1781	rBV2	752	417	0.00%	0.001%
53	6.841	1799	1804	1805	rBV3	730	475	0.00%	0.001%
54	6.876	1812	1815	1820	rVB2	938	876	0.00%	0.001%
55	6.902	1820	1823	1825	rBV3	510	262	0.00%	0.000%
56	6.921	1825	1829	1830	rBV2	642	365	0.00%	0.001%
57	6.989	1839	1850	1878	rBV	305126	551052	1.48%	0.918%
58	7.320	1940	1953	1971	rBV	1155289	1973797	5.30%	3.289%
59	7.625	2038	2048	2065	rBV	213798	368438	0.99%	0.614%
60	7.831	2109	2112	2114	rBV3	871	487	0.00%	0.001%
61	7.982	2142	2159	2184	rBV	22538878	37240761	100.00%	62.049%
62	8.091	2185	2193	2226	rVB	582955	1090091	2.93%	1.816%
63	8.718	2383	2388	2389	rBV5	1020	889	0.00%	0.001%
64	8.796	2407	2412	2416	rBV6	1094	1204	0.00%	0.002%
65	8.857	2419	2431	2459	rBV	1128621	1838197	4.94%	3.063%
66	9.246	2545	2552	2553	rBV5	923	1090	0.00%	0.002%
67	9.281	2561	2563	2568	rBV2	590	536	0.00%	0.001%
68	9.326	2574	2577	2580	rVB3	880	474	0.00%	0.001%
69	9.349	2580	2584	2587	rBV4	602	616	0.00%	0.001%
70	9.628	2666	2671	2673	rBV2	619	624	0.00%	0.001%
71	9.673	2683	2685	2687	rBV3	868	410	0.00%	0.001%
72	9.731	2701	2703	2705	rBV2	575	308	0.00%	0.001%
73	9.876	2743	2748	2751	rBV2	631	477	0.00%	0.001%
74	9.889	2751	2752	2755	rBV2	361	181	0.00%	0.000%
75	10.008	2786	2789	2791	rBV	736	416	0.00%	0.001%
76	10.050	2798	2802	2804	rBV2	1200	816	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
 Data File : VV021170.D
 Acq On : 27 Apr 2021 13:05
 Operator : SY/MD
 Sample : M2326-02 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	10.130	2820	2827	2837	rVB6	5731	8559	0.02%	0.014%
78	10.172	2837	2840	2843	rBV4	676	478	0.00%	0.001%
79	10.220	2844	2855	2877	rBV	758383	1211727	3.25%	2.019%
80	10.525	2945	2950	2953	rBV4	1267	1241	0.00%	0.002%
81	10.751	3015	3020	3025	rBV4	1208	1181	0.00%	0.002%
82	10.924	3063	3074	3088	rVB4	6146	10406	0.03%	0.017%
83	10.972	3088	3089	3091	rBV4	494	191	0.00%	0.000%
84	11.005	3096	3099	3101	rVB2	761	329	0.00%	0.001%
85	11.146	3136	3143	3144	rBV6	2681	2509	0.01%	0.004%
86	11.255	3165	3177	3198	rBV	1143106	1775542	4.77%	2.958%
87	11.503	3252	3254	3256	rBV2	816	398	0.00%	0.001%
88	11.632	3281	3294	3312	rBV	1178566	1863779	5.00%	3.105%
89	11.943	3389	3391	3393	rBV	577	239	0.00%	0.000%
90	12.050	3421	3424	3426	rBV2	907	698	0.00%	0.001%
91	12.191	3463	3468	3472	rBV4	840	978	0.00%	0.002%
92	12.226	3476	3479	3483	rBV2	622	582	0.00%	0.001%
93	12.410	3533	3536	3538	rBV	727	535	0.00%	0.001%
94	12.525	3570	3572	3575	rVB2	972	412	0.00%	0.001%
95	12.599	3590	3595	3596	rBV3	1153	714	0.00%	0.001%
96	12.676	3617	3619	3623	rBV4	918	574	0.00%	0.001%
97	12.812	3659	3661	3665	rBV2	914	475	0.00%	0.001%
98	12.908	3687	3691	3694	rBV2	1275	1059	0.00%	0.002%
99	13.149	3762	3766	3770	rBV3	1155	911	0.00%	0.002%
100	13.828	3973	3977	3983	rVB5	1224	1236	0.00%	0.002%




Sum of corrected areas: 60018636

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
Data File : VV021170.D
Acq On : 27 Apr 2021 13:05
Operator : SY/MD
Sample : M2326-02 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

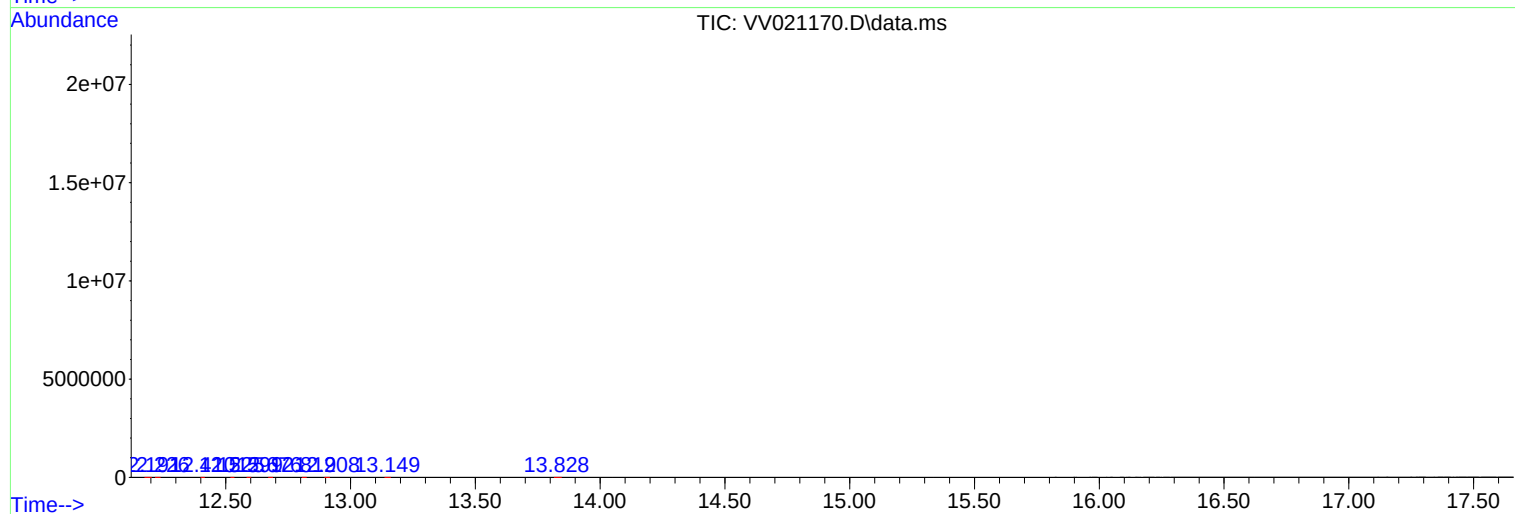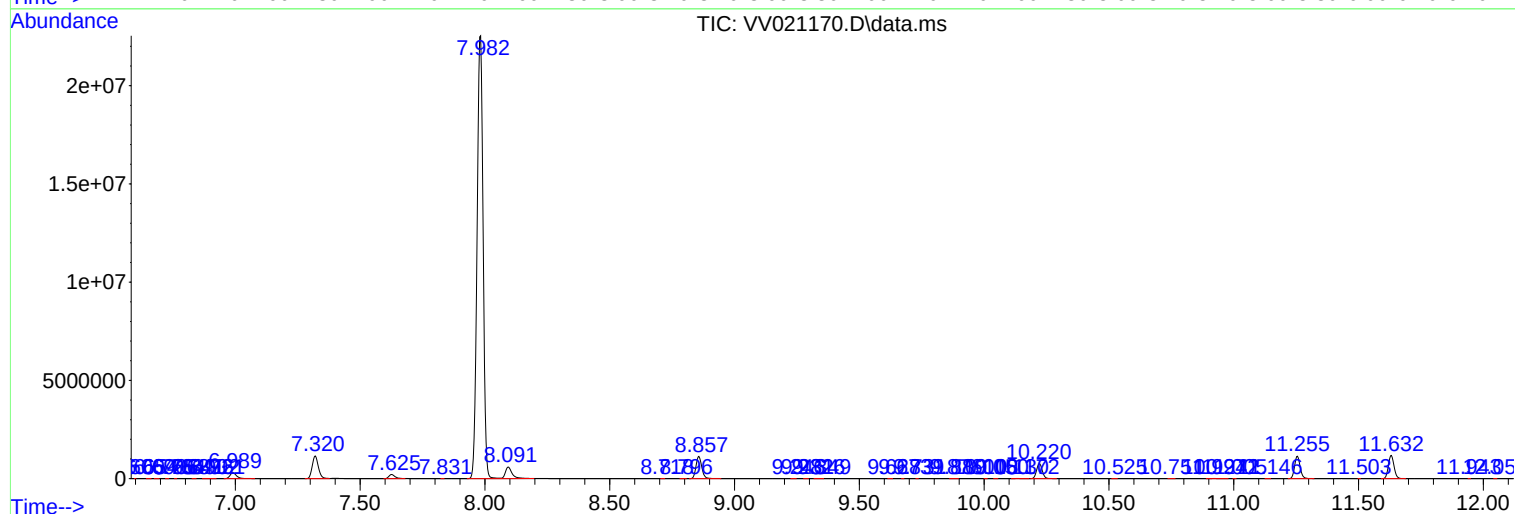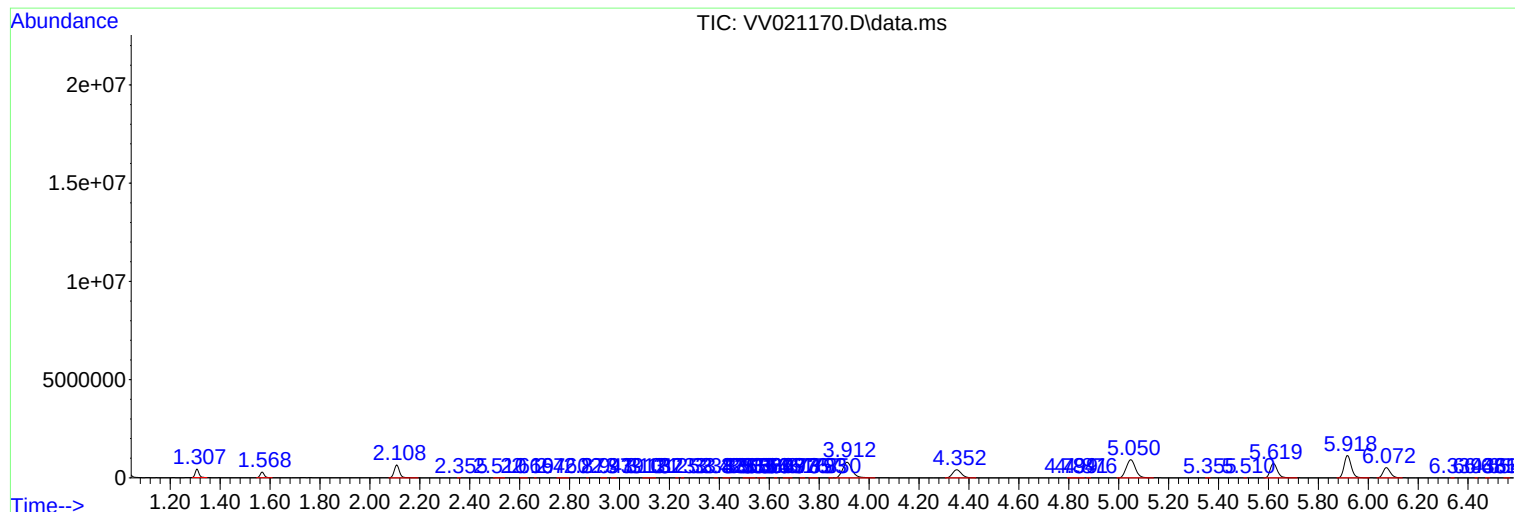

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
Data File : VV021170.D
Acq On : 27 Apr 2021 13:05
Operator : SY/MD
Sample : M2326-02 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
Data File : VV021170.D
Acq On : 27 Apr 2021 13:05
Operator : SY/MD
Sample : M2326-02 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
