

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
 Data File : VV021172.D
 Acq On : 27 Apr 2021 13:57
 Operator : SY/MD
 Sample : M2326-01DL 1000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

Signal : TIC: VV021172.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	97	rVB	387694	392812	16.08%	1.855%
2	1.571	158	165	176	rVB	297307	334368	13.69%	1.579%
3	2.108	323	332	360	rVB	670903	981320	40.18%	4.635%
4	2.359	407	410	413	rBV2	760	454	0.02%	0.002%
5	2.378	413	416	418	rBV2	691	423	0.02%	0.002%
6	2.436	431	434	437	rBV3	1069	833	0.03%	0.004%
7	2.506	450	456	466	rBV6	4507	6785	0.28%	0.032%
8	2.564	471	474	476	rVB2	632	370	0.02%	0.002%
9	2.577	476	478	479	rBV2	666	300	0.01%	0.001%
10	2.629	492	494	497	rVB3	906	557	0.02%	0.003%
11	2.764	533	536	539	rBV2	633	467	0.02%	0.002%
12	2.780	539	541	544	rBV2	488	328	0.01%	0.002%
13	3.018	613	615	617	rBV2	458	244	0.01%	0.001%
14	3.031	617	619	621	rBV	598	285	0.01%	0.001%
15	3.098	636	640	642	rBV2	904	507	0.02%	0.002%
16	3.111	642	644	646	rVB2	524	218	0.01%	0.001%
17	3.214	672	676	678	rBV	383	286	0.01%	0.001%
18	3.285	694	698	700	rBV2	754	599	0.02%	0.003%
19	3.359	718	721	726	rVB3	688	433	0.02%	0.002%
20	3.397	726	733	735	rBV	488	604	0.02%	0.003%
21	3.561	780	784	788	rVB	400	287	0.01%	0.001%
22	3.670	813	818	820	rVV3	590	492	0.02%	0.002%
23	3.703	825	828	829	rBV	544	297	0.01%	0.001%
24	3.744	838	841	843	rBV2	477	343	0.01%	0.002%
25	3.854	872	875	877	rBV2	484	290	0.01%	0.001%
26	3.902	879	890	926	rBV	123472	448244	18.35%	2.117%
27	4.349	1014	1029	1060	rBV	422588	1045590	42.81%	4.939%
28	4.558	1092	1094	1098	rBV2	816	599	0.02%	0.003%
29	4.764	1155	1158	1160	rBV4	709	487	0.02%	0.002%
30	4.818	1172	1175	1177	rVB3	798	391	0.02%	0.002%
31	4.860	1184	1188	1189	rBV2	530	393	0.02%	0.002%
32	4.902	1198	1201	1204	rBV2	497	428	0.02%	0.002%
33	4.924	1204	1208	1211	rVV3	698	556	0.02%	0.003%
34	4.966	1219	1221	1224	rBV3	592	233	0.01%	0.001%
35	5.050	1230	1247	1276	rBV2	963446	2442532	100.00%	11.538%
36	5.397	1352	1355	1356	rBV2	916	558	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
 Data File : VV021172.D
 Acq On : 27 Apr 2021 13:57
 Operator : SY/MD
 Sample : M2326-01DL 1000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	5.481	1379	1381	1384	rVV4	739	306	0.01%	0.001%
38	5.510	1388	1390	1392	rVB3	918	388	0.02%	0.002%
39	5.529	1394	1396	1402	rBV4	672	519	0.02%	0.002%
40	5.619	1410	1424	1458	rBV	766546	1564376	64.05%	7.390%
41	5.921	1505	1518	1538	rBV8	57333	137546	5.63%	0.650%
42	6.072	1550	1565	1590	rBV	533257	1086204	44.47%	5.131%
43	6.304	1633	1637	1638	rBV2	977	695	0.03%	0.003%
44	6.416	1670	1672	1673	rBV2	489	256	0.01%	0.001%
45	6.445	1679	1681	1685	rVB3	943	464	0.02%	0.002%
46	6.465	1685	1687	1690	rBV	519	331	0.01%	0.002%
47	6.577	1719	1722	1724	rBV2	877	573	0.02%	0.003%
48	6.670	1749	1751	1753	rBV3	661	233	0.01%	0.001%
49	6.780	1779	1785	1789	rBV4	1279	1257	0.05%	0.006%
50	6.841	1802	1804	1807	rVB2	561	291	0.01%	0.001%
51	6.857	1807	1809	1811	rBV	552	336	0.01%	0.002%
52	6.989	1839	1850	1872	rBV	303372	555065	22.72%	2.622%
53	7.210	1917	1919	1924	rBV3	892	588	0.02%	0.003%
54	7.320	1940	1953	1971	rBV	1168657	2021405	82.76%	9.548%
55	7.625	2036	2048	2075	rBV	225355	390253	15.98%	1.843%
56	7.866	2121	2123	2126	rVB	942	420	0.02%	0.002%
57	7.918	2136	2139	2141	rBV	1005	767	0.03%	0.004%
58	7.979	2145	2158	2176	rBV	1156003	1922142	78.69%	9.079%
59	8.091	2184	2193	2232	rBV	523969	979565	40.10%	4.627%
60	8.516	2320	2325	2329	rBV3	898	876	0.04%	0.004%
61	8.558	2336	2338	2343	rVB3	758	551	0.02%	0.003%
62	8.596	2346	2350	2352	rBV3	638	535	0.02%	0.003%
63	8.673	2372	2374	2376	rBV2	664	318	0.01%	0.002%
64	8.802	2410	2414	2417	rBV4	451	348	0.01%	0.002%
65	8.857	2419	2431	2452	rBV	1185129	1917896	78.52%	9.059%
66	9.072	2496	2498	2504	rVB5	1440	1001	0.04%	0.005%
67	9.143	2515	2520	2522	rBV3	1380	1201	0.05%	0.006%
68	9.207	2538	2540	2543	rBV	867	544	0.02%	0.003%
69	9.259	2553	2556	2558	rBV3	951	499	0.02%	0.002%
70	9.355	2583	2586	2591	rVB2	916	605	0.02%	0.003%
71	9.452	2610	2616	2617	rBV3	706	616	0.03%	0.003%
72	9.522	2636	2638	2641	rBV2	560	390	0.02%	0.002%
73	9.587	2656	2658	2660	rBV2	870	371	0.02%	0.002%
74	9.677	2683	2686	2687	rBV2	700	348	0.01%	0.002%
75	9.731	2699	2703	2708	rBV3	463	506	0.02%	0.002%
76	9.783	2716	2719	2722	rBV2	742	352	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
 Data File : VV021172.D
 Acq On : 27 Apr 2021 13:57
 Operator : SY/MD
 Sample : M2326-01DL 1000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B3DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	9.802	2723	2725	2728	rBV2	637	378	0.02%	0.002%
78	9.863	2740	2744	2745	rBV2	506	362	0.01%	0.002%
79	10.008	2787	2789	2791	rVB	980	362	0.01%	0.002%
80	10.056	2802	2804	2807	rBV2	488	256	0.01%	0.001%
81	10.133	2820	2828	2834	rBV4	6778	9661	0.40%	0.046%
82	10.175	2839	2841	2843	rBV	692	263	0.01%	0.001%
83	10.223	2843	2856	2879	rBV	780097	1216963	49.82%	5.748%
84	10.439	2920	2923	2924	rBV2	577	261	0.01%	0.001%
85	10.709	3003	3007	3009	rBV2	709	560	0.02%	0.003%
86	10.902	3063	3067	3068	rBV2	1824	1150	0.05%	0.005%
87	10.927	3069	3075	3086	rVB2	5809	9239	0.38%	0.044%
88	11.030	3103	3107	3111	rBV3	1116	993	0.04%	0.005%
89	11.255	3165	3177	3199	rBV	1154723	1800976	73.73%	8.507%
90	11.574	3272	3276	3279	rBV3	1204	848	0.03%	0.004%
91	11.632	3281	3294	3310	rBV	1166134	1866403	76.41%	8.816%
92	11.841	3354	3359	3360	rBV5	1076	955	0.04%	0.005%
93	11.995	3404	3407	3408	rBV	1121	603	0.02%	0.003%
94	12.027	3415	3417	3420	rVB3	1010	551	0.02%	0.003%
95	12.255	3484	3488	3493	rBV6	959	1215	0.05%	0.006%
96	12.895	3685	3687	3689	rBV	632	265	0.01%	0.001%
97	13.066	3738	3740	3743	rBV2	494	336	0.01%	0.002%
98	13.583	3897	3901	3904	rBV4	1454	1279	0.05%	0.006%
99	13.715	3938	3942	3946	rBV4	1033	934	0.04%	0.004%
100	13.940	4010	4012	4015	rBV2	720	543	0.02%	0.003%




Sum of corrected areas: 21170206

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
Data File : VV021172.D
Acq On : 27 Apr 2021 13:57
Operator : SY/MD
Sample : M2326-01DL 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

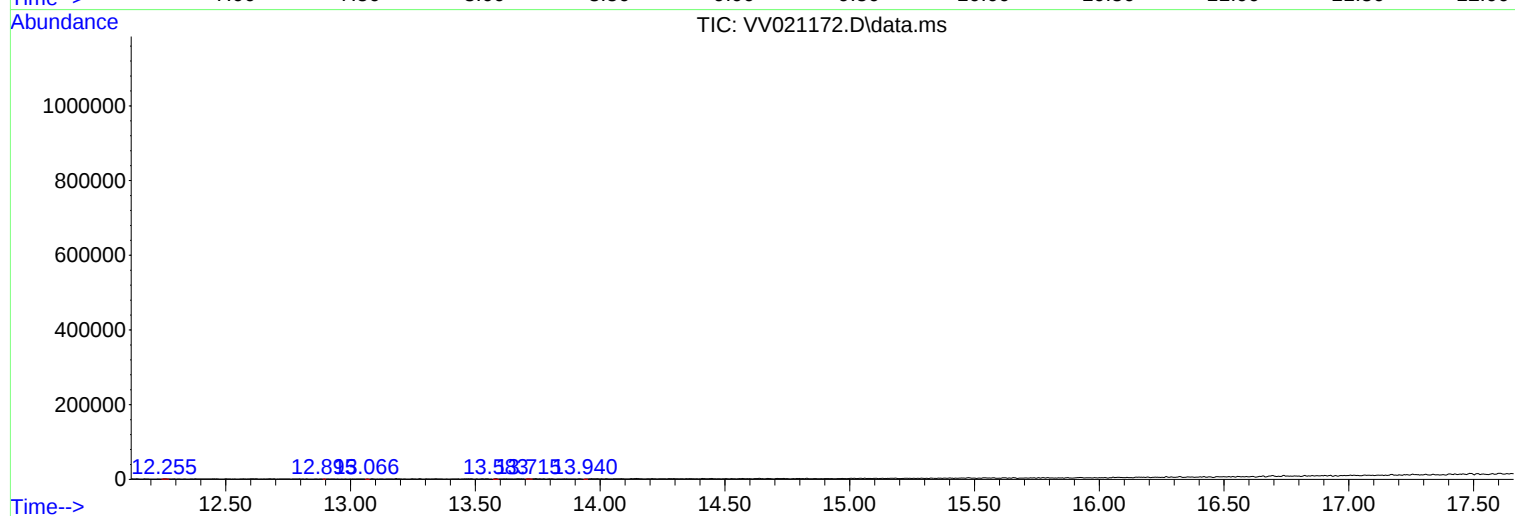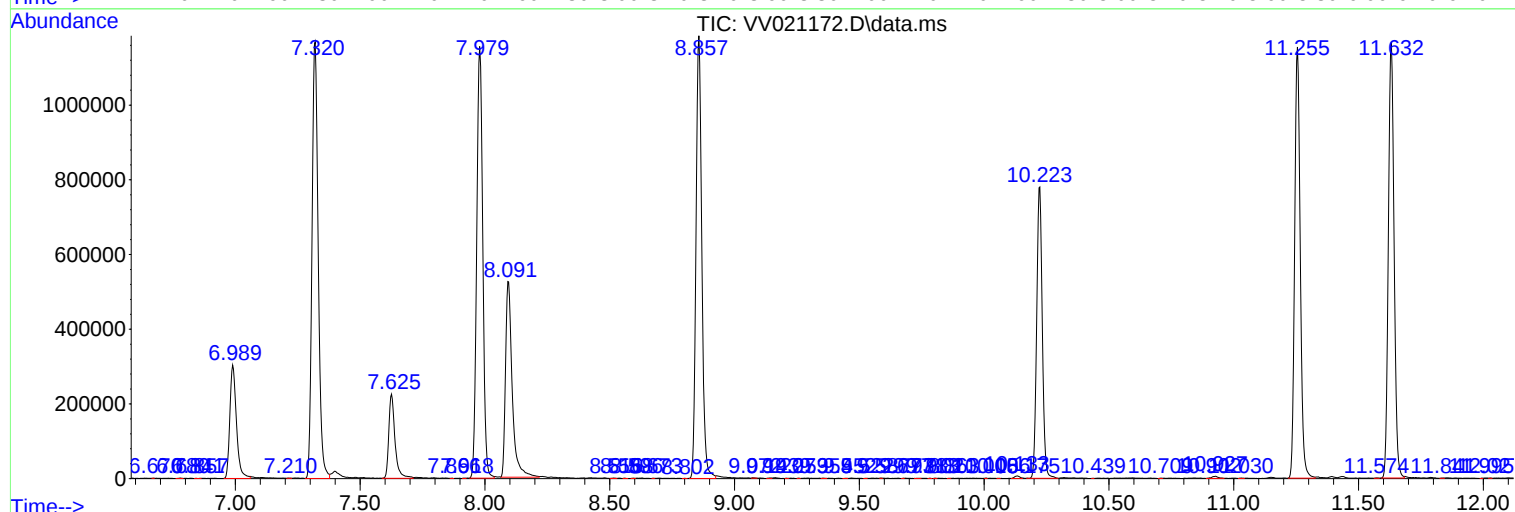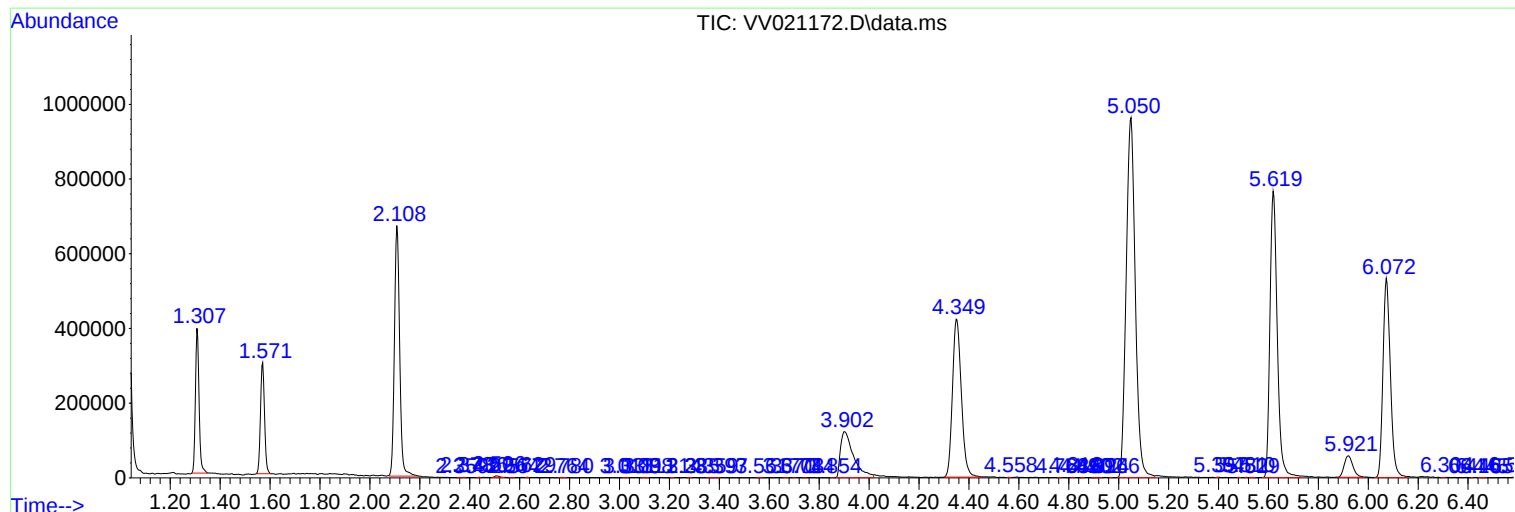

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
Data File : VV021172.D
Acq On : 27 Apr 2021 13:57
Operator : SY/MD
Sample : M2326-01DL 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
Data File : VV021172.D
Acq On : 27 Apr 2021 13:57
Operator : SY/MD
Sample : M2326-01DL 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B3DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
