

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
 Data File : VV021173.D
 Acq On : 27 Apr 2021 14:19
 Operator : SY/MD
 Sample : M2326-02DL 1000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M

Title : VOC Analysis

Signal : TIC: VV021173.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	99	rVB	371641	392362	16.06%	1.882%
2	1.571	158	165	177	rVB	290581	329940	13.51%	1.583%
3	2.111	322	333	362	rBV	646574	962141	39.39%	4.615%
4	2.294	388	390	396	rVB4	1263	1087	0.04%	0.005%
5	2.320	396	398	399	rBV4	812	388	0.02%	0.002%
6	2.400	421	423	425	rBV2	693	359	0.01%	0.002%
7	2.481	446	448	451	rBV2	745	430	0.02%	0.002%
8	2.584	477	480	482	rBV2	935	498	0.02%	0.002%
9	2.619	487	491	492	rBV2	756	622	0.03%	0.003%
10	2.773	533	539	541	rBV3	819	736	0.03%	0.004%
11	2.879	567	572	576	rBV2	762	797	0.03%	0.004%
12	2.950	591	594	598	rVB	471	282	0.01%	0.001%
13	3.040	619	622	624	rBV3	532	303	0.01%	0.001%
14	3.198	669	671	675	rBV2	528	342	0.01%	0.002%
15	3.217	675	677	681	rVB	670	299	0.01%	0.001%
16	3.246	681	686	689	rBV3	574	329	0.01%	0.002%
17	3.368	719	724	728	rBV2	781	692	0.03%	0.003%
18	3.442	744	747	750	rBV3	680	460	0.02%	0.002%
19	3.548	778	780	784	rBV2	602	433	0.02%	0.002%
20	3.725	831	835	837	rVB2	857	614	0.03%	0.003%
21	3.764	843	847	849	rBV3	457	380	0.02%	0.002%
22	3.912	877	893	927	rBV3	150512	534305	21.87%	2.563%
23	4.355	1015	1031	1064	rVV	416627	1037572	42.48%	4.977%
24	4.481	1068	1070	1073	rBV5	1008	539	0.02%	0.003%
25	4.632	1115	1117	1119	rVB3	904	338	0.01%	0.002%
26	4.667	1125	1128	1133	rVB2	1143	912	0.04%	0.004%
27	4.690	1133	1135	1138	rBV2	551	453	0.02%	0.002%
28	4.805	1165	1171	1176	rVB4	656	974	0.04%	0.005%
29	4.831	1176	1179	1181	rBV2	734	527	0.02%	0.003%
30	4.860	1186	1188	1189	rBV	622	301	0.01%	0.001%
31	4.918	1204	1206	1209	rVB2	682	367	0.02%	0.002%
32	4.937	1209	1212	1214	rBV	629	346	0.01%	0.002%
33	4.947	1214	1215	1222	rBV3	468	455	0.02%	0.002%
34	5.050	1230	1247	1286	rBV2	930756	2442683	100.00%	11.717%
35	5.413	1357	1360	1361	rBV2	1013	451	0.02%	0.002%
36	5.487	1380	1383	1386	rVB4	910	507	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
 Data File : VV021173.D
 Acq On : 27 Apr 2021 14:19
 Operator : SY/MD
 Sample : M2326-02DL 1000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

37	5.622	1412	1425	1454	rBV	775606	1537741	62.95%	7.376%
38	5.921	1505	1518	1538	rBV7	63387	146207	5.99%	0.701%
39	6.075	1552	1566	1596	rBV	520215	1076667	44.08%	5.165%
40	6.268	1624	1626	1630	rBV4	1076	713	0.03%	0.003%
41	6.677	1750	1753	1755	rVB2	1029	582	0.02%	0.003%
42	6.690	1755	1757	1762	rVB	526	288	0.01%	0.001%
43	6.719	1763	1766	1770	rVB3	707	522	0.02%	0.003%
44	6.953	1835	1839	1840	rBV2	577	357	0.01%	0.002%
45	6.992	1840	1851	1871	rBV	298141	546537	22.37%	2.622%
46	7.178	1907	1909	1913	rVB3	1313	629	0.03%	0.003%
47	7.275	1936	1939	1941	rBV2	956	614	0.03%	0.003%
48	7.320	1941	1953	1972	rBV	1135748	1973612	80.80%	9.467%
49	7.625	2037	2048	2065	rBV	210598	368079	15.07%	1.766%
50	7.979	2143	2158	2183	rBV	1036911	1740983	71.27%	8.351%
51	8.095	2184	2194	2224	rBV	546585	1019540	41.74%	4.891%
52	8.416	2292	2294	2298	rBV4	1295	1067	0.04%	0.005%
53	8.500	2318	2320	2322	rBV2	1013	526	0.02%	0.003%
54	8.545	2332	2334	2339	rBV2	840	551	0.02%	0.003%
55	8.567	2339	2341	2343	rBV2	589	297	0.01%	0.001%
56	8.857	2419	2431	2460	rBV	1145570	1874145	76.72%	8.990%
57	9.082	2498	2501	2503	rBV3	941	614	0.03%	0.003%
58	9.111	2509	2510	2514	rVB3	845	279	0.01%	0.001%
59	9.153	2519	2523	2524	rBV4	1584	1084	0.04%	0.005%
60	9.178	2529	2531	2533	rBV2	749	380	0.02%	0.002%
61	9.609	2662	2665	2668	rBV3	933	552	0.02%	0.003%
62	9.661	2679	2681	2686	rBV3	617	528	0.02%	0.003%
63	9.808	2724	2727	2730	rBV2	669	555	0.02%	0.003%
64	9.844	2735	2738	2739	rBV2	703	350	0.01%	0.002%
65	10.133	2821	2828	2838	rVB4	6610	9228	0.38%	0.044%
66	10.223	2843	2856	2876	rBV	789251	1238081	50.69%	5.939%
67	10.387	2904	2907	2912	rVB6	1546	1244	0.05%	0.006%
68	10.506	2942	2944	2947	rBV3	423	277	0.01%	0.001%
69	10.770	3023	3026	3030	rVB	1049	789	0.03%	0.004%
70	10.796	3030	3034	3035	rBV	681	461	0.02%	0.002%
71	10.828	3041	3044	3049	rBV4	983	860	0.04%	0.004%
72	10.921	3069	3073	3082	rVB5	5255	6648	0.27%	0.032%
73	10.985	3091	3093	3096	rVB2	957	480	0.02%	0.002%
74	11.037	3106	3109	3114	rBV3	840	788	0.03%	0.004%
75	11.114	3131	3133	3136	rVB	705	303	0.01%	0.001%
76	11.156	3138	3146	3154	rBV8	3113	4859	0.20%	0.023%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
 Data File : VV021173.D
 Acq On : 27 Apr 2021 14:19
 Operator : SY/MD
 Sample : M2326-02DL 1000X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7B4DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis

77	11.197	3157	3159	3164	rBV2	912	667	0.03%	0.003%
78	11.255	3165	3177	3197	rBV	1112629	1713410	70.14%	8.219%
79	11.570	3270	3275	3277	rBV3	1357	1260	0.05%	0.006%
80	11.632	3282	3294	3317	rVV	1177015	1846310	75.59%	8.856%
81	11.914	3379	3382	3385	rBV4	971	770	0.03%	0.004%
82	12.021	3413	3415	3420	rVB2	1184	630	0.03%	0.003%
83	12.050	3420	3424	3426	rBV3	1199	957	0.04%	0.005%
84	12.329	3509	3511	3515	rBV3	662	488	0.02%	0.002%
85	12.374	3522	3525	3527	rBV	857	599	0.02%	0.003%
86	12.448	3544	3548	3553	rBV4	813	856	0.04%	0.004%
87	12.513	3564	3568	3569	rBV3	1128	865	0.04%	0.004%
88	12.651	3609	3611	3613	rBV2	589	315	0.01%	0.002%
89	12.712	3625	3630	3634	rBV2	608	687	0.03%	0.003%
90	12.779	3648	3651	3654	rVB	1351	837	0.03%	0.004%
91	12.850	3670	3673	3676	rVB3	866	426	0.02%	0.002%
92	13.217	3784	3787	3791	rBV2	942	691	0.03%	0.003%
93	13.355	3828	3830	3833	rBV	740	475	0.02%	0.002%
94	13.429	3849	3853	3856	rBV3	1160	940	0.04%	0.005%
95	13.458	3860	3862	3865	rVB3	598	284	0.01%	0.001%
96	13.480	3865	3869	3870	rBV2	832	655	0.03%	0.003%
97	13.631	3914	3916	3919	rBV	1072	641	0.03%	0.003%
98	13.702	3935	3938	3939	rBV	788	438	0.02%	0.002%
99	14.024	4035	4038	4040	rBV2	805	538	0.02%	0.003%
100	14.455	4170	4172	4178	rBV2	1225	972	0.04%	0.005%


Sum of corrected areas: 20846952

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
Data File : VV021173.D
Acq On : 27 Apr 2021 14:19
Operator : SY/MD
Sample : M2326-02DL 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

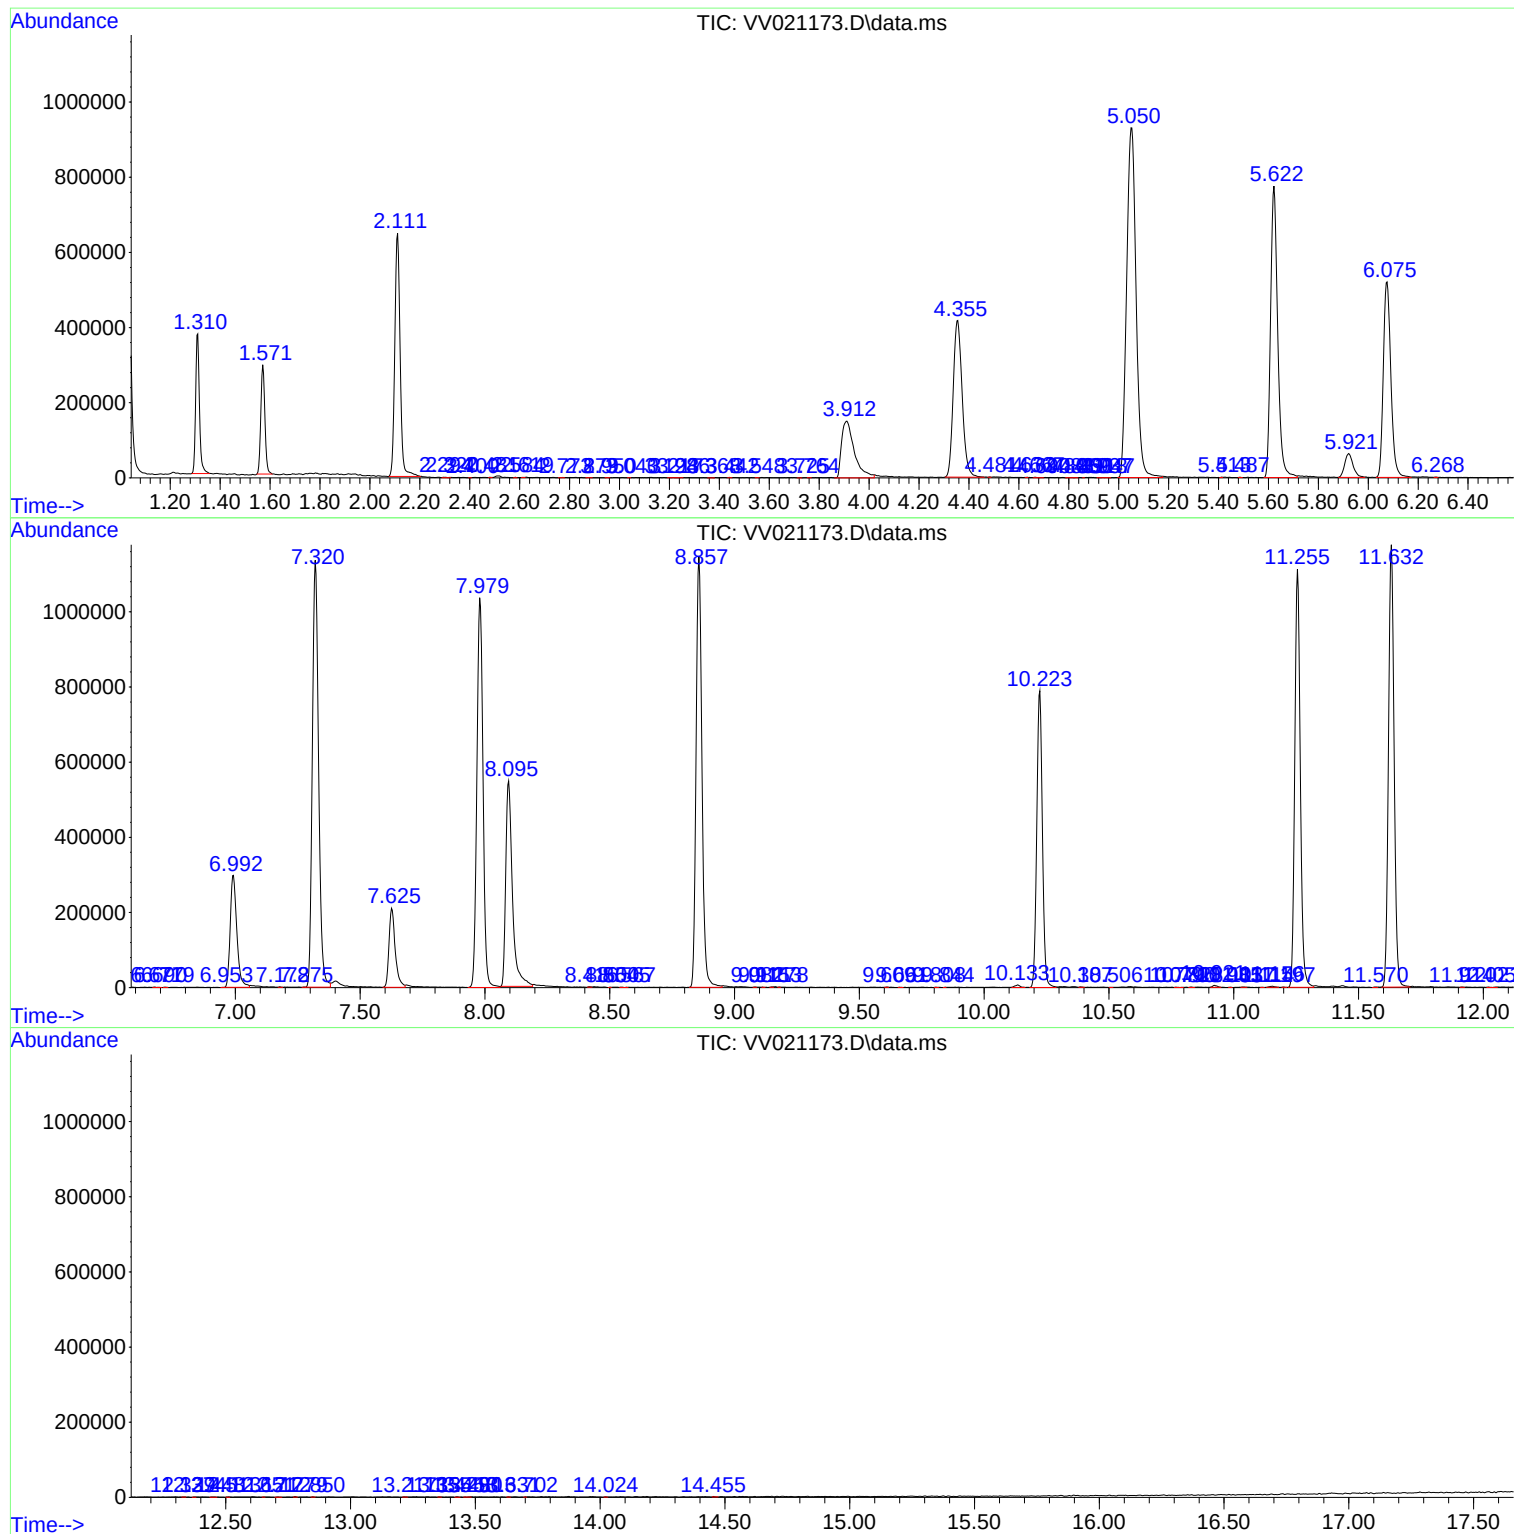

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
Data File : VV021173.D
Acq On : 27 Apr 2021 14:19
Operator : SY/MD
Sample : M2326-02DL 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
Data File : VV021173.D
Acq On : 27 Apr 2021 14:19
Operator : SY/MD
Sample : M2326-02DL 1000X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7B4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
