


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042721\
 Data File : VV021162.D
 Acq On : 27 Apr 2021 09:32
 Operator : SY/MD
 Sample : BFB90
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB190

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM042121WMA.M
 Title : VOC Analysis
 Last Update : Fri Apr 30 05:55:34 2021

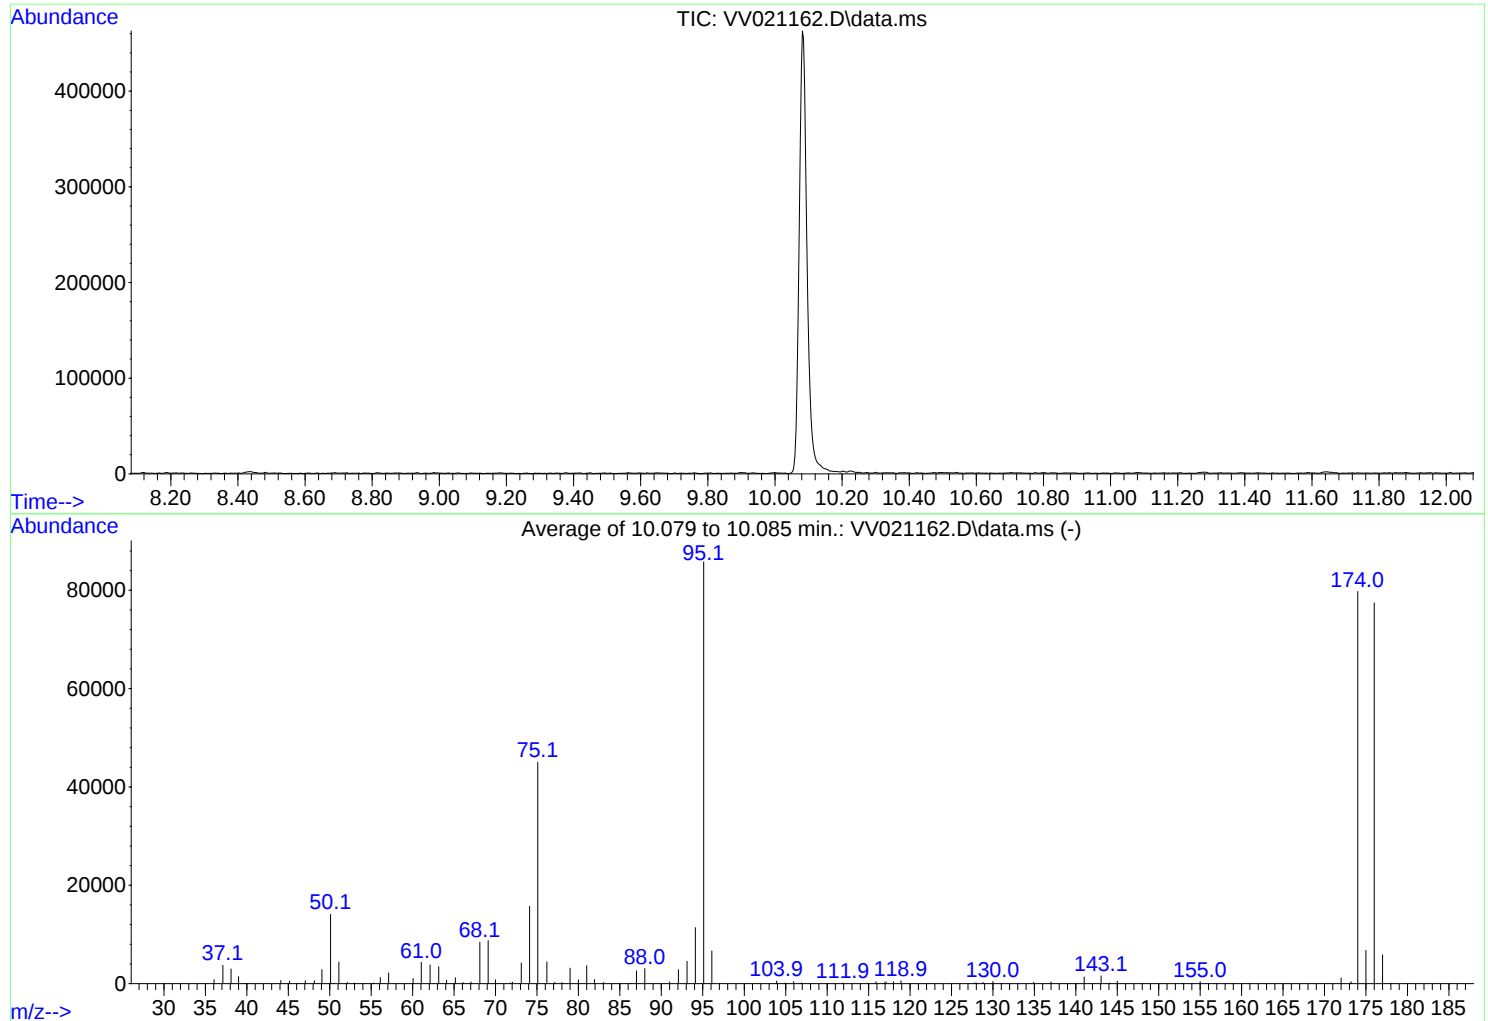

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2800

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	14092	PASS
75	95	30	80	52.5	45024	PASS
95	95	100	100	100.0	85779	PASS
96	95	5	9	7.8	6654	PASS
173	174	0.00	2	0.5	390	PASS
174	95	50	120	93.0	79747	PASS
175	174	5	9	8.5	6763	PASS
176	174	95	105	97.1	77437	PASS
177	176	5	10	7.6	5849	PASS

Scan 2800 (10.043 min): VV021162.D\data.ms
BFB90

m/z	Abundance
39.90	197.0
44.10	250.0
48.90	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB190

m/z	Abundance
36.10	882.0
37.10	3882.0
38.10	3063.0
39.00	1491.0
39.90	212.0
44.10	942.0
45.20	500.0
46.20	177.0
47.00	555.0
48.10	602.0
49.10	3046.0
50.10	14391.0
51.10	4586.0
52.20	234.0
53.00	172.0
55.30	172.0
56.10	1260.0
57.10	2239.0
60.10	1133.0
61.00	4427.0
62.10	4011.0
63.20	3623.0
64.10	662.0
65.20	1219.0
66.10	296.0
67.00	350.0
68.10	8583.0
69.10	9284.0
70.00	837.0
72.10	494.0
73.10	4324.0
74.10	16177.0
75.10	46672.0
76.20	4833.0
77.20	304.0
78.00	235.0
79.00	3294.0
80.00	803.0
81.00	3765.0
82.00	815.0
83.10	271.0
87.00	2640.0
88.00	3182.0
91.00	352.0
92.10	2957.0
93.10	4743.0
94.10	11798.0
95.10	88576.0
96.10	7013.0
103.90	587.0
105.00	104.0
105.90	406.0
106.90	169.0
111.90	173.0
114.90	128.0
115.90	402.0
117.10	566.0
118.00	407.0
118.90	620.0
127.80	280.0
128.80	283.0
130.00	492.0
134.90	304.0
137.00	387.0
141.00	1426.0
143.10	1622.0
144.10	159.0
145.00	550.0
147.90	104.0
152.80	135.0
155.00	475.0
172.00	1235.0
174.00	82320.0
175.00	7115.0
176.00	80120.0
177.00	6077.0
178.00	154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB190

m/z	Abundance
36.00	829.0
37.10	3697.0
38.10	2876.0
39.00	1411.0
39.90	211.0
43.50	114.0
44.10	851.0
45.20	570.0
47.00	622.0
48.10	512.0
49.10	2799.0
50.10	13576.0
51.10	4689.0
52.20	233.0
56.10	1111.0
57.10	2142.0
60.10	882.0
61.00	4860.0
62.10	4104.0
63.10	3166.0
64.10	604.0
65.10	1210.0
66.10	245.0
67.10	346.0
68.10	8616.0
69.10	8873.0
70.00	713.0
71.80	534.0
73.10	4477.0
74.10	15371.0
75.10	45416.0
76.20	4193.0
77.00	255.0
79.00	3189.0
80.00	710.0
81.00	3474.0
82.00	899.0
83.00	206.0
87.00	2639.0
88.00	3143.0
91.00	469.0
92.00	2960.0
93.10	4488.0
94.10	11593.0
95.10	85304.0
96.10	7149.0
103.90	456.0
104.90	109.0
106.00	437.0
106.80	201.0
111.90	125.0
115.90	355.0
117.10	571.0
118.00	462.0
118.90	543.0
128.00	398.0
128.80	140.0
130.00	412.0
130.90	151.0
134.90	251.0
137.00	338.0
141.00	1475.0
143.00	1463.0
144.10	134.0
145.00	386.0
148.00	138.0
152.90	160.0
155.00	336.0
159.10	107.0
161.00	167.0
172.00	1208.0
173.20	1171.0
174.00	82904.0
175.00	6775.0
176.00	81544.0
177.00	5406.0

Instrument :
MSVOA_V
ClientSampleId :
BFB190

m/z	Abundance
36.10	746.0
37.10	3577.0
38.10	3017.0
39.00	1394.0
39.90	218.0
44.10	876.0
45.10	491.0
46.20	167.0
47.10	620.0
48.20	628.0
49.10	3112.0
50.10	14310.0
51.10	3926.0
52.10	203.0
53.00	261.0
54.20	103.0
55.30	279.0
56.10	1284.0
57.10	2177.0
60.00	1085.0
61.10	3691.0
62.10	3357.0
63.20	3568.0
64.10	779.0
65.20	1197.0
66.10	181.0
67.10	266.0
68.10	8062.0
69.10	8150.0
70.00	777.0
72.00	429.0
73.10	3774.0
74.10	15629.0
75.10	42984.0
76.20	4263.0
77.20	335.0
78.00	420.0
79.00	3031.0
80.00	853.0
81.00	3680.0
81.90	685.0
83.10	254.0
86.30	216.0
87.00	2509.0
88.00	2820.0
91.00	225.0
92.10	2606.0
93.10	4485.0
94.10	10791.0
95.10	83456.0
96.10	5801.0
97.00	176.0
103.90	553.0
105.00	152.0
105.90	466.0
107.00	113.0
111.90	140.0
114.90	123.0
115.90	424.0
116.90	563.0
118.00	328.0
118.90	569.0
127.80	218.0
128.80	337.0
130.00	451.0
131.20	104.0
134.90	302.0
137.00	346.0
141.00	1154.0
143.10	1591.0
144.10	100.0
145.00	622.0
153.90	118.0
155.00	466.0
156.90	159.0
172.00	1027.0
174.00	74016.0
175.00	6398.0
176.00	70648.0
177.00	6065.0
178.00	172.0

Instrument :
MSVOA_V
ClientSampleId :
BFB190