

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042723\
 Data File : VW030901.D
 Acq On : 27 Apr 2023 12:57
 Operator : SY/MD
 Sample : 02475-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Apr 28 00:52:21 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 27 04:45:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	216092	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	211739	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	109775	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	67753	42.770	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	85.540%
7) Chloroethane-d5	1.536	69	56952	42.902	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	85.800%
11) 1,1-Dichloroethene-d2	2.063	65	32666	43.483	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.960%
21) 2-Butanone-d5	3.796	46	90020	103.460	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	103.460%
24) Chloroform-d	4.256	84	142325	49.577	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.160%
26) 1,2-Dichloroethane-d4	4.947	65	108293	58.673	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	117.340%
32) Benzene-d6	4.966	84	257346	51.406	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	102.820%
36) 1,2-Dichloropropane-d6	5.995	67	79255	50.967	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.940%
41) Toluene-d8	7.249	98	228329	48.578	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.160%
43) trans-1,3-Dichloroprop...	7.558	79	41956	53.531	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	107.060%
47) 2-Hexanone-d5	8.030	63	59308	96.816	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	96.820%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	113302	50.213	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	100.420%
66) 1,2-Dichlorobenzene-d4	11.567	152	99189	56.847	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	113.700%
Target Compounds						
44) trans-1,3-Dichloropropene	7.558	75	2392	0.937	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
Data File : VV030901.D
Acq On : 27 Apr 2023 12:57
Operator : SY/MD
Sample : 02475-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Apr 28 00:52:21 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 27 04:45:18 2023
Response via : Initial Calibration

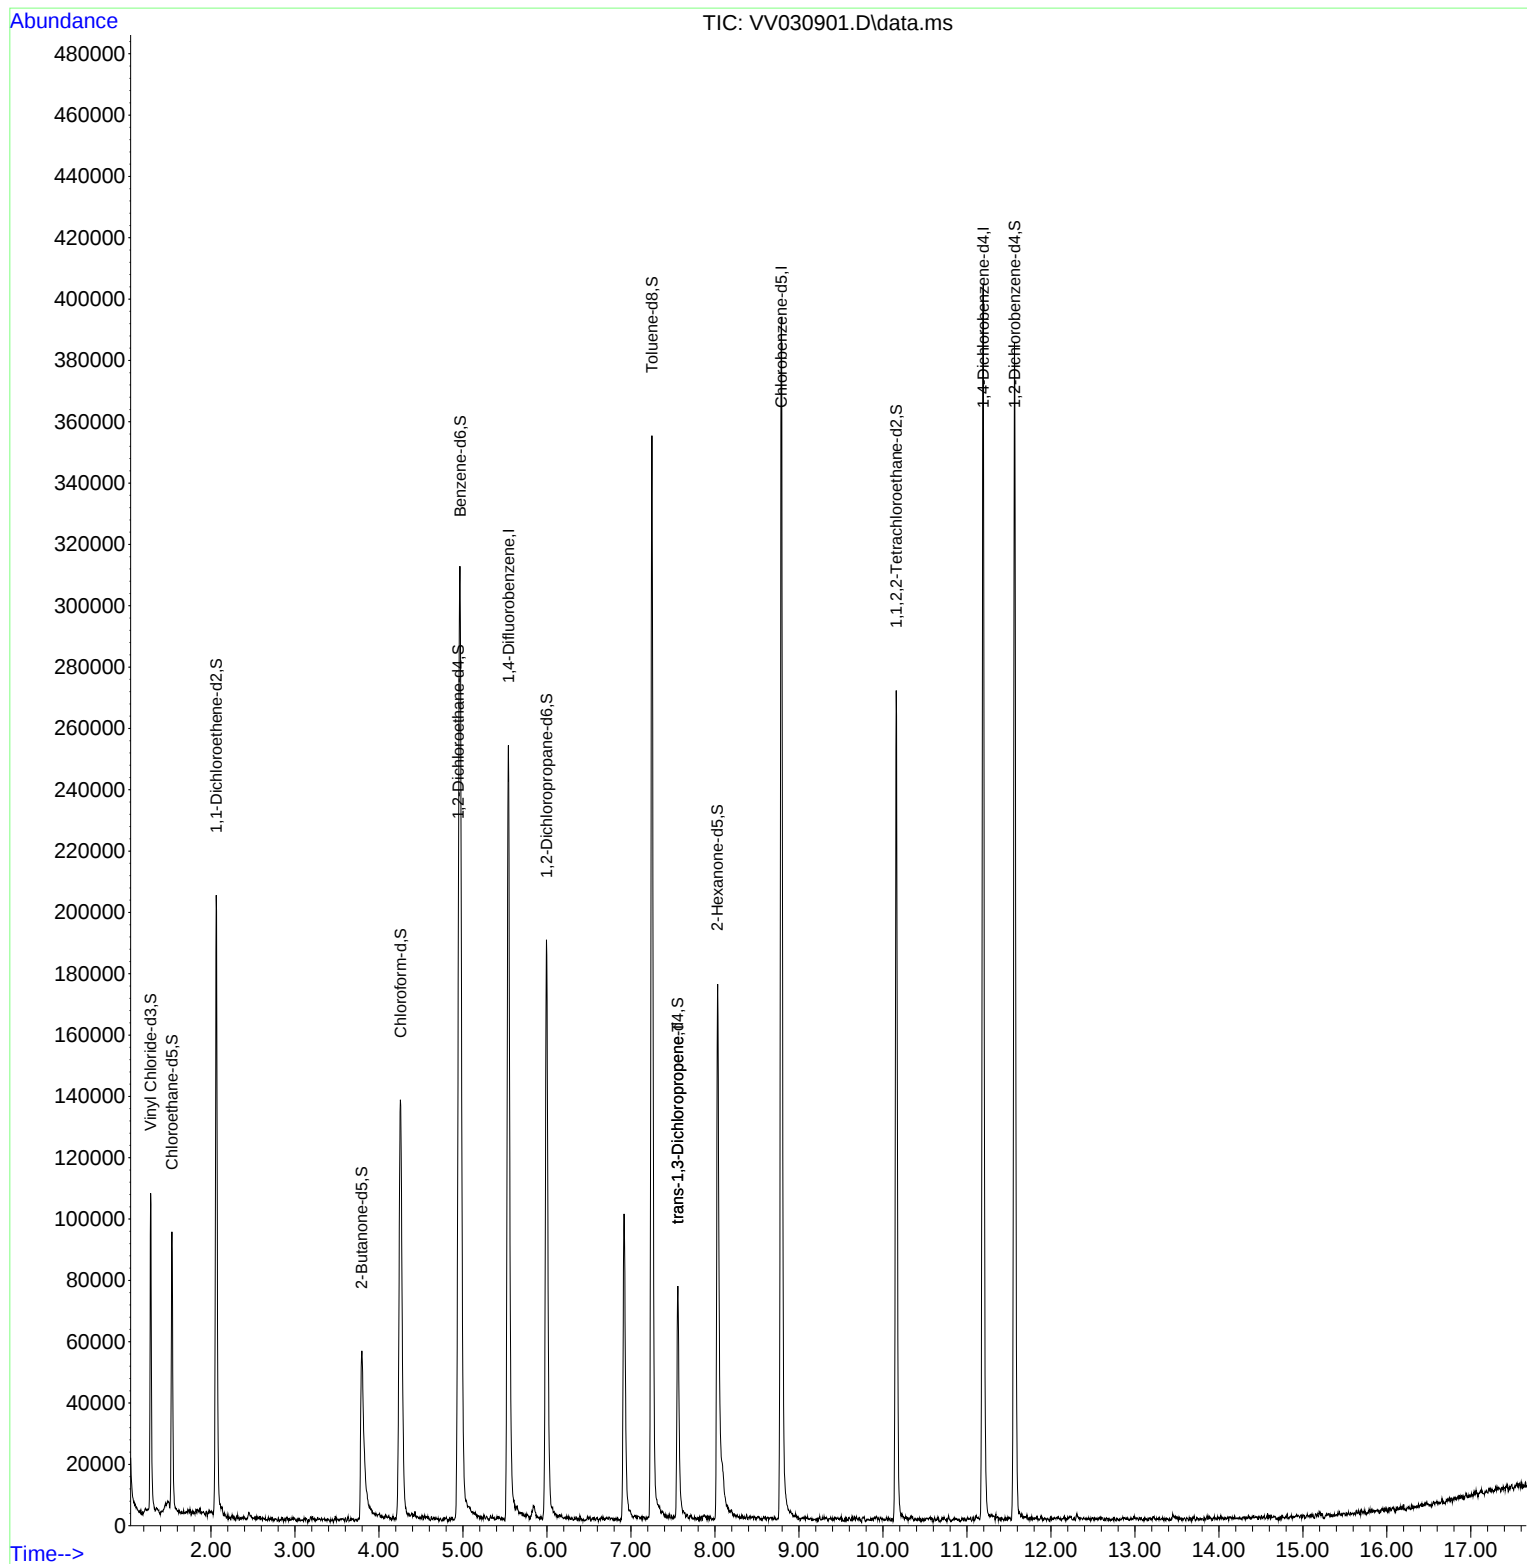

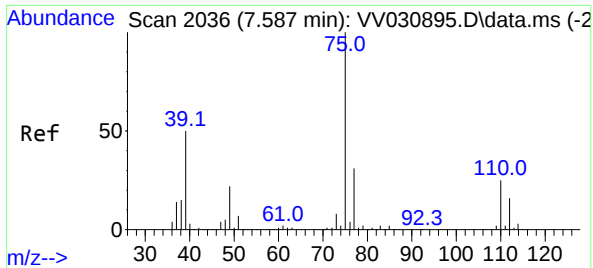

#44
 trans-1,3-Dichloropropene
 Concen: 0.937 ug/L
 RT: 7.558 min Scan# 2036
 Delta R.T. -0.029 min
 Lab File: VV030901.D
 Acq: 27 Apr 2023 12:57

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Tgt Ion:	75	Resp:	2392
Ion Ratio	Lower	Upper	
75	100		
77	36.7	22.1	41.1

