

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042723\
 Data File : VW030905.D
 Acq On : 27 Apr 2023 16:49
 Operator : SY/MD
 Sample : 02419-14ME
 Misc : 4.32g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW927ME

Quant Time: Apr 28 00:52:48 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 27 04:45:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	238803	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	231633	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	120868	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	73706	42.103	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	84.200%
7) Chloroethane-d5	1.536	69	59050	40.252	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	80.500%
11) 1,1-Dichloroethene-d2	2.063	65	36366	43.804	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.600%
21) 2-Butanone-d5	3.796	46	90064	93.667	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	93.670%
24) Chloroform-d	4.259	84	140827	44.390	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	88.780%
26) 1,2-Dichloroethane-d4	4.950	65	99251	48.660	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.320%
32) Benzene-d6	4.970	84	254107	46.400	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.800%
36) 1,2-Dichloropropane-d6	5.998	67	76470	44.952	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	89.900%
41) Toluene-d8	7.252	98	230391	44.807	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.620%
43) trans-1,3-Dichloroprop...	7.561	79	38340	44.716	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	89.440%
47) 2-Hexanone-d5	8.034	63	56039	83.623	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	83.620%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	106284	43.057	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.120%
66) 1,2-Dichlorobenzene-d4	11.567	152	98822	51.439	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.880%
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.561	75	2314	0.829	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
Data File : VV030905.D
Acq On : 27 Apr 2023 16:49
Operator : SY/MD
Sample : 02419-14ME
Misc : 4.32g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW927ME

Quant Time: Apr 28 00:52:48 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 27 04:45:18 2023
Response via : Initial Calibration

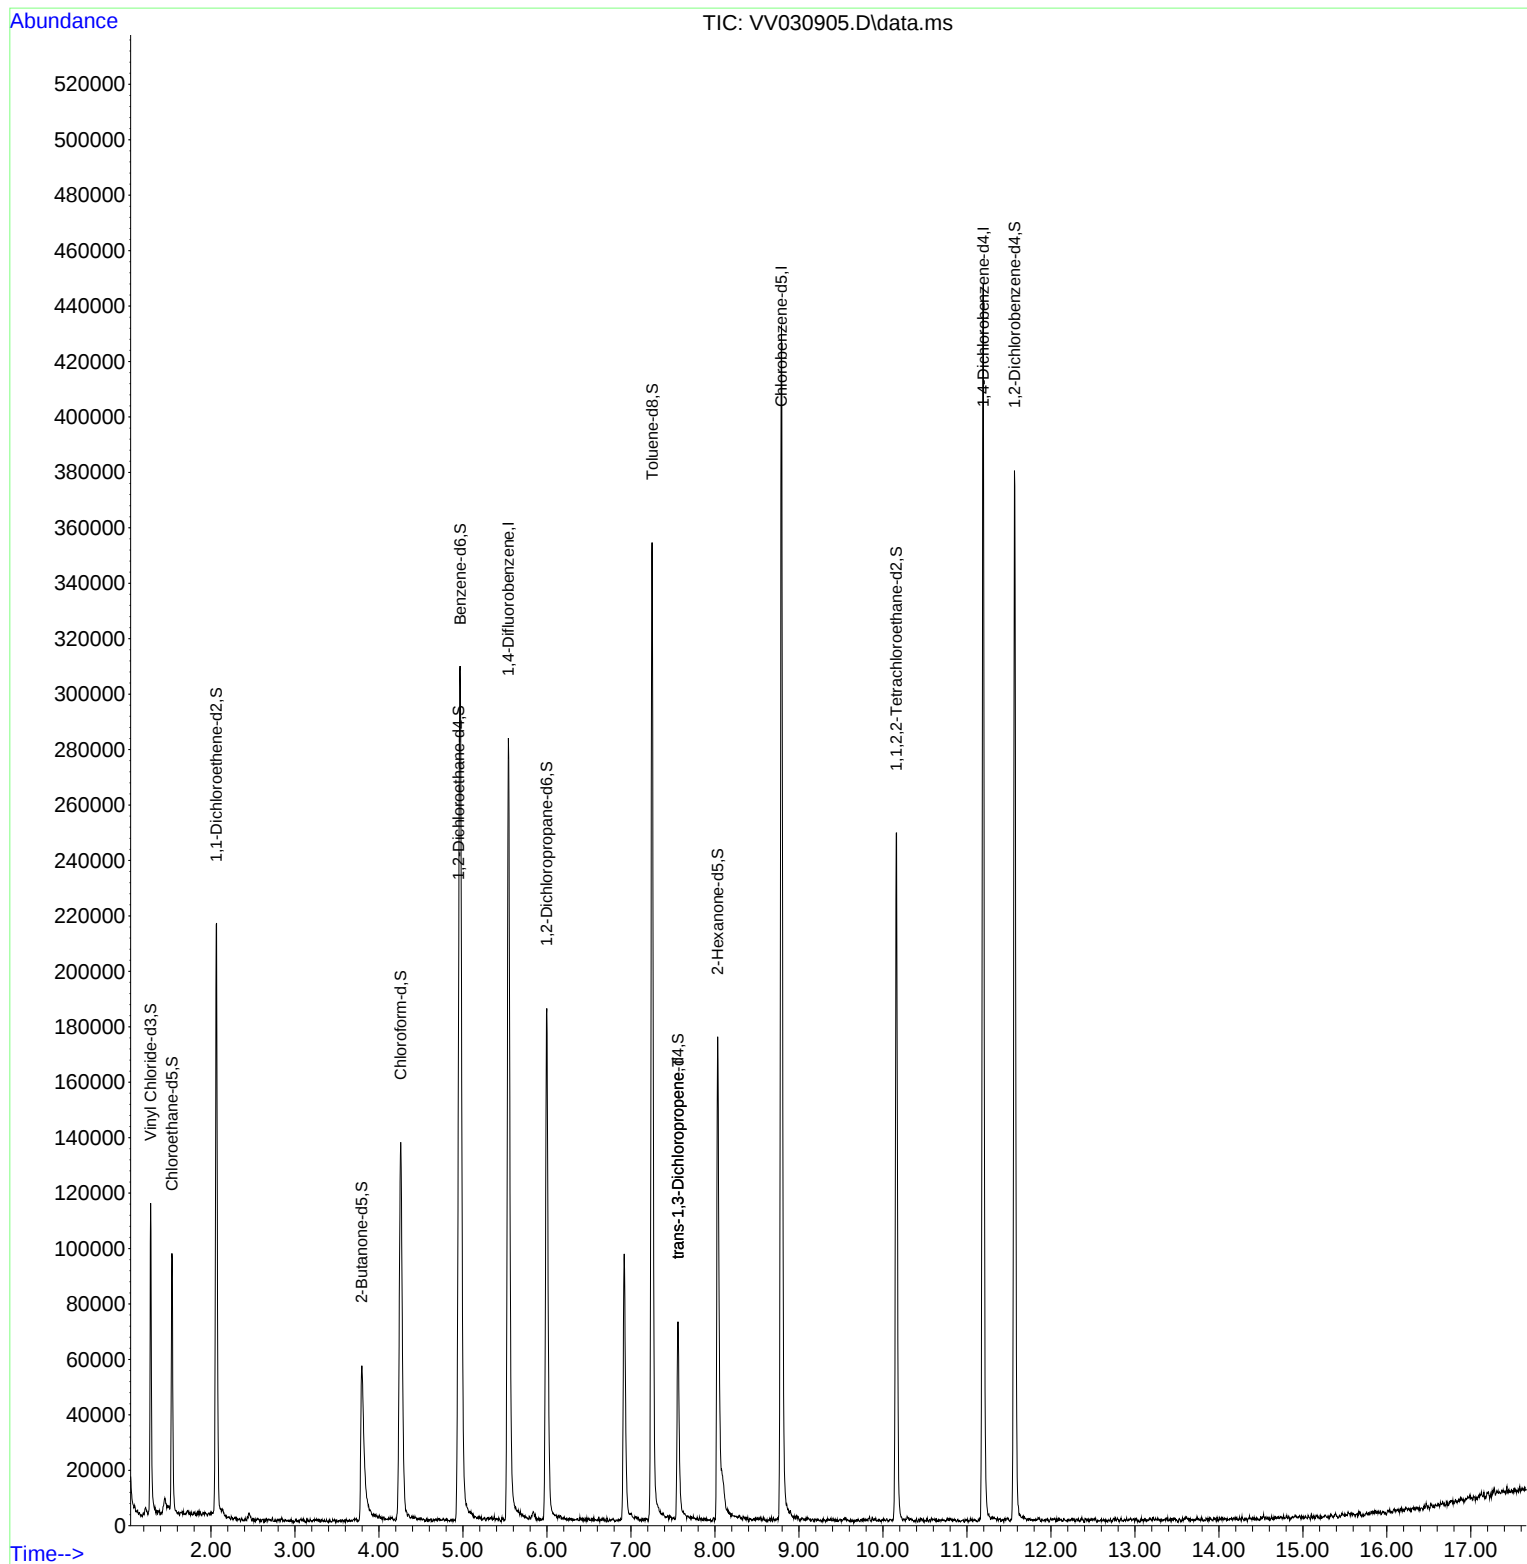

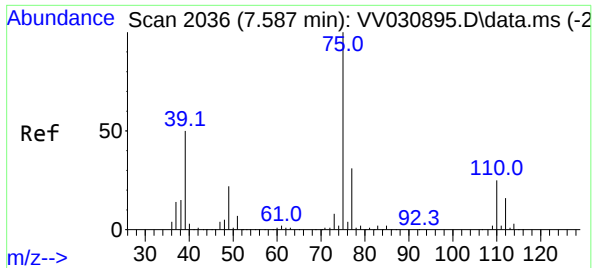

#44
 trans-1,3-Dichloropropene
 Concen: 0.829 ug/L
 RT: 7.561 min Scan# 20
 Delta R.T. -0.026 min
 Lab File: VV030905.D
 Acq: 27 Apr 2023 16:49

Instrument :
 MSVOA_V
 ClientSampleId :
 EW927ME

Tgt Ion: 75 Resp: 2314

Ion	Ratio	Lower	Upper
75	100		
77	39.2	22.1	41.1

