

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
 Data File : VV030897.D
 Acq On : 27 Apr 2023 11:11
 Operator : SY/MD
 Sample : VV0427WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK339

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030897.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	90	rBV	124241	139835	14.98%	1.886%
2	1.536	148	154	168	rVB	104433	132168	14.16%	1.783%
3	2.066	310	319	332	rBV	237262	342759	36.72%	4.623%
4	2.317	394	397	399	rBV3	1238	727	0.08%	0.010%
5	2.336	401	403	407	rBV4	785	636	0.07%	0.009%
6	2.439	429	435	436	rBV5	1623	1483	0.16%	0.020%
7	2.677	506	509	512	rBV5	799	605	0.06%	0.008%
8	2.716	516	521	525	rVV6	1228	1462	0.16%	0.020%
9	2.847	560	562	566	rVV5	1036	559	0.06%	0.008%
10	2.966	595	599	601	rBV5	1400	884	0.09%	0.012%
11	3.060	623	628	631	rVB6	1446	1193	0.13%	0.016%
12	3.079	631	634	641	rBV9	1186	1545	0.17%	0.021%
13	3.381	725	728	730	rBV3	1029	548	0.06%	0.007%
14	3.407	733	736	739	rBV5	1412	851	0.09%	0.011%
15	3.439	743	746	750	rBV4	1093	601	0.06%	0.008%
16	3.510	763	768	769	rBV4	711	532	0.06%	0.007%
17	3.571	785	787	790	rBV4	956	627	0.07%	0.008%
18	3.587	790	792	795	rVV3	1307	900	0.10%	0.012%
19	3.799	847	858	888	rBV2	61553	180791	19.37%	2.438%
20	4.259	987	1001	1023	rBV2	149175	374567	40.13%	5.052%
21	4.462	1061	1064	1066	rVB3	1286	788	0.08%	0.011%
22	4.481	1068	1070	1072	rBV2	990	518	0.06%	0.007%
23	4.700	1136	1138	1140	rBV3	1288	563	0.06%	0.008%
24	4.786	1161	1165	1167	rBV5	1357	1164	0.12%	0.016%
25	4.825	1173	1177	1182	rBV7	977	1085	0.12%	0.015%
26	4.909	1200	1203	1204	rBV2	1134	521	0.06%	0.007%
27	4.966	1204	1221	1247	rVV2	349465	933432	100.00%	12.590%
28	5.397	1353	1355	1358	rBV4	1350	969	0.10%	0.013%
29	5.445	1366	1370	1372	rBV5	1200	957	0.10%	0.013%
30	5.542	1386	1400	1424	rBV	303159	630534	67.55%	8.504%
31	5.783	1473	1475	1481	rVB7	1417	1168	0.13%	0.016%
32	5.825	1481	1488	1489	rBV6	2368	2100	0.22%	0.028%
33	5.899	1509	1511	1514	rBV4	1050	640	0.07%	0.009%
34	5.995	1528	1541	1560	rBV2	202911	422724	45.29%	5.701%
35	6.207	1605	1607	1610	rBV4	1833	1206	0.13%	0.016%
36	6.474	1686	1690	1691	rBV2	1308	849	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
 Data File : VV030897.D
 Acq On : 27 Apr 2023 11:11
 Operator : SY/MD
 Sample : VV0427WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK339

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.519	1701	1704	1706	rBV4	1297	565	0.06%	0.008%
38	6.728	1767	1769	1772	rVB4	1369	627	0.07%	0.008%
39	6.754	1772	1777	1780	rBV6	1266	1270	0.14%	0.017%
40	6.921	1819	1829	1845	rBV2	108190	202242	21.67%	2.728%
41	7.252	1920	1932	1954	rBV	412932	734115	78.65%	9.901%
42	7.561	2016	2028	2042	rBV	82708	150269	16.10%	2.027%
43	7.789	2097	2099	2103	rVB3	1350	700	0.07%	0.009%
44	7.889	2125	2130	2133	rBV6	1535	1433	0.15%	0.019%
45	8.034	2166	2175	2207	rBV	194957	401381	43.00%	5.414%
46	8.606	2350	2353	2359	rBV7	1464	1325	0.14%	0.018%
47	8.793	2398	2411	2438	rBV	456378	769855	82.48%	10.383%
48	9.005	2475	2477	2480	rBV3	1183	525	0.06%	0.007%
49	9.076	2495	2499	2501	rBV5	1152	935	0.10%	0.013%
50	9.256	2552	2555	2558	rBV4	1207	667	0.07%	0.009%
51	9.400	2596	2600	2603	rBV4	780	605	0.06%	0.008%
52	9.587	2654	2658	2662	rVB3	1031	963	0.10%	0.013%
53	9.619	2666	2668	2670	rVV3	849	555	0.06%	0.007%
54	9.735	2702	2704	2708	rBV5	1172	799	0.09%	0.011%
55	9.786	2716	2720	2723	rVB6	1516	1084	0.12%	0.015%
56	9.873	2744	2747	2754	rBV6	1582	2026	0.22%	0.027%
57	9.973	2775	2778	2780	rBV3	947	614	0.07%	0.008%
58	10.159	2821	2836	2857	rBV	281964	453192	48.55%	6.112%
59	10.493	2932	2940	2943	rBV10	1411	1849	0.20%	0.025%
60	10.580	2962	2967	2968	rBV3	1168	693	0.07%	0.009%
61	10.603	2972	2974	2979	rVV5	861	585	0.06%	0.008%
62	10.706	3000	3006	3011	rVB10	1014	1235	0.13%	0.017%
63	10.815	3038	3040	3043	rVB3	1035	517	0.06%	0.007%
64	10.860	3046	3054	3059	rBV10	1689	2751	0.29%	0.037%
65	10.956	3081	3084	3086	rBV4	1358	833	0.09%	0.011%
66	10.989	3092	3094	3098	rVV4	783	571	0.06%	0.008%
67	11.075	3118	3121	3122	rBV2	1235	589	0.06%	0.008%
68	11.114	3131	3133	3135	rBV2	928	542	0.06%	0.007%
69	11.127	3135	3137	3143	rVB6	2182	1687	0.18%	0.023%
70	11.194	3146	3158	3177	rBV	463546	748432	80.18%	10.094%
71	11.326	3197	3199	3204	rBV4	1258	1176	0.13%	0.016%
72	11.452	3235	3238	3239	rBV3	909	544	0.06%	0.007%
73	11.468	3241	3243	3246	rVB3	1446	725	0.08%	0.010%
74	11.510	3252	3256	3260	rBV6	1006	809	0.09%	0.011%
75	11.567	3262	3274	3290	rBV	444257	704256	75.45%	9.499%
76	11.976	3398	3401	3403	rBV2	1001	667	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
 Data File : VV030897.D
 Acq On : 27 Apr 2023 11:11
 Operator : SY/MD
 Sample : VV0427WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK339

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.008	3408	3411	3413	rVV4	860	588	0.06%	0.008%
78	12.030	3417	3418	3425	rBV6	1282	1246	0.13%	0.017%
79	12.075	3429	3432	3435	rVV3	734	528	0.06%	0.007%
80	12.268	3488	3492	3494	rVB4	903	670	0.07%	0.009%
81	12.419	3537	3539	3543	rVV4	1302	995	0.11%	0.013%
82	12.484	3554	3559	3564	rVB6	1767	1327	0.14%	0.018%
83	12.558	3578	3582	3587	rVB6	1570	1636	0.18%	0.022%
84	12.596	3587	3594	3601	rBV6	2904	4872	0.52%	0.066%
85	12.709	3625	3629	3631	rBV4	786	581	0.06%	0.008%
86	12.947	3699	3703	3707	rBV4	1403	1139	0.12%	0.015%
87	13.050	3731	3735	3736	rBV3	1281	893	0.10%	0.012%
88	13.149	3762	3766	3769	rVB5	1054	837	0.09%	0.011%
89	13.210	3778	3785	3796	rVV5	4845	7183	0.77%	0.097%
90	13.326	3816	3821	3822	rBV2	1162	826	0.09%	0.011%
91	13.529	3880	3884	3886	rVB5	1002	714	0.08%	0.010%
92	13.689	3926	3934	3941	rBV10	4542	7948	0.85%	0.107%
93	13.735	3946	3948	3952	rBV5	971	639	0.07%	0.009%
94	13.786	3961	3964	3965	rBV3	1497	700	0.07%	0.009%
95	13.815	3971	3973	3975	rBV3	1114	590	0.06%	0.008%
96	13.960	4016	4018	4021	rBV3	805	563	0.06%	0.008%
97	14.201	4090	4093	4095	rBV3	1104	893	0.10%	0.012%
98	14.310	4125	4127	4129	rBV3	1114	669	0.07%	0.009%
99	14.625	4223	4225	4229	rVB5	1375	722	0.08%	0.010%
100	14.853	4294	4296	4300	rBV5	984	818	0.09%	0.011%




Sum of corrected areas: 7414276

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
Data File : VV030897.D
Acq On : 27 Apr 2023 11:11
Operator : SY/MD
Sample : VV0427WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK339

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

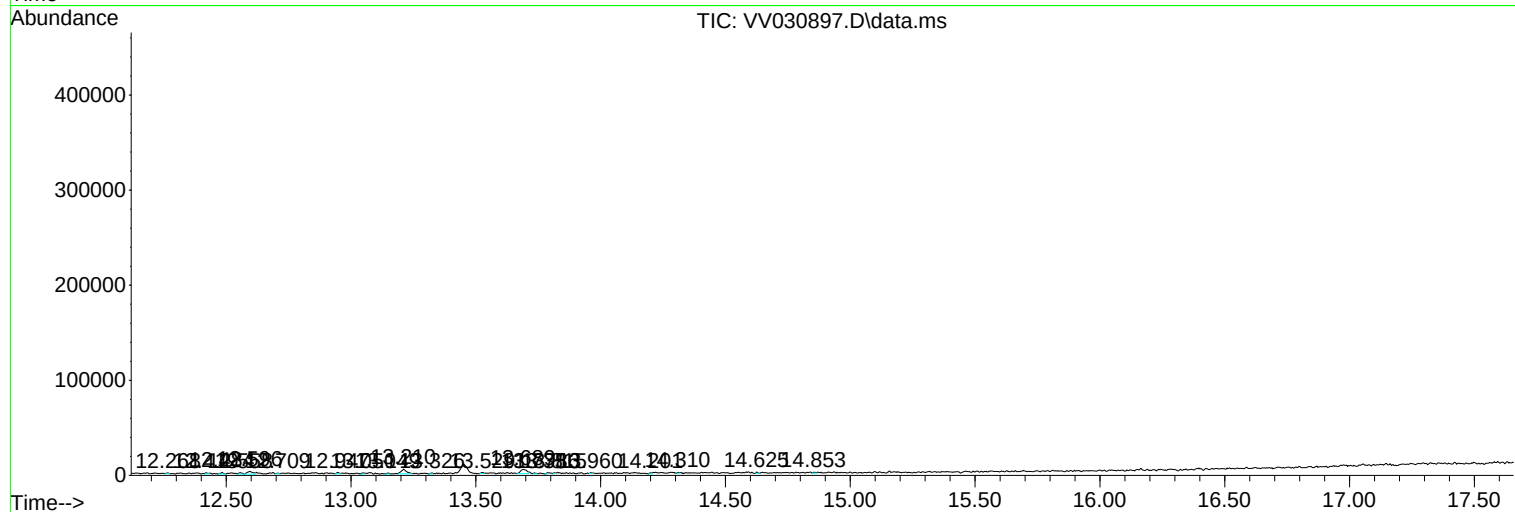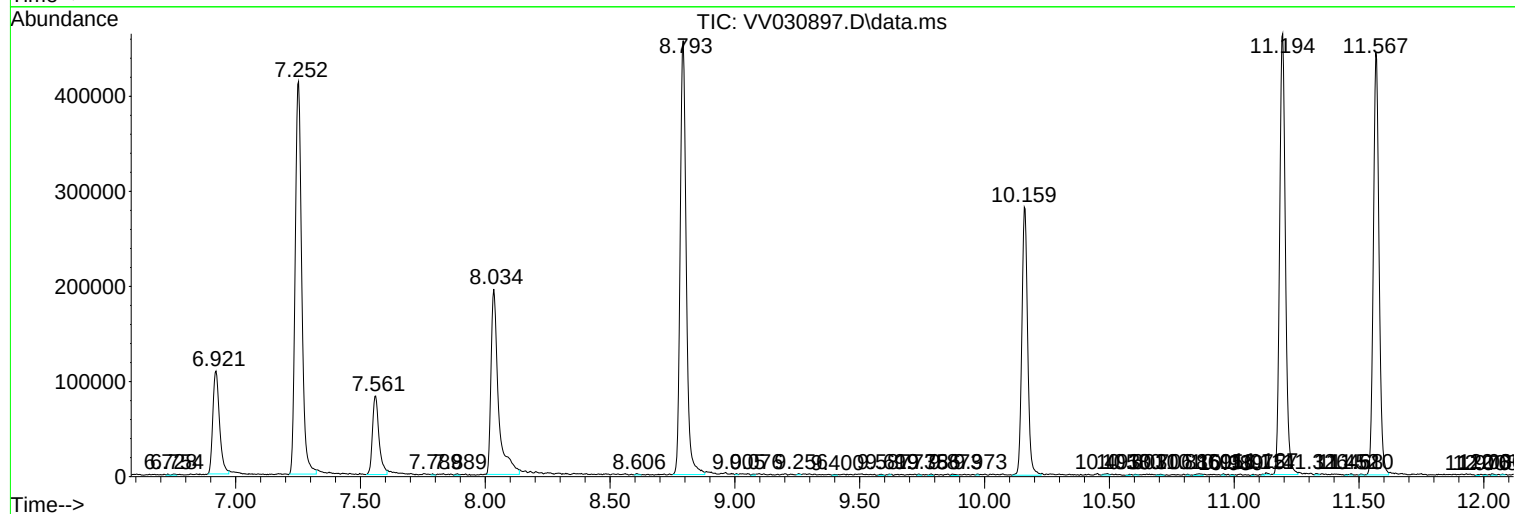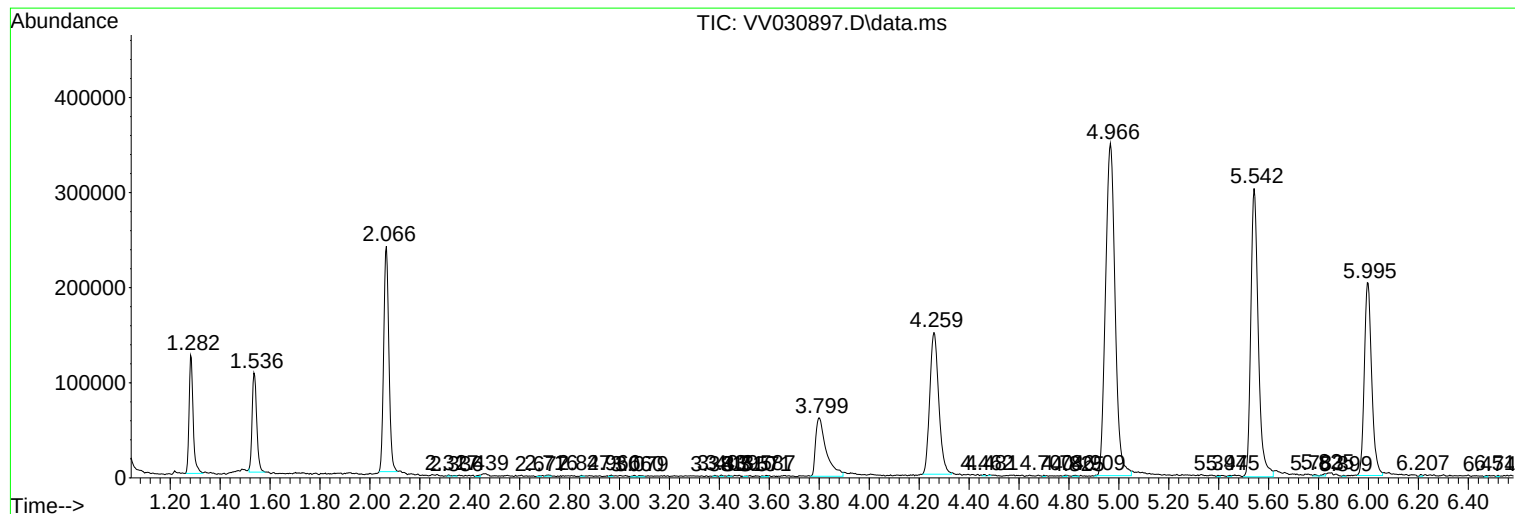

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
Data File : VV030897.D
Acq On : 27 Apr 2023 11:11
Operator : SY/MD
Sample : VV0427WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK339

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
Data File : VV030897.D
Acq On : 27 Apr 2023 11:11
Operator : SY/MD
Sample : VV0427WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK339

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------