

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
 Data File : VV030898.D
 Acq On : 27 Apr 2023 11:35
 Operator : SY/MD
 Sample : 02475-06DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030898.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	94	rVB	125875	144355	15.24%	1.866%
2	1.539	148	155	169	rVB	110195	135375	14.30%	1.750%
3	2.066	310	319	332	rBV	245969	353670	37.35%	4.573%
4	2.227	366	369	371	rBV4	1337	1123	0.12%	0.015%
5	2.339	402	404	406	rBV3	1109	428	0.05%	0.006%
6	2.439	432	435	436	rBV3	1785	1111	0.12%	0.014%
7	2.612	486	489	491	rBV3	763	641	0.07%	0.008%
8	2.780	538	541	542	rBV3	1032	534	0.06%	0.007%
9	2.799	546	547	551	rVB4	661	339	0.04%	0.004%
10	2.876	570	571	574	rBV2	834	429	0.05%	0.006%
11	3.002	606	610	612	rBV4	974	761	0.08%	0.010%
12	3.085	634	636	638	rBV2	797	351	0.04%	0.005%
13	3.095	638	639	642	rVV3	623	302	0.03%	0.004%
14	3.117	643	646	647	rVV	886	517	0.05%	0.007%
15	3.140	650	653	655	rBV4	852	685	0.07%	0.009%
16	3.243	683	685	687	rBV	519	310	0.03%	0.004%
17	3.275	692	695	697	rBV3	1041	710	0.07%	0.009%
18	3.375	723	726	728	rVB4	1022	552	0.06%	0.007%
19	3.465	751	754	755	rBV3	598	238	0.03%	0.003%
20	3.474	755	757	760	rVV3	1173	560	0.06%	0.007%
21	3.522	770	772	774	rBV2	1019	492	0.05%	0.006%
22	3.606	796	798	801	rVB3	759	350	0.04%	0.005%
23	3.693	823	825	826	rBV	1227	451	0.05%	0.006%
24	3.799	848	858	884	rBV	61292	183419	19.37%	2.371%
25	4.120	957	958	961	rBV3	783	365	0.04%	0.005%
26	4.259	987	1001	1026	rBV	154365	389164	41.09%	5.032%
27	4.966	1204	1221	1244	rBV2	358251	946994	100.00%	12.244%
28	5.484	1380	1382	1385	rBV4	1067	589	0.06%	0.008%
29	5.542	1387	1400	1425	rBV	283503	592320	62.55%	7.658%
30	5.841	1480	1493	1514	rBV	193742	397469	41.97%	5.139%
31	5.998	1529	1542	1563	rBV	212902	432392	45.66%	5.590%
32	6.214	1605	1609	1611	rBV5	1411	1057	0.11%	0.014%
33	6.551	1712	1714	1716	rVB3	778	313	0.03%	0.004%
34	6.754	1775	1777	1781	rVB4	1196	687	0.07%	0.009%
35	6.783	1784	1786	1789	rBV3	1147	626	0.07%	0.008%
36	6.847	1803	1806	1810	rVB5	1436	1028	0.11%	0.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042723\
 Data File : VW030898.D
 Acq On : 27 Apr 2023 11:35
 Operator : SY/MD
 Sample : 02475-06DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.873	1810	1814	1815	rBV4	1291	807	0.09%	0.010%
38	6.921	1819	1829	1845	rVV	111874	204331	21.58%	2.642%
39	7.252	1920	1932	1951	rBV	419091	735449	77.66%	9.509%
40	7.561	2018	2028	2051	rBV	80093	147098	15.53%	1.902%
41	7.953	2144	2150	2152	rBV6	1022	910	0.10%	0.012%
42	7.972	2152	2156	2159	rBV4	1284	933	0.10%	0.012%
43	8.034	2166	2175	2208	rBV	195207	397721	42.00%	5.142%
44	8.712	2383	2386	2388	rBV4	766	570	0.06%	0.007%
45	8.792	2399	2411	2434	rBV	434810	724703	76.53%	9.370%
46	9.111	2508	2510	2513	rBV3	831	456	0.05%	0.006%
47	9.210	2539	2541	2543	rBV3	1625	779	0.08%	0.010%
48	9.249	2551	2553	2556	rBV3	1403	885	0.09%	0.011%
49	9.262	2556	2557	2559	rVV	1013	408	0.04%	0.005%
50	9.291	2563	2566	2568	rBV3	1005	591	0.06%	0.008%
51	9.403	2597	2601	2603	rBV3	950	664	0.07%	0.009%
52	9.490	2622	2628	2629	rBV4	1109	1095	0.12%	0.014%
53	9.654	2673	2679	2682	rBV6	1294	1342	0.14%	0.017%
54	9.683	2686	2688	2690	rBV2	773	422	0.04%	0.005%
55	9.754	2705	2710	2712	rBV5	1189	1125	0.12%	0.015%
56	9.937	2765	2767	2769	rBV3	865	364	0.04%	0.005%
57	10.017	2790	2792	2793	rBV2	771	247	0.03%	0.003%
58	10.159	2825	2836	2857	rBV	286895	458044	48.37%	5.922%
59	10.258	2864	2867	2870	rVB4	935	643	0.07%	0.008%
60	10.406	2911	2913	2914	rBV	753	308	0.03%	0.004%
61	10.455	2925	2928	2932	rVB4	1290	995	0.11%	0.013%
62	10.480	2932	2936	2937	rBV3	1190	911	0.10%	0.012%
63	10.551	2956	2958	2960	rBV2	881	434	0.05%	0.006%
64	10.750	3016	3020	3025	rBV6	1212	1365	0.14%	0.018%
65	10.908	3063	3069	3073	rBV7	2151	2335	0.25%	0.030%
66	10.940	3077	3079	3081	rBV3	752	373	0.04%	0.005%
67	11.062	3115	3117	3120	rBV4	930	471	0.05%	0.006%
68	11.101	3121	3129	3137	rBV10	10077	18310	1.93%	0.237%
69	11.194	3147	3158	3180	rBV	429368	697485	73.65%	9.018%
70	11.381	3214	3216	3219	rBV3	900	396	0.04%	0.005%
71	11.487	3248	3249	3254	rVB5	1116	656	0.07%	0.008%
72	11.512	3254	3257	3259	rBV3	966	654	0.07%	0.008%
73	11.567	3262	3274	3295	rVV	444059	706789	74.64%	9.138%
74	11.850	3360	3362	3363	rBV2	1239	597	0.06%	0.008%
75	12.062	3426	3428	3430	rBV3	914	583	0.06%	0.008%
76	12.117	3444	3445	3449	rVB4	944	499	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
 Data File : VV030898.D
 Acq On : 27 Apr 2023 11:35
 Operator : SY/MD
 Sample : 02475-06DL 5X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW8DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.139	3449	3452	3453	rBV2	1150	543	0.06%	0.007%
78	12.175	3461	3463	3467	rVB5	1175	829	0.09%	0.011%
79	12.242	3482	3484	3487	rBV4	891	645	0.07%	0.008%
80	12.300	3495	3502	3511	rBV9	7801	13015	1.37%	0.168%
81	12.442	3544	3546	3548	rBV3	865	356	0.04%	0.005%
82	12.464	3548	3553	3555	rVB3	911	744	0.08%	0.010%
83	12.512	3565	3568	3570	rBV3	901	586	0.06%	0.008%
84	12.590	3586	3592	3595	rBV7	1995	2464	0.26%	0.032%
85	12.754	3642	3643	3647	rVB3	882	516	0.05%	0.007%
86	12.786	3651	3653	3655	rBV3	1158	708	0.07%	0.009%
87	12.831	3665	3667	3668	rBV2	751	251	0.03%	0.003%
88	13.001	3715	3720	3721	rBV5	997	794	0.08%	0.010%
89	13.056	3733	3737	3740	rVB6	1317	1003	0.11%	0.013%
90	13.123	3755	3758	3760	rBV4	1076	790	0.08%	0.010%
91	13.307	3813	3815	3817	rBV3	824	562	0.06%	0.007%
92	13.416	3847	3849	3852	rBV4	1226	736	0.08%	0.010%
93	13.535	3884	3886	3889	rBV4	900	670	0.07%	0.009%
94	13.583	3899	3901	3904	rVB4	1283	736	0.08%	0.010%
95	13.770	3956	3959	3963	rBV5	1713	1687	0.18%	0.022%
96	13.799	3966	3968	3971	rVB4	1253	659	0.07%	0.009%
97	13.856	3984	3986	3987	rBV	762	339	0.04%	0.004%
98	13.918	4003	4005	4008	rVB4	1186	797	0.08%	0.010%
99	13.988	4024	4027	4029	rBV4	1170	673	0.07%	0.009%
100	14.522	4190	4193	4195	rBV3	1280	870	0.09%	0.011%




Sum of corrected areas: 7734428

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
Data File : VV030898.D
Acq On : 27 Apr 2023 11:35
Operator : SY/MD
Sample : 02475-06DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

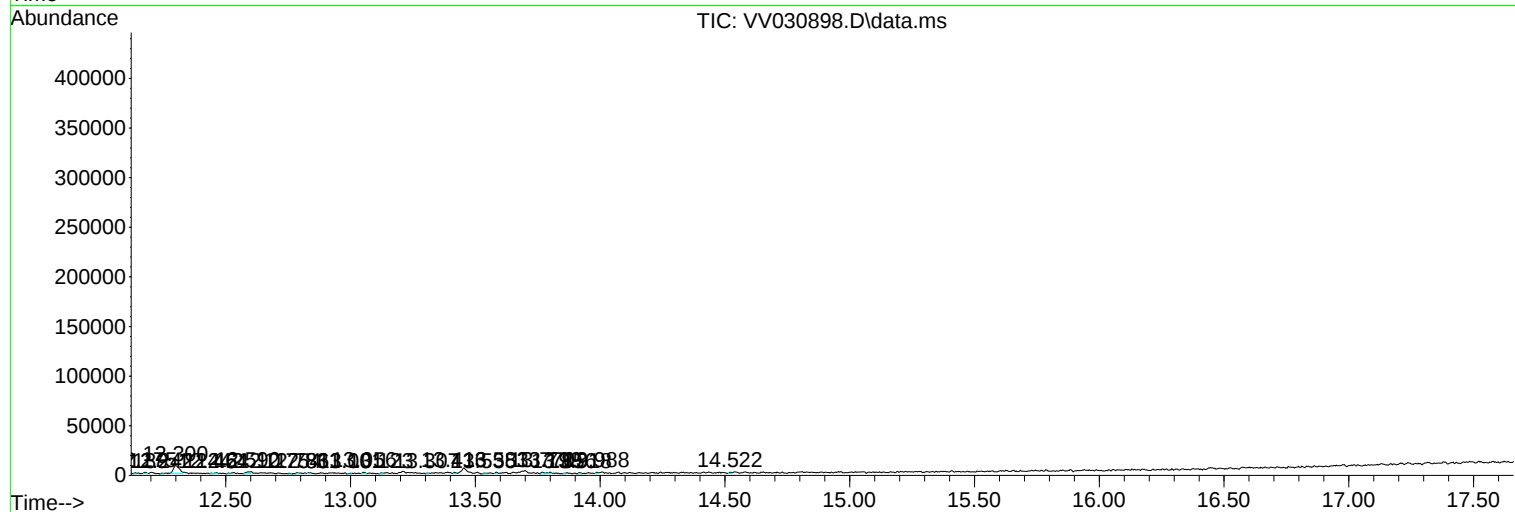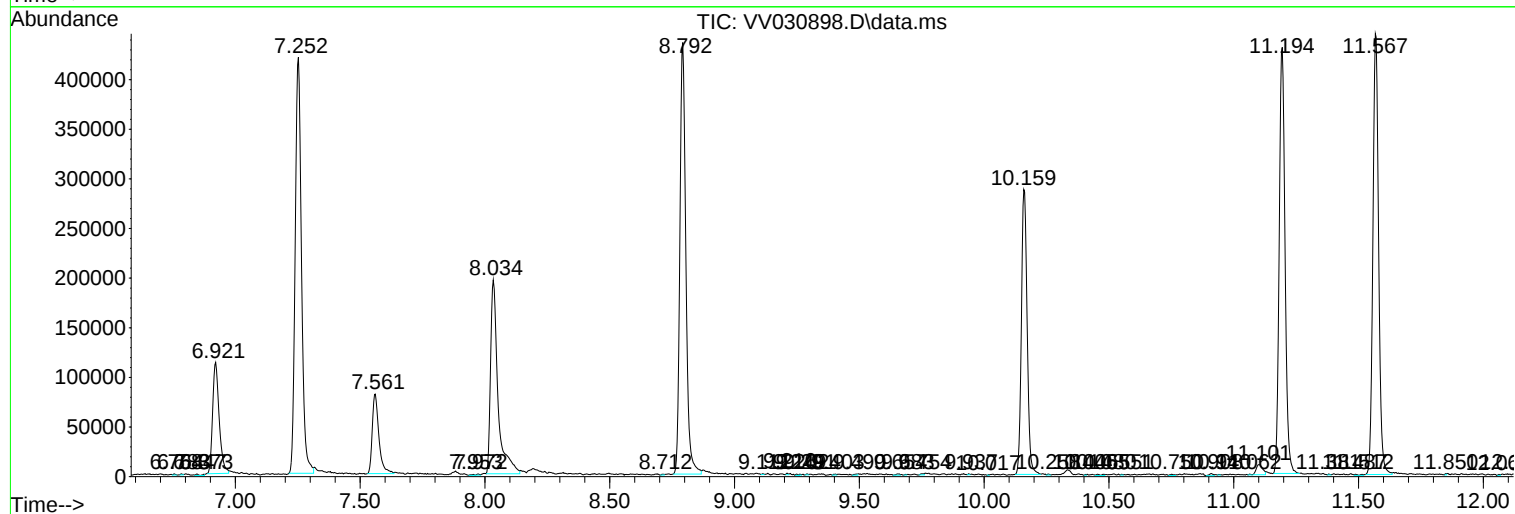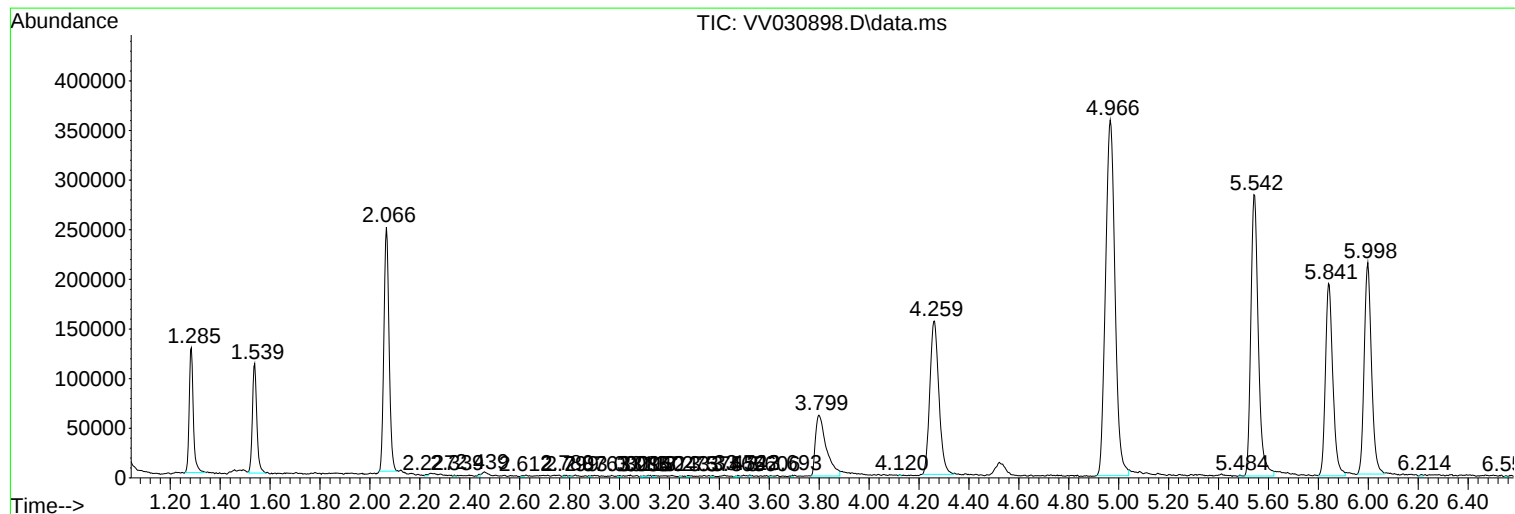

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
Data File : VV030898.D
Acq On : 27 Apr 2023 11:35
Operator : SY/MD
Sample : 02475-06DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
Data File : VV030898.D
Acq On : 27 Apr 2023 11:35
Operator : SY/MD
Sample : 02475-06DL 5X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------