

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
 Data File : VV030899.D
 Acq On : 27 Apr 2023 11:59
 Operator : SY/MD
 Sample : 02475-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030899.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.285	69	76	94	rVB	133746	152077	15.30%	1.981%
2	1.539	148	155	167	rVB	114044	137755	13.86%	1.795%
3	2.066	308	319	332	rBV	257661	378681	38.11%	4.934%
4	2.590	479	482	484	rBV3	874	522	0.05%	0.007%
5	2.664	504	505	507	rBV2	822	443	0.04%	0.006%
6	2.770	534	538	543	rVB4	1676	1474	0.15%	0.019%
7	2.796	543	546	548	rBV4	787	312	0.03%	0.004%
8	2.809	548	550	553	rBV2	782	501	0.05%	0.007%
9	2.982	603	604	606	rVB2	570	155	0.02%	0.002%
10	3.008	606	612	614	rBV5	1662	1514	0.15%	0.020%
11	3.060	626	628	629	rBV3	602	234	0.02%	0.003%
12	3.182	664	666	669	rBV3	1487	741	0.07%	0.010%
13	3.240	681	684	687	rBV4	916	544	0.05%	0.007%
14	3.269	689	693	694	rBV4	862	614	0.06%	0.008%
15	3.394	729	732	734	rBV4	1366	1068	0.11%	0.014%
16	3.503	762	766	770	rVB6	1550	1412	0.14%	0.018%
17	3.532	770	775	776	rBV3	804	670	0.07%	0.009%
18	3.542	776	778	780	rBV3	1532	599	0.06%	0.008%
19	3.568	785	786	790	rBV4	708	473	0.05%	0.006%
20	3.632	804	806	807	rBV3	808	221	0.02%	0.003%
21	3.661	813	815	820	rVB4	1097	658	0.07%	0.009%
22	3.683	820	822	823	rBV2	738	185	0.02%	0.002%
23	3.751	841	843	844	rBV	953	486	0.05%	0.006%
24	3.760	844	846	848	rVV3	1097	521	0.05%	0.007%
25	3.799	848	858	883	rVV	61820	179478	18.06%	2.338%
26	4.130	955	961	966	rVB7	1350	1798	0.18%	0.023%
27	4.162	966	971	973	rBV5	1621	1343	0.14%	0.017%
28	4.259	987	1001	1023	rBV2	158536	400697	40.32%	5.220%
29	4.641	1118	1120	1121	rBV	998	346	0.03%	0.005%
30	4.773	1159	1161	1164	rBV4	976	598	0.06%	0.008%
31	4.966	1203	1221	1248	rBV2	370766	993782	100.00%	12.947%
32	5.375	1346	1348	1351	rBV3	865	562	0.06%	0.007%
33	5.542	1388	1400	1427	rBV	292329	609223	61.30%	7.937%
34	5.998	1530	1542	1564	rBV	214007	442250	44.50%	5.762%
35	6.358	1650	1654	1655	rBV4	1128	752	0.08%	0.010%
36	6.403	1665	1668	1672	rBV5	997	796	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
 Data File : VV030899.D
 Acq On : 27 Apr 2023 11:59
 Operator : SY/MD
 Sample : 02475-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	6.465	1685	1687	1689	rBV3	833	377	0.04%	0.005%
38	6.487	1693	1694	1696	rBV2	1074	434	0.04%	0.006%
39	6.584	1722	1724	1727	rVB3	882	402	0.04%	0.005%
40	6.600	1727	1729	1730	rBV	1113	540	0.05%	0.007%
41	6.805	1789	1793	1795	rBV4	827	630	0.06%	0.008%
42	6.854	1807	1808	1811	rBV3	884	596	0.06%	0.008%
43	6.921	1818	1829	1851	rBV	115720	219141	22.05%	2.855%
44	7.252	1918	1932	1955	rBV	436840	787537	79.25%	10.260%
45	7.558	2018	2027	2050	rBV	86659	157586	15.86%	2.053%
46	8.034	2165	2175	2210	rBV	200480	413610	41.62%	5.389%
47	8.792	2400	2411	2435	rBV	448309	751790	75.65%	9.794%
48	9.114	2509	2511	2515	rVB5	1260	747	0.08%	0.010%
49	9.204	2537	2539	2543	rBV5	932	624	0.06%	0.008%
50	9.236	2546	2549	2552	rBV5	1635	1470	0.15%	0.019%
51	9.551	2645	2647	2648	rBV2	425	96	0.01%	0.001%
52	9.564	2648	2651	2652	rBV3	879	519	0.05%	0.007%
53	9.590	2656	2659	2663	rBV5	1609	1249	0.13%	0.016%
54	9.628	2669	2671	2675	rVB4	1336	842	0.08%	0.011%
55	9.648	2675	2677	2682	rBV4	1059	1063	0.11%	0.014%
56	9.889	2749	2752	2754	rVB3	998	459	0.05%	0.006%
57	10.072	2805	2809	2810	rBV3	2014	1118	0.11%	0.015%
58	10.159	2825	2836	2853	rBV	293454	470483	47.34%	6.130%
59	10.278	2870	2873	2876	rVB3	1353	766	0.08%	0.010%
60	10.297	2876	2879	2880	rBV3	782	489	0.05%	0.006%
61	10.333	2880	2890	2902	rVB	34260	57979	5.83%	0.755%
62	10.397	2907	2910	2912	rBV3	851	536	0.05%	0.007%
63	10.461	2928	2930	2933	rBV3	1234	734	0.07%	0.010%
64	10.474	2933	2934	2937	rVV3	583	334	0.03%	0.004%
65	10.522	2946	2949	2950	rBV3	925	493	0.05%	0.006%
66	10.625	2979	2981	2985	rBV4	643	515	0.05%	0.007%
67	10.667	2992	2994	2996	rBV3	1010	703	0.07%	0.009%
68	10.786	3027	3031	3032	rBV2	1057	783	0.08%	0.010%
69	10.844	3045	3049	3052	rBV5	1221	985	0.10%	0.013%
70	10.937	3075	3078	3081	rBV4	1003	821	0.08%	0.011%
71	11.088	3122	3125	3126	rBV3	1200	626	0.06%	0.008%
72	11.194	3147	3158	3180	rVB	448269	714717	71.92%	9.311%
73	11.410	3223	3225	3229	rVB3	1090	599	0.06%	0.008%
74	11.455	3236	3239	3242	rBV5	1264	902	0.09%	0.012%
75	11.567	3261	3274	3289	rBV	462690	741666	74.63%	9.663%
76	11.824	3351	3354	3358	rBV4	1225	775	0.08%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
 Data File : VV030899.D
 Acq On : 27 Apr 2023 11:59
 Operator : SY/MD
 Sample : 02475-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.879	3368	3371	3375	rVB5	1183	939	0.09%	0.012%
78	11.902	3375	3378	3380	rBV3	833	453	0.05%	0.006%
79	11.960	3392	3396	3397	rBV4	970	670	0.07%	0.009%
80	12.021	3413	3415	3417	rBV3	997	595	0.06%	0.008%
81	12.062	3426	3428	3430	rBV3	1396	824	0.08%	0.011%
82	12.130	3447	3449	3453	rBV3	912	721	0.07%	0.009%
83	12.207	3463	3473	3479	rBV2	8258	14669	1.48%	0.191%
84	12.271	3491	3493	3494	rBV	935	437	0.04%	0.006%
85	12.297	3499	3501	3504	rBV3	1416	947	0.10%	0.012%
86	12.432	3541	3543	3545	rBV3	563	281	0.03%	0.004%
87	12.464	3551	3553	3556	rBV3	773	417	0.04%	0.005%
88	12.586	3589	3591	3594	rBV3	1109	739	0.07%	0.010%
89	12.693	3619	3624	3626	rVB6	1270	993	0.10%	0.013%
90	12.715	3629	3631	3635	rBV4	1174	796	0.08%	0.010%
91	13.271	3801	3804	3806	rBV3	874	660	0.07%	0.009%
92	13.320	3817	3819	3821	rBV2	899	512	0.05%	0.007%
93	13.503	3875	3876	3880	rVB5	824	519	0.05%	0.007%
94	13.612	3907	3910	3911	rBV4	867	526	0.05%	0.007%
95	14.339	4134	4136	4141	rBV6	903	722	0.07%	0.009%




Sum of corrected areas: 7675641

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
Data File : VV030899.D
Acq On : 27 Apr 2023 11:59
Operator : SY/MD
Sample : 02475-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

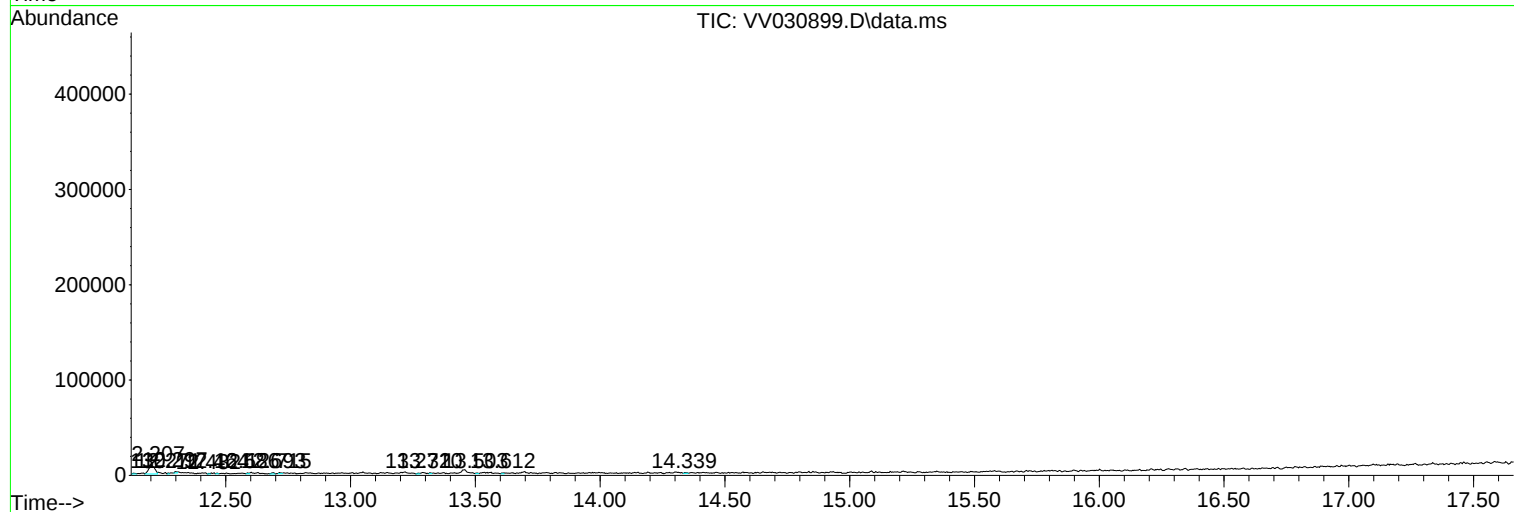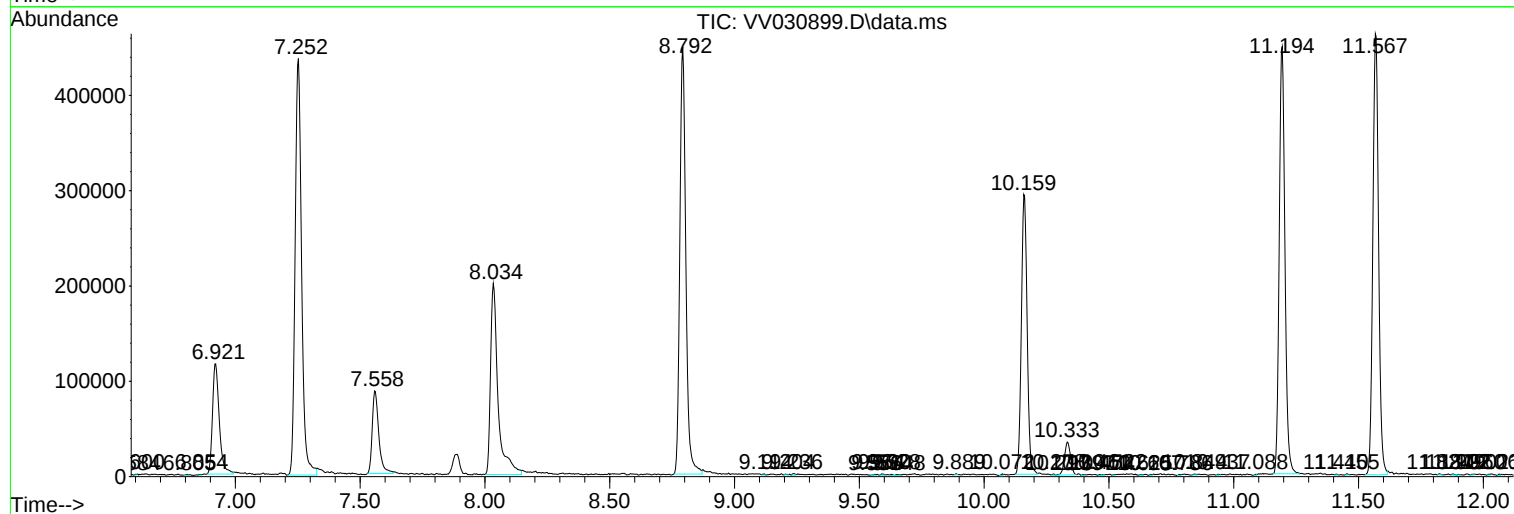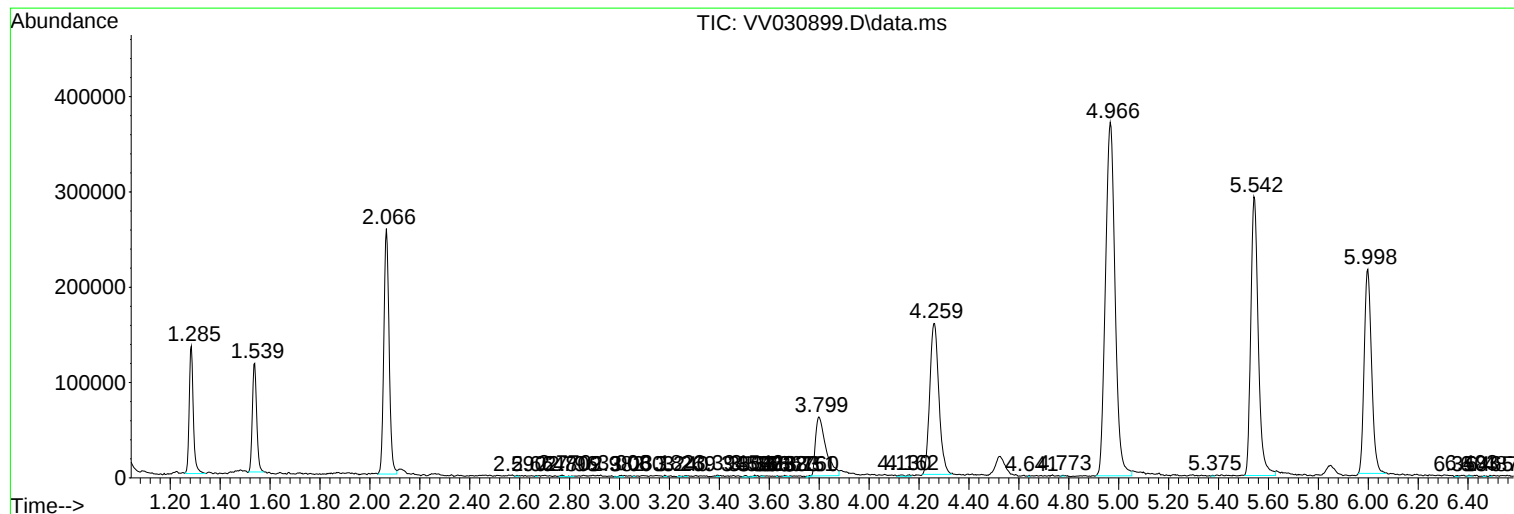

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
Data File : VV030899.D
Acq On : 27 Apr 2023 11:59
Operator : SY/MD
Sample : 02475-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
Data File : VV030899.D
Acq On : 27 Apr 2023 11:59
Operator : SY/MD
Sample : 02475-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------