

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
 Data File : VV030900.D
 Acq On : 27 Apr 2023 12:25
 Operator : SY/MD
 Sample : 02475-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030900.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	67	75	89	rVB	125984	151302	7.51%	1.614%
2	1.536	148	154	170	rVB	112377	135593	6.73%	1.446%
3	2.066	310	319	333	rBV	237575	349420	17.34%	3.727%
4	2.516	456	459	462	rVV4	946	648	0.03%	0.007%
5	2.558	470	472	475	rBV4	1237	785	0.04%	0.008%
6	2.584	477	480	482	rVV4	1001	560	0.03%	0.006%
7	2.748	528	531	533	rBV4	960	611	0.03%	0.007%
8	3.028	616	618	622	rBV4	1495	821	0.04%	0.009%
9	3.188	664	668	671	rBV5	627	616	0.03%	0.007%
10	3.214	673	676	680	rBV5	833	611	0.03%	0.007%
11	3.362	720	722	725	rVB5	1271	564	0.03%	0.006%
12	3.478	756	758	765	rVB7	905	769	0.04%	0.008%
13	3.523	768	772	774	rBV4	1177	950	0.05%	0.010%
14	3.593	790	794	797	rBV4	886	662	0.03%	0.007%
15	3.626	801	804	807	rVB4	1239	775	0.04%	0.008%
16	3.661	813	815	818	rBV3	784	537	0.03%	0.006%
17	3.709	828	830	832	rVB3	1260	579	0.03%	0.006%
18	3.738	832	839	846	rBV9	1340	2138	0.11%	0.023%
19	3.799	847	858	886	rBV	57645	190983	9.48%	2.037%
20	4.101	950	952	954	rBV3	1331	664	0.03%	0.007%
21	4.150	965	967	971	rVB4	1498	764	0.04%	0.008%
22	4.259	987	1001	1023	rBV	146229	365086	18.12%	3.894%
23	4.687	1131	1134	1135	rBV3	1072	647	0.03%	0.007%
24	4.745	1148	1152	1153	rBV4	1203	768	0.04%	0.008%
25	4.844	1180	1183	1184	rBV2	867	555	0.03%	0.006%
26	4.966	1202	1221	1253	rBV2	339034	917062	45.51%	9.782%
27	5.288	1318	1321	1323	rBV3	1068	669	0.03%	0.007%
28	5.542	1388	1400	1428	rBV	294532	611983	30.37%	6.528%
29	5.838	1479	1492	1515	rBV	1031557	2015240	100.00%	21.497%
30	5.995	1531	1541	1562	rVB	205409	406204	20.16%	4.333%
31	6.400	1662	1667	1668	rBV5	1002	702	0.03%	0.007%
32	6.455	1682	1684	1688	rBV4	1424	832	0.04%	0.009%
33	6.754	1775	1777	1780	rBV2	1158	774	0.04%	0.008%
34	6.918	1816	1828	1846	rBV	108350	206241	10.23%	2.200%
35	7.111	1886	1888	1892	rVB4	1615	973	0.05%	0.010%
36	7.249	1920	1931	1953	rBV	400751	712388	35.35%	7.599%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW042723\
 Data File : VW030900.D
 Acq On : 27 Apr 2023 12:25
 Operator : SY/MD
 Sample : 02475-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	7.558	2017	2027	2053	rBV	78743	149737	7.43%	1.597%
38	7.825	2107	2110	2112	rBV4	1054	712	0.04%	0.008%
39	7.883	2120	2128	2139	rBV2	10157	18282	0.91%	0.195%
40	8.034	2165	2175	2190	rBV	178301	336736	16.71%	3.592%
41	8.548	2332	2335	2337	rBV3	1285	665	0.03%	0.007%
42	8.619	2354	2357	2360	rBV5	1262	943	0.05%	0.010%
43	8.793	2399	2411	2434	rBV	453936	765771	38.00%	8.168%
44	8.992	2471	2473	2477	rVB4	1644	962	0.05%	0.010%
45	9.159	2521	2525	2530	rVB5	1387	1115	0.06%	0.012%
46	9.326	2575	2577	2581	rBV4	799	555	0.03%	0.006%
47	9.487	2624	2627	2630	rVV6	1036	865	0.04%	0.009%
48	9.529	2636	2640	2644	rVV5	1226	1078	0.05%	0.011%
49	9.558	2646	2649	2653	rVB4	1227	1097	0.05%	0.012%
50	9.596	2658	2661	2664	rBV5	1083	908	0.05%	0.010%
51	9.667	2681	2683	2687	rVB4	1314	714	0.04%	0.008%
52	9.719	2695	2699	2706	rVB8	1366	1501	0.07%	0.016%
53	9.767	2706	2714	2717	rBV8	3017	2904	0.14%	0.031%
54	9.809	2724	2727	2730	rBV4	1169	1055	0.05%	0.011%
55	10.002	2783	2787	2789	rBV4	1530	978	0.05%	0.010%
56	10.159	2825	2836	2856	rVV	268801	436478	21.66%	4.656%
57	10.249	2862	2864	2867	rBV4	886	608	0.03%	0.006%
58	10.297	2873	2879	2881	rBV6	1540	1466	0.07%	0.016%
59	10.333	2881	2890	2904	rVV	19884	33024	1.64%	0.352%
60	10.465	2929	2931	2937	rVB5	928	856	0.04%	0.009%
61	10.500	2937	2942	2943	rBV4	933	654	0.03%	0.007%
62	10.529	2948	2951	2954	rBV4	1006	663	0.03%	0.007%
63	10.593	2969	2971	2974	rVV3	1043	554	0.03%	0.006%
64	10.638	2983	2985	2989	rVB4	1053	625	0.03%	0.007%
65	10.757	3017	3022	3024	rBV4	1101	1018	0.05%	0.011%
66	10.789	3027	3032	3037	rVV8	1630	1343	0.07%	0.014%
67	10.809	3037	3038	3042	rVV4	998	744	0.04%	0.008%
68	10.854	3050	3052	3056	rVB5	904	545	0.03%	0.006%
69	11.101	3121	3129	3137	rBV7	14221	22264	1.10%	0.237%
70	11.194	3145	3158	3177	rBV	473453	752639	37.35%	8.028%
71	11.358	3207	3209	3213	rBV4	954	694	0.03%	0.007%
72	11.567	3261	3274	3294	rBV	441413	689611	34.22%	7.356%
73	11.715	3318	3320	3326	rBV7	1254	870	0.04%	0.009%
74	11.908	3378	3380	3384	rVB4	1320	676	0.03%	0.007%
75	11.973	3398	3400	3403	rBV5	1001	588	0.03%	0.006%
76	12.204	3466	3472	3482	rVB4	5487	9049	0.45%	0.097%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
 Data File : VV030900.D
 Acq On : 27 Apr 2023 12:25
 Operator : SY/MD
 Sample : 02475-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AW7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	12.239	3482	3483	3488	rVB3	1204	703	0.03%	0.007%
78	12.265	3488	3491	3492	rBV2	1247	746	0.04%	0.008%
79	12.297	3493	3501	3513	rVV6	18889	30916	1.53%	0.330%
80	12.413	3532	3537	3541	rBV6	1345	1430	0.07%	0.015%
81	12.558	3577	3582	3584	rBV5	1097	843	0.04%	0.009%
82	12.747	3638	3641	3646	rBV5	1408	1101	0.05%	0.012%
83	12.808	3658	3660	3663	rVB3	1707	743	0.04%	0.008%
84	12.853	3672	3674	3677	rBV4	966	547	0.03%	0.006%
85	12.899	3685	3688	3692	rBV5	1090	901	0.04%	0.010%
86	12.966	3705	3709	3711	rBV4	931	865	0.04%	0.009%
87	13.075	3739	3743	3749	rVB5	1261	1401	0.07%	0.015%
88	13.108	3749	3753	3756	rBV6	1781	1400	0.07%	0.015%
89	13.127	3756	3759	3762	rBV4	985	574	0.03%	0.006%
90	13.349	3826	3828	3830	rBV3	1139	568	0.03%	0.006%
91	13.381	3834	3838	3839	rBV3	2936	1955	0.10%	0.021%
92	13.516	3877	3880	3882	rVB2	1198	613	0.03%	0.007%
93	13.664	3924	3926	3930	rVV5	929	597	0.03%	0.006%
94	13.937	4007	4011	4014	rBV6	1452	1134	0.06%	0.012%
95	13.969	4019	4021	4023	rBV3	916	579	0.03%	0.006%
96	14.040	4040	4043	4044	rBV3	1554	915	0.05%	0.010%
97	14.156	4078	4079	4084	rBV4	1385	1168	0.06%	0.012%
98	14.204	4091	4094	4096	rBV4	1250	761	0.04%	0.008%
99	14.706	4247	4250	4253	rBV5	1526	1089	0.05%	0.012%
100	14.863	4294	4299	4301	rBV4	1633	1118	0.06%	0.012%




Sum of corrected areas: 9374690

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
Data File : VV030900.D
Acq On : 27 Apr 2023 12:25
Operator : SY/MD
Sample : 02475-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

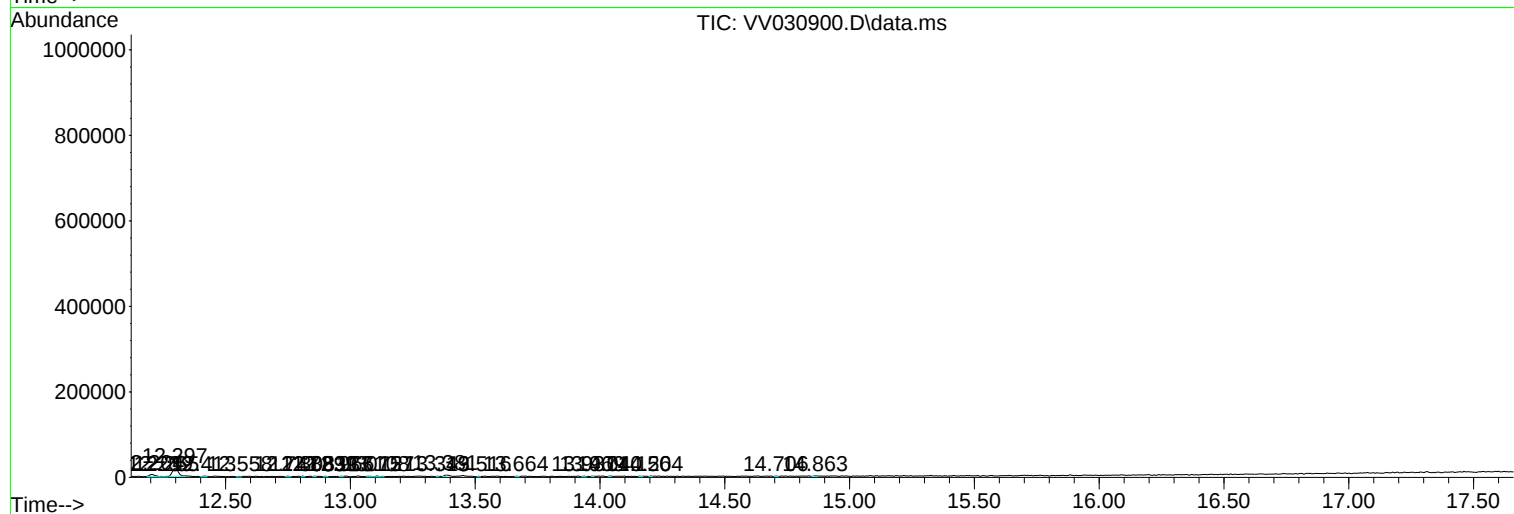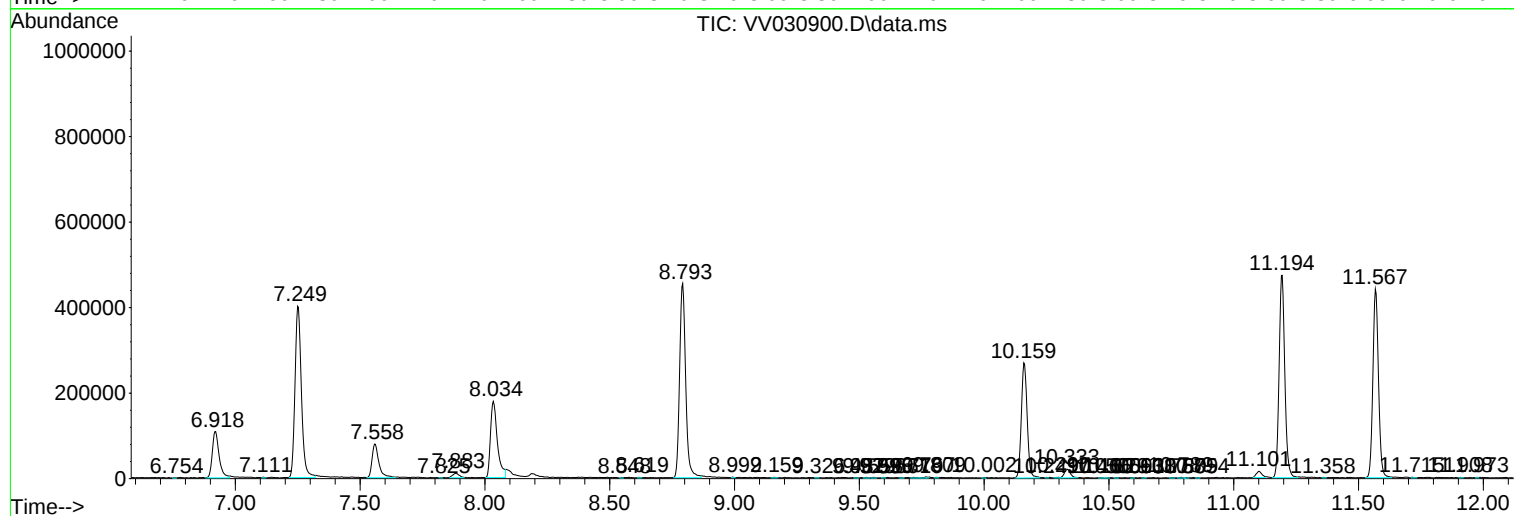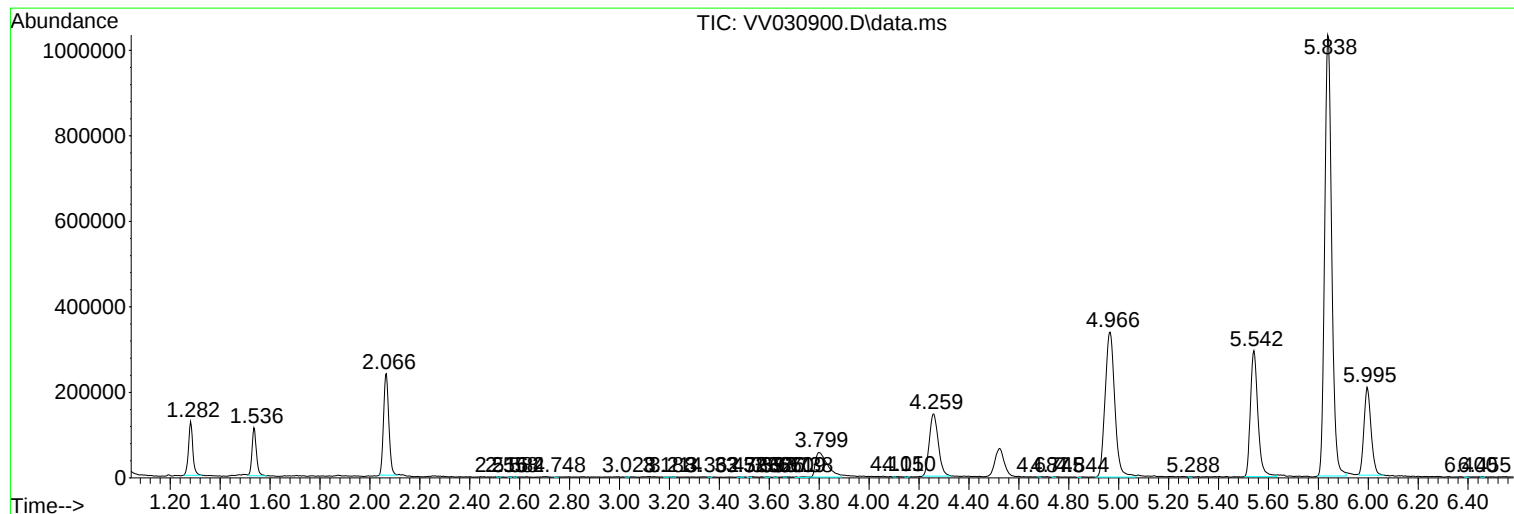

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
Data File : VV030900.D
Acq On : 27 Apr 2023 12:25
Operator : SY/MD
Sample : 02475-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
Data File : VV030900.D
Acq On : 27 Apr 2023 12:25
Operator : SY/MD
Sample : 02475-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AW7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc