

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
 Data File : VV030901.D
 Acq On : 27 Apr 2023 12:57
 Operator : SY/MD
 Sample : 02475-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

Signal : TIC: VV030901.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	89	rVB	102794	113071	13.50%	1.733%
2	1.536	147	154	169	rVB	90498	109842	13.12%	1.684%
3	2.063	309	318	332	rBV	200093	285860	34.13%	4.382%
4	2.211	362	364	366	rBV3	1205	542	0.06%	0.008%
5	2.304	390	393	394	rBV3	1192	603	0.07%	0.009%
6	2.346	404	406	409	rBV4	1007	588	0.07%	0.009%
7	2.539	464	466	468	rVB3	1155	453	0.05%	0.007%
8	2.555	468	471	474	rBV5	980	674	0.08%	0.010%
9	2.616	489	490	497	rBV4	1087	1055	0.13%	0.016%
10	2.687	508	512	514	rBV3	1226	815	0.10%	0.012%
11	2.732	523	526	528	rVB5	1024	576	0.07%	0.009%
12	2.802	545	548	551	rVB5	1280	754	0.09%	0.012%
13	2.822	551	554	558	rBV4	657	661	0.08%	0.010%
14	2.870	567	569	572	rBV4	1035	698	0.08%	0.011%
15	2.905	576	580	586	rVB7	1358	1477	0.18%	0.023%
16	3.108	641	643	645	rBV2	1182	649	0.08%	0.010%
17	3.130	648	650	656	rVB5	1420	1512	0.18%	0.023%
18	3.211	672	675	678	rBV5	1188	813	0.10%	0.012%
19	3.269	691	693	696	rBV3	966	553	0.07%	0.008%
20	3.388	728	730	733	rBV4	750	528	0.06%	0.008%
21	3.426	740	742	746	rBV4	997	689	0.08%	0.011%
22	3.449	747	749	752	rVB4	1095	627	0.07%	0.010%
23	3.468	752	755	757	rBV3	1137	817	0.10%	0.013%
24	3.481	757	759	761	rVV3	1482	597	0.07%	0.009%
25	3.600	794	796	800	rVB5	1273	975	0.12%	0.015%
26	3.632	800	806	810	rBV7	1674	1487	0.18%	0.023%
27	3.719	830	833	838	rBV6	740	790	0.09%	0.012%
28	3.764	841	847	848	rBV3	1093	1093	0.13%	0.017%
29	3.796	848	857	885	rBV	54665	154786	18.48%	2.373%
30	4.256	983	1000	1024	rBV2	136898	352454	42.08%	5.403%
31	4.625	1112	1115	1118	rBV4	1079	665	0.08%	0.010%
32	4.735	1143	1149	1152	rBV7	1011	1064	0.13%	0.016%
33	4.764	1154	1158	1159	rBV3	967	516	0.06%	0.008%
34	4.844	1180	1183	1185	rBV4	959	513	0.06%	0.008%
35	4.963	1204	1220	1249	rBV2	309865	837507	100.00%	12.839%
36	5.249	1307	1309	1316	rBV6	1397	1006	0.12%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
 Data File : VV030901.D
 Acq On : 27 Apr 2023 12:57
 Operator : SY/MD
 Sample : 02475-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

37	5.542	1387	1400	1419	rBV	252935	530099	63.29%	8.126%
38	5.995	1526	1541	1559	rBV	189101	392839	46.91%	6.022%
39	6.368	1655	1657	1662	rVB4	899	764	0.09%	0.012%
40	6.394	1662	1665	1668	rBV4	1681	1068	0.13%	0.016%
41	6.484	1690	1693	1697	rBV6	1159	812	0.10%	0.012%
42	6.545	1705	1712	1713	rBV7	1142	1088	0.13%	0.017%
43	6.648	1741	1744	1746	rVV3	1263	767	0.09%	0.012%
44	6.918	1817	1828	1846	rVV2	99833	192324	22.96%	2.948%
45	7.079	1876	1878	1881	rBV5	985	736	0.09%	0.011%
46	7.149	1897	1900	1901	rBV3	1007	612	0.07%	0.009%
47	7.182	1908	1910	1913	rBV4	1035	562	0.07%	0.009%
48	7.249	1920	1931	1953	rBV	352747	625957	74.74%	9.596%
49	7.558	2018	2027	2045	rBV	75224	133943	15.99%	2.053%
50	7.818	2106	2108	2111	rBV4	1520	952	0.11%	0.015%
51	7.838	2111	2114	2117	rVB4	1440	1014	0.12%	0.016%
52	7.857	2117	2120	2121	rBV3	1459	722	0.09%	0.011%
53	7.912	2135	2137	2139	rBV2	1355	686	0.08%	0.011%
54	8.034	2165	2175	2207	rBV	173938	364433	43.51%	5.587%
55	8.400	2287	2289	2292	rBV4	869	720	0.09%	0.011%
56	8.468	2308	2310	2312	rBV3	980	559	0.07%	0.009%
57	8.619	2355	2357	2359	rBV3	788	557	0.07%	0.009%
58	8.793	2399	2411	2436	rBV	391708	669777	79.97%	10.268%
59	9.024	2480	2483	2484	rBV3	809	445	0.05%	0.007%
60	9.426	2606	2608	2610	rBV2	977	537	0.06%	0.008%
61	9.596	2658	2661	2669	rBV8	1156	1270	0.15%	0.019%
62	9.899	2751	2755	2757	rBV5	1239	994	0.12%	0.015%
63	9.969	2774	2777	2781	rBV5	1096	1035	0.12%	0.016%
64	10.111	2817	2821	2824	rVB4	1042	929	0.11%	0.014%
65	10.159	2824	2836	2854	rBV	270992	426822	50.96%	6.543%
66	10.304	2880	2881	2885	rBV3	813	666	0.08%	0.010%
67	10.616	2972	2978	2980	rBV7	1636	1502	0.18%	0.023%
68	10.686	2998	3000	3003	rBV4	634	476	0.06%	0.007%
69	10.702	3003	3005	3007	rVV3	1213	659	0.08%	0.010%
70	10.728	3011	3013	3020	rVB7	1191	924	0.11%	0.014%
71	10.966	3086	3087	3093	rBV6	1035	785	0.09%	0.012%
72	11.005	3095	3099	3100	rBV5	754	509	0.06%	0.008%
73	11.075	3117	3121	3123	rVB4	1330	854	0.10%	0.013%
74	11.101	3126	3129	3130	rBV4	943	492	0.06%	0.008%
75	11.194	3145	3158	3180	rBV	403074	648730	77.46%	9.945%
76	11.345	3202	3205	3208	rBV5	2055	1375	0.16%	0.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
 Data File : VV030901.D
 Acq On : 27 Apr 2023 12:57
 Operator : SY/MD
 Sample : 02475-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
 Title : VOC Analysis

77	11.403	3221	3223	3225	rBV3	873	481	0.06%	0.007%
78	11.416	3225	3227	3232	rVV3	808	481	0.06%	0.007%
79	11.567	3262	3274	3291	rBV	383723	619251	73.94%	9.493%
80	11.773	3335	3338	3341	rBV4	1337	676	0.08%	0.010%
81	11.998	3403	3408	3409	rBV5	1568	1128	0.13%	0.017%
82	12.191	3464	3468	3469	rBV2	888	624	0.07%	0.010%
83	12.310	3499	3505	3506	rBV5	2321	2034	0.24%	0.031%
84	12.477	3555	3557	3559	rBV3	1010	531	0.06%	0.008%
85	12.641	3606	3608	3612	rBV5	837	523	0.06%	0.008%
86	12.664	3612	3615	3616	rBV3	868	556	0.07%	0.009%
87	12.693	3621	3624	3627	rBV3	982	698	0.08%	0.011%
88	12.757	3642	3644	3650	rVB5	1090	795	0.09%	0.012%
89	12.783	3650	3652	3654	rBV2	972	583	0.07%	0.009%
90	13.053	3734	3736	3741	rBV4	855	612	0.07%	0.009%
91	13.374	3834	3836	3838	rBV3	954	554	0.07%	0.008%
92	13.413	3846	3848	3851	rBV4	924	511	0.06%	0.008%
93	13.564	3894	3895	3899	rBV3	768	558	0.07%	0.009%
94	13.741	3946	3950	3953	rBV3	862	688	0.08%	0.011%
95	14.024	4034	4038	4041	rBV4	1334	997	0.12%	0.015%
96	14.127	4067	4070	4072	rBV3	1251	975	0.12%	0.015%
97	14.188	4087	4089	4094	rBV5	1033	575	0.07%	0.009%
98	14.477	4177	4179	4184	rBV5	1276	1093	0.13%	0.017%
99	14.580	4210	4211	4213	rVB2	1784	518	0.06%	0.008%
100	15.191	4399	4401	4402	rBV2	1308	474	0.06%	0.007%




Sum of corrected areas: 6523221

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
Data File : VV030901.D
Acq On : 27 Apr 2023 12:57
Operator : SY/MD
Sample : 02475-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

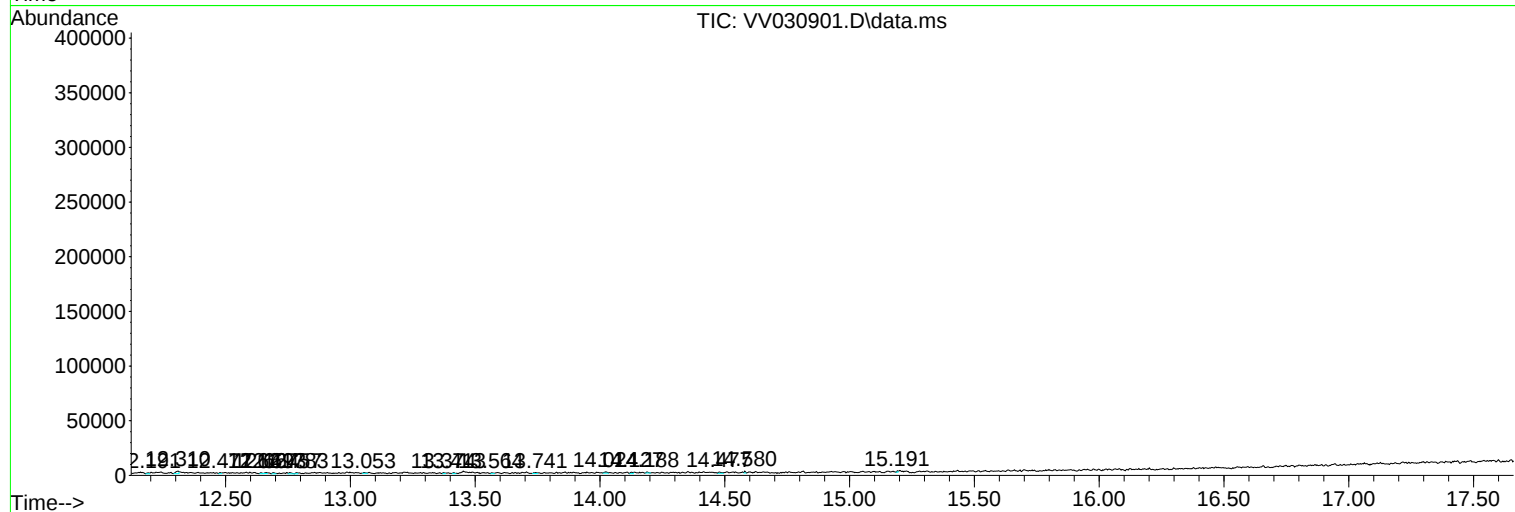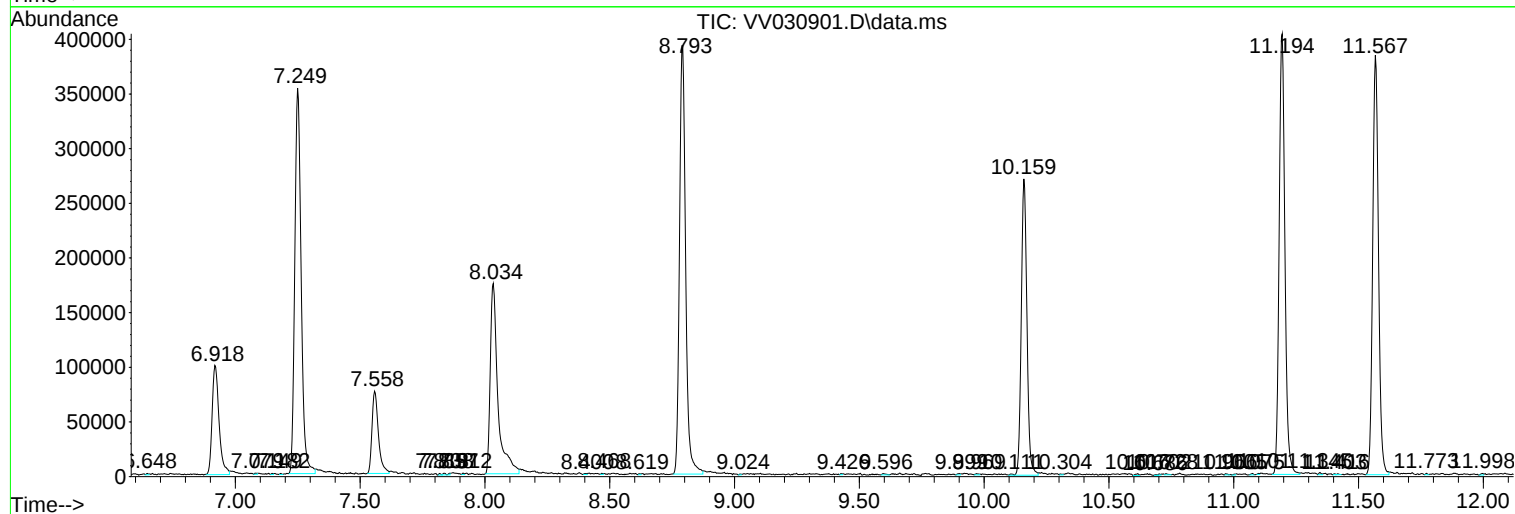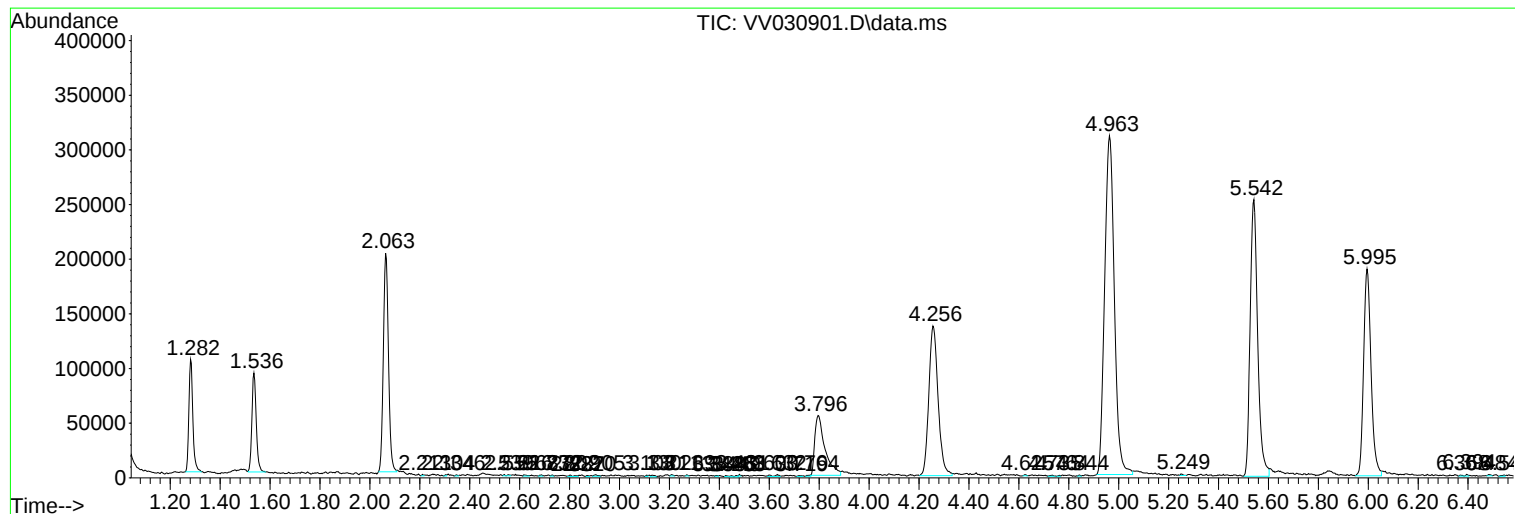

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
Data File : VV030901.D
Acq On : 27 Apr 2023 12:57
Operator : SY/MD
Sample : 02475-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV042723\
Data File : VV030901.D
Acq On : 27 Apr 2023 12:57
Operator : SY/MD
Sample : 02475-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM041723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------